

Data File : VW014249.D
Acq On : 06 Dec 2019 15:04
Operator : SY/VA
Sample : K6171-03
Misc : 5.48G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BS2

Quant Time: Dec 07 04:13:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 04:10:05 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1163979	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	971709	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	332423	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	368817	20.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.68%
7) Chloroethane-d5	2.89	69	341504	26.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.24%
10) 1,1-Dichloroethene-d2	4.02	63	562899	18.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.32%
20) 2-Butanone-d5	7.07	46	129632	28.22	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.44%
24) Chloroform-d	7.64	84	727776	24.56	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.24%
26) 1,2-Dichloroethane-d4	8.11	65	65	0.00	ug/L	-0.19
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.00%#
29) Benzene-d6	8.27	84	1528478	26.84	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.36%
33) 1,2-Dichloropropane-d6	9.27	67	477972	27.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.12%
37) Toluene-d8	10.32	98	1302305	25.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.16%
38) trans-1,3-Dichloropropene-	10.57	79	156135	21.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.96%
39) 2-Hexanone-d5	10.92	63	103097	29.59	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.18%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	300468	21.04	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.16%
61) 1,2-Dichlorobenzene-d4	13.85	152	333731	26.27	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.08%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	13.56	75	39236	3.592 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014249.D
Acq On : 06 Dec 2019 15:04
Operator : SY/VA
Sample : K6171-03
Misc : 5.48G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BS2

Quant Time: Dec 07 04:13:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 04:10:05 2019
Response via : Initial Calibration

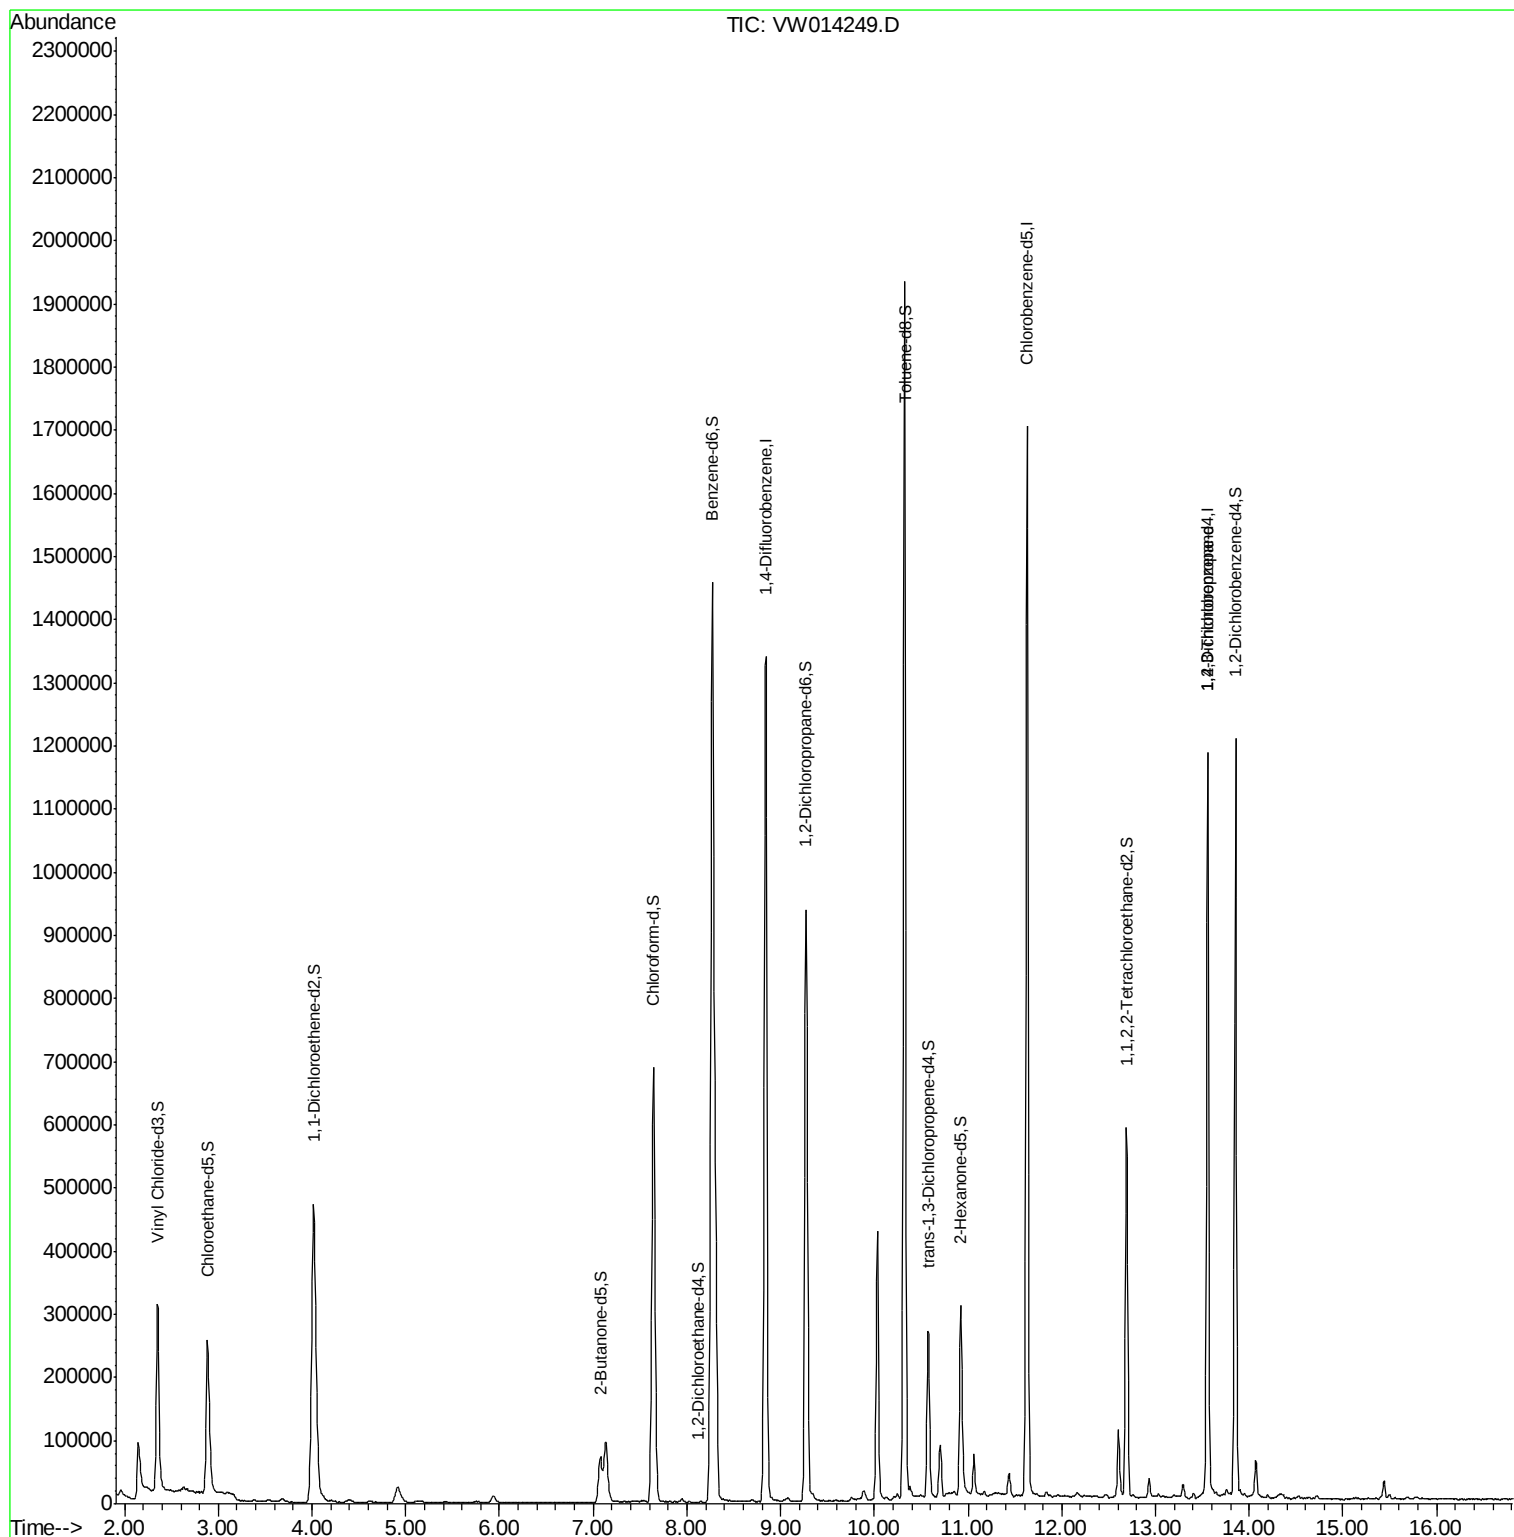

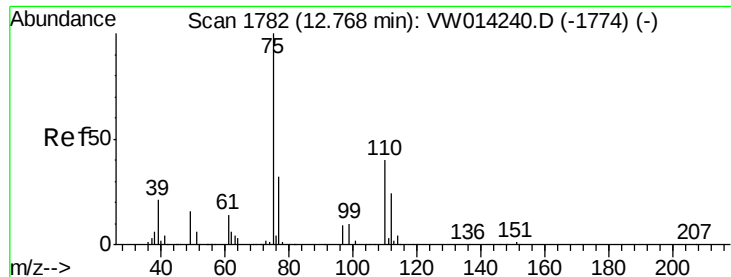

#59

1,2,3-Trichloropropane

Concen: 3.592 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW014249.D

Acq: 06 Dec 2019 15:04

Instrument :

MSVOA_W

ClientSampleId :

C0BS2

Tgt Ion: 75 Resp: 39236

Ion Ratio Lower Upper

75 100

77 34.3 25.9 38.9

