

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW120619\
Quantitation Report (Qedit)




Data File : VW014255.D
Acq On : 06 Dec 2019 17:43
Operator : SY/VA
Sample : K6172-06
Misc : 4.26G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BT2

Manual Integrations
APPROVED

apatel
12/9/2019 2:04:50 PM

Quant Time: Dec 07 04:14:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 04:10:05 2019
Response via : Initial Calibration

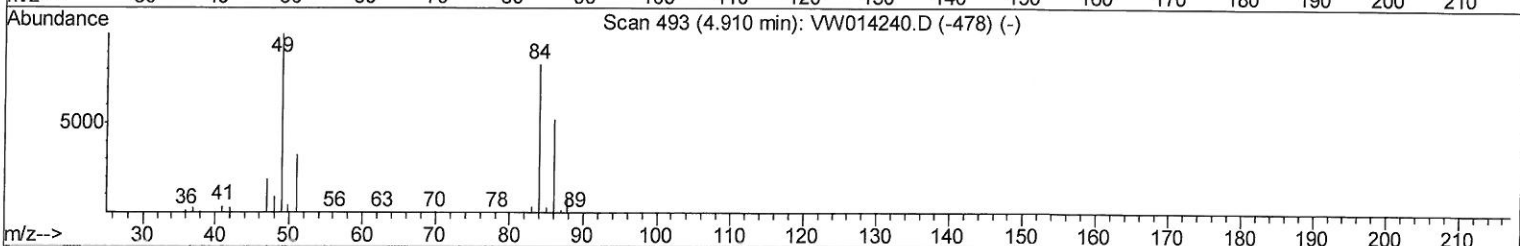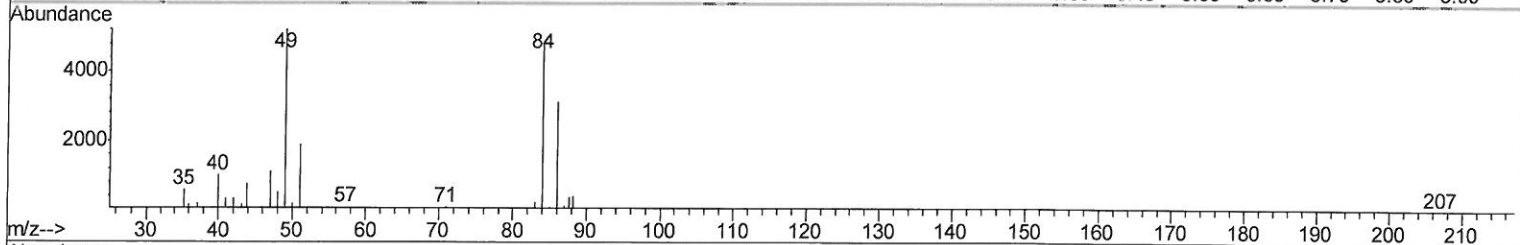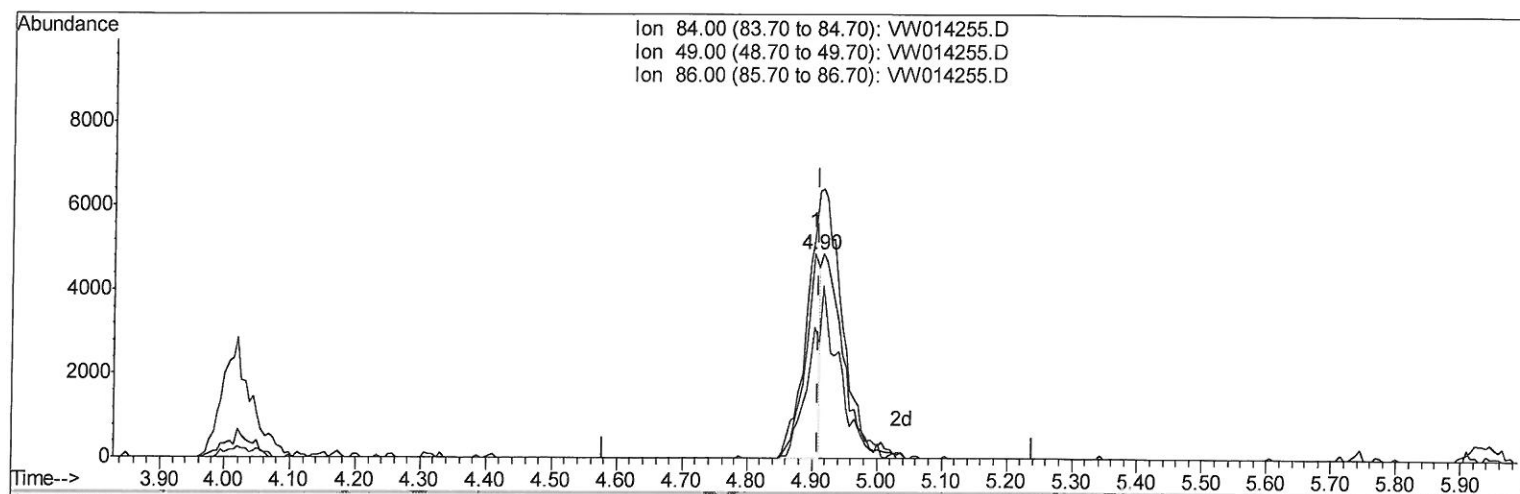

TIC: VW014255.D

(16) Methylene chloride (T)

4.903min (-0.006) 0.70ug/L

response 7490

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	107.30
86.00	62.40	64.12
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW120619\
Quantitation Report (Qedit)




Data File : VW014255.D
Acq On : 06 Dec 2019 17:43
Operator : SY/VA
Sample : K6172-06
Misc : 4.26G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BT2

Manual Integrations
APPROVED

apatel
12/9/2019 2:04:50 PM

Quant Time: Dec 07 04:14:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 04:10:05 2019
Response via : Initial Calibration

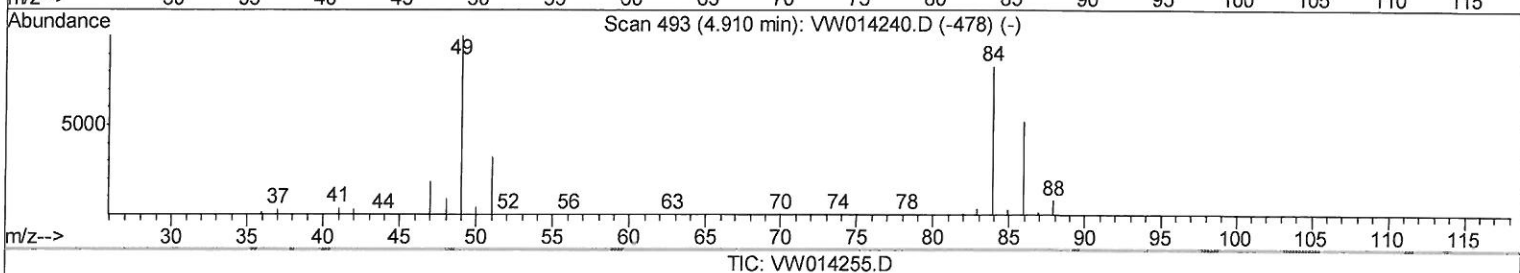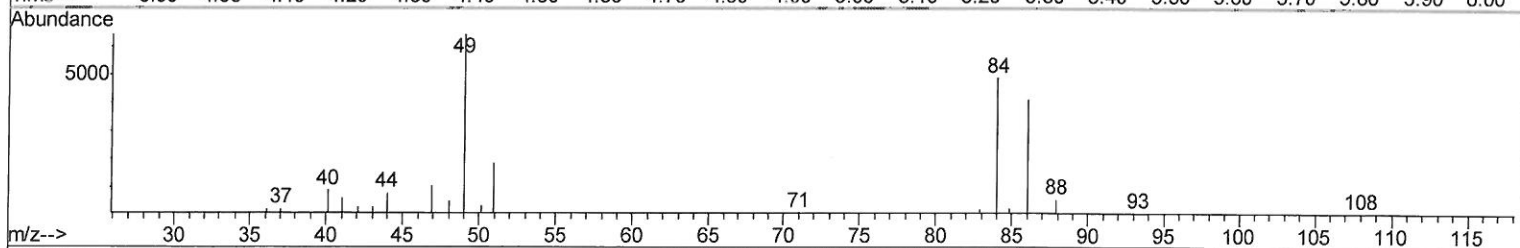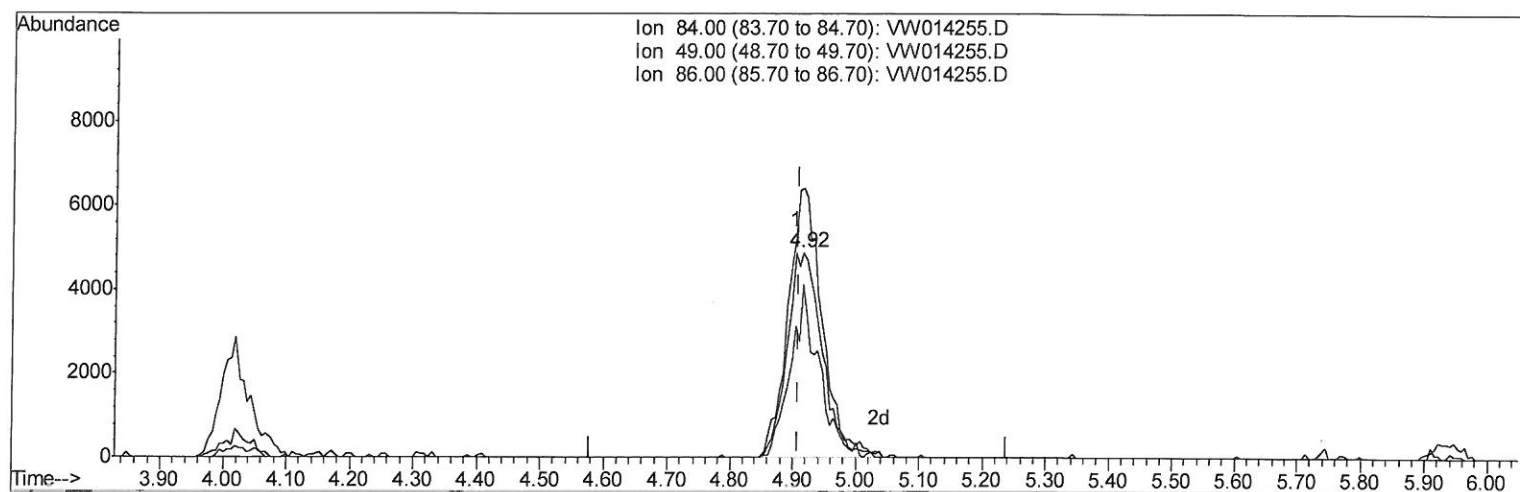

(16) Methylene chloride (T)

4.915min (+0.006) 1.77ug/L m

response 18872

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	131.39
86.00	62.40	84.47#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW120619\
 Quantitation Report (QT Reviewed)

Data File : VW014255.D
 Acq On : 06 Dec 2019 17:43
 Operator : SY/VA
 Sample : K6172-06
 Misc : 4.26G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BT2

Manual Integrations
 APPROVED

apatel
 12/9/2019 2:04:50 PM

Quant Time: Dec 07 05:35:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 04:10:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	693899	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	349822	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	38330	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	302416	28.78	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	115.12%		
7) Chloroethane-d5	2.89	69	244613	31.31	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	125.24%		
10) 1,1-Dichloroethene-d2	4.01	63	354404	19.10	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	76.40%		
20) 2-Butanone-d5	7.07	46	155696	56.86	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	113.72%		
24) Chloroform-d	7.64	84	515103	29.16	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	116.64%		
26) 1,2-Dichloroethane-d4	8.30	65	237392	25.63	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	102.52%		
29) Benzene-d6	8.27	84	1016794	49.59	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	198.36%#		
33) 1,2-Dichloropropane-d6	9.27	67	354033	56.13	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	224.52%#		
37) Toluene-d8	10.32	98	615783	33.22	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	132.88%#		
38) trans-1,3-Dichloropropene-	10.58	79	47227	17.85	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.40%		
39) 2-Hexanone-d5	10.93	63	88214	70.33	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	140.66%#		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	240965	46.88	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	187.52%#		
61) 1,2-Dichlorobenzene-d4	13.85	152	82205	56.12	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	224.48%#		

Target Compounds

					Qvalue
13) Acetone	4.12	43	30128	11.412 ug/L	99
14) Carbon disulfide	4.38	76	6575	0.231 ug/L #	93
16) Methylene chloride	4.92	84	18872m	1.774 ug/L	97
44) Toluene	10.38	91	75022	3.231 ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

12/09/19 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW120619\
Quantitation Report (QT Reviewed)

Data File : VW014255.D
Acq On : 06 Dec 2019 17:43
Operator : SY/VA
Sample : K6172-06
Misc : 4.26G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
C0BT2

Manual Integrations
APPROVED

apatel
12/9/2019 2:04:50 PM

Quant Time: Dec 07 05:35:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 04:10:05 2019
Response via : Initial Calibration

