

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120619\
 Data File : VW014257.D
 Acq On : 06 Dec 2019 18:36
 Operator : SY/VA
 Sample : K6171-12
 Misc : 5.14G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BW1

Quant Time: Dec 07 05:45:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 04:10:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1066370	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	853125	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	251292	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	392564	24.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.24%
7) Chloroethane-d5	2.89	69	299848	24.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.88%
10) 1,1-Dichloroethene-d2	4.02	63	496484	17.41	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.64%
20) 2-Butanone-d5	7.07	46	161905	38.48	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.96%
24) Chloroform-d	7.64	84	666686	24.55	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.20%
26) 1,2-Dichloroethane-d4	8.30	65	337258	23.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.76%
29) Benzene-d6	8.27	84	1375990	27.52	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	110.08%
33) 1,2-Dichloropropane-d6	9.27	67	436311	28.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.44%
37) Toluene-d8	10.32	98	1138784	25.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.76%
38) trans-1,3-Dichloropropene-	10.58	79	134230	20.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.20%
39) 2-Hexanone-d5	10.92	63	121850	39.84	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.68%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	296956	23.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.76%
61) 1,2-Dichlorobenzene-d4	13.85	152	284503	29.63	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	118.52%


Target Compounds					Ovalue
13) Acetone	4.12	43	26927	6.637 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW120619\
Data File : VW014257.D
Acq On : 06 Dec 2019 18:36
Operator : SY/VA
Sample : K6171-12
Misc : 5.14G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BW1

Quant Time: Dec 07 05:45:45 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 04:10:05 2019
Response via : Initial Calibration

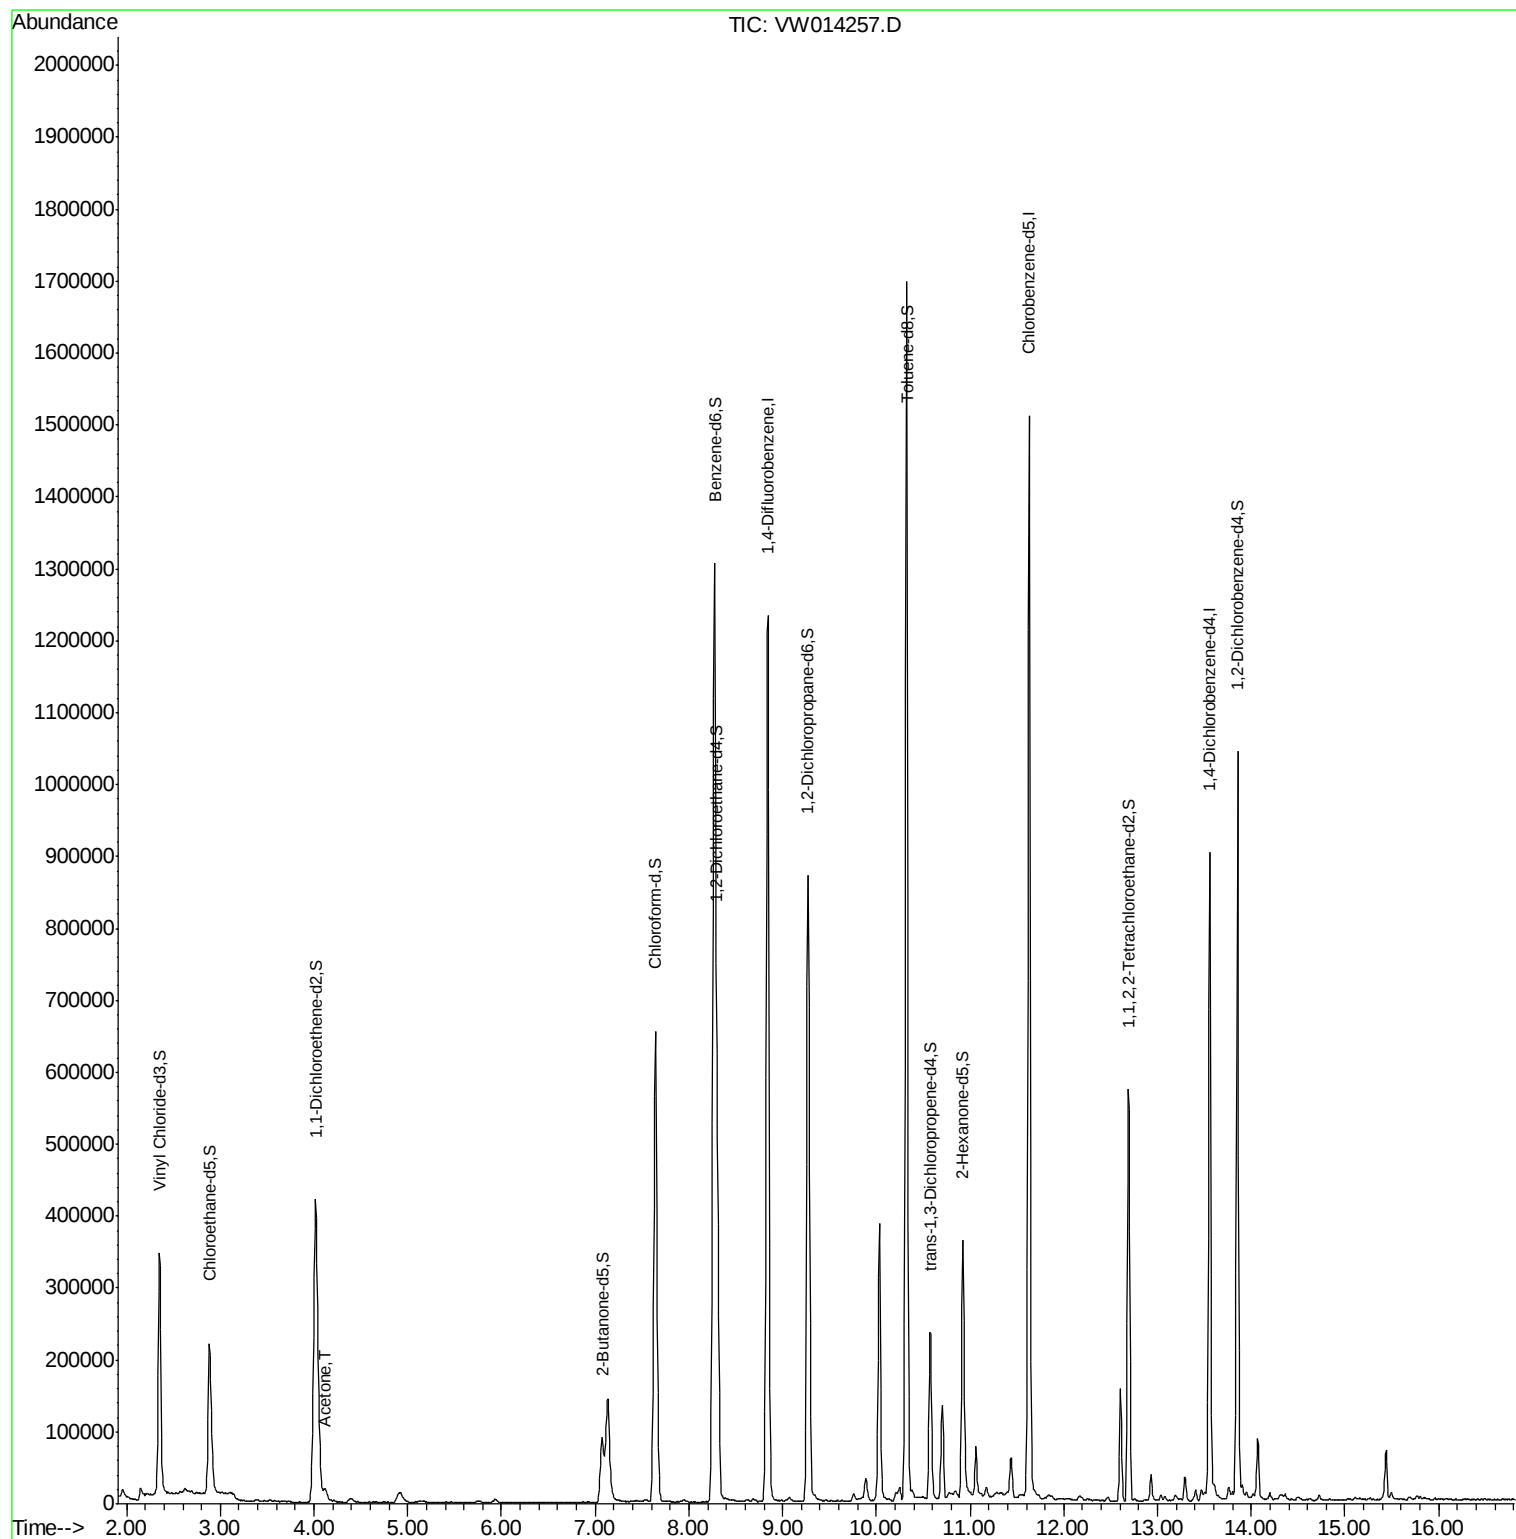

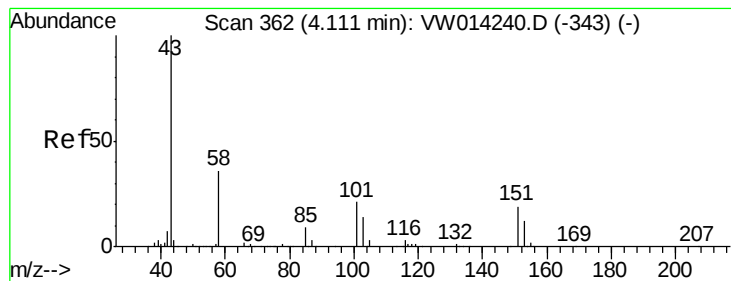

#13
 Acetone
 Concen: 6.637 ug/L
 RT: 4.12 min Scan# 364
 Delta R.T. 0.01 min
 Lab File: VW014257.D
 Acq: 06 Dec 2019 18:36

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BW1

Tot Ion: 43 Resp: 26927
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 65.4

