

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
 Data File : VW031141.D
 Acq On : 06 Dec 2024 11:25
 Operator : SY/MD
 Sample : P5066-14
 Misc : 4.45g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 06 23:37:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 06 23:31:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	342122	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	291553	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	98801	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	109561	20.810	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.240%
7) Chloroethane-d5	2.899	69	77701	19.022	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.080%
11) 1,1-Dichloroethene-d2	4.009	65	55974	23.302	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	93.200%
21) 2-Butanone-d5	7.093	46	30521	33.147	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.300%
24) Chloroform-d	7.642	84	215506	21.507	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.040%
26) 1,2-Dichloroethane-d4	8.307	65	109799	22.268	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.080%
32) Benzene-d6	8.270	84	413442	23.072	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.280%
36) 1,2-Dichloropropane-d6	9.270	67	127300	24.252	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.000%
41) Toluene-d8	10.319	98	370066	22.884	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.520%
43) trans-1,3-Dichloroprop...	10.575	79	44004	20.823	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.280%
47) 2-Hexanone-d5	10.922	63	23680	38.506	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.020%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	73296	20.691	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	80438	22.921	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.680%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3242	0.438	ug/L	Qvalue # 56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031141.D
Acq On : 06 Dec 2024 11:25
Operator : SY/MD
Sample : P5066-14
Misc : 4.45g/10mL/MSVOA_W/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 06 23:37:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

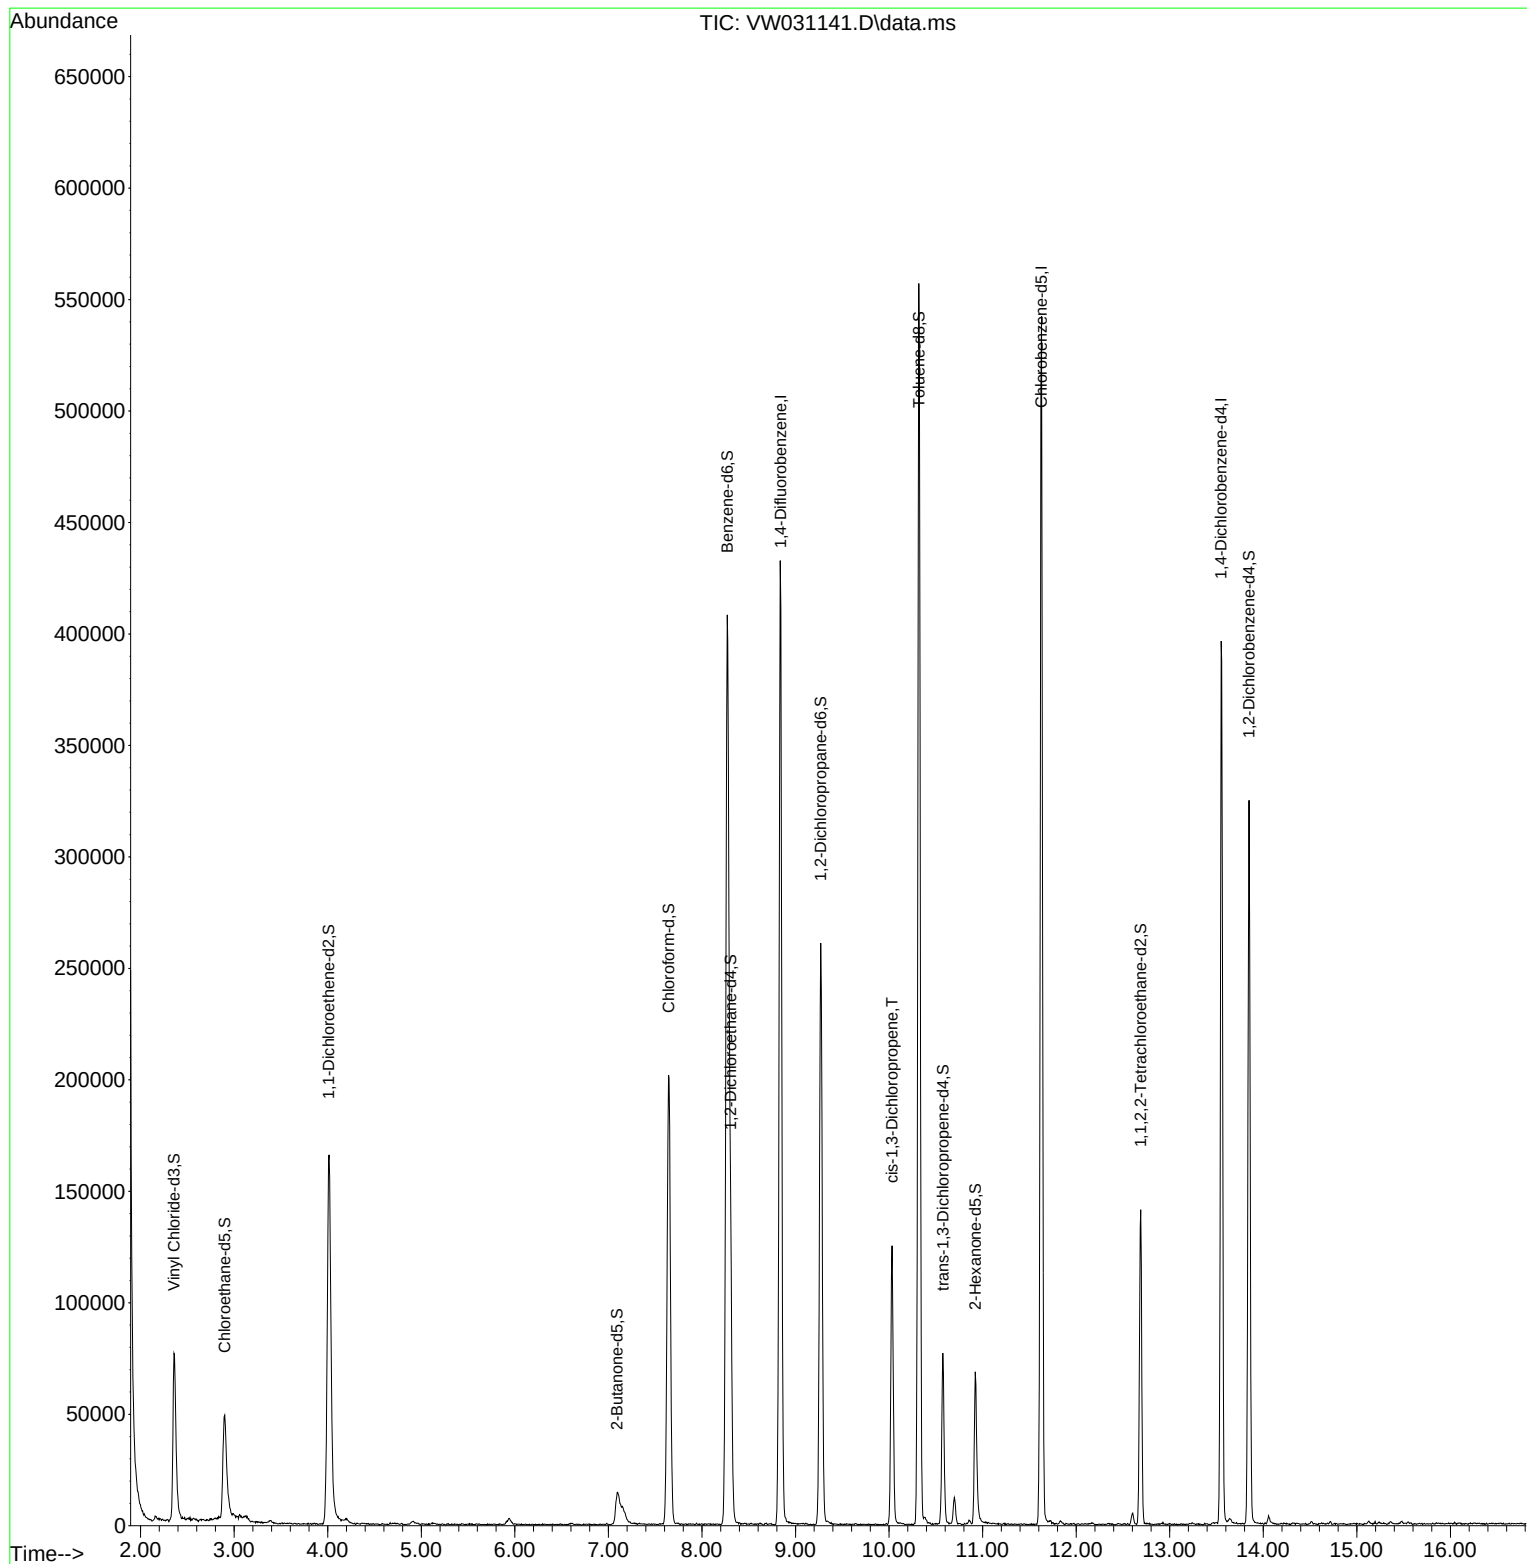

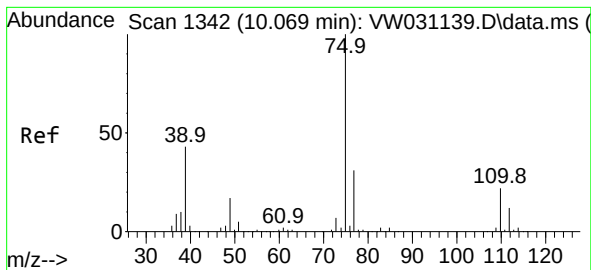

#39
cis-1,3-Dichloropropene
Concen: 0.438 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.037 min
Lab File: VW031141.D
Acq: 06 Dec 2024 11:25

Instrument :
MSVOA_W
ClientSampleId :

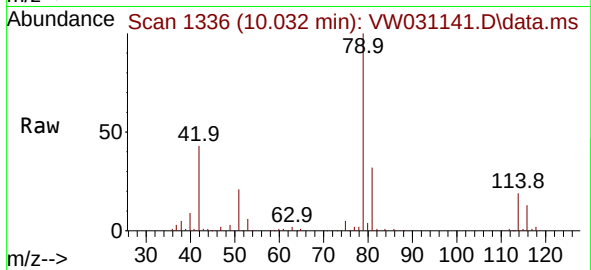

Tgt Ion: 75 Resp: 3242
Ion Ratio Lower Upper
75 100
77 55.2 21.6 40.2#

