

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
 Data File : VW031153.D
 Acq On : 06 Dec 2024 16:12
 Operator : SY/MD
 Sample : P5066-03
 Misc : 3.35g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 06 23:41:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 06 23:31:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	13953	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117	11580	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	3583	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	8309	38.696	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 154.800%#	
7) Chloroethane-d5	2.887	69	6658	39.966	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 159.880%#	
11) 1,1-Dichloroethene-d2	4.021	65	3607	36.819	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 147.280%#	
21) 2-Butanone-d5	7.106	46	1110	29.559	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 59.120%	
24) Chloroform-d	7.642	84	9459	23.146	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 92.600%	
26) 1,2-Dichloroethane-d4	8.307	65	7050	35.059	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 140.240%#	
32) Benzene-d6	8.276	84	19754	27.755	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 111.000%	
36) 1,2-Dichloropropane-d6	9.270	67	6735	32.305	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 129.200%#	
41) Toluene-d8	10.318	98	14667	22.835	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 91.320%	
43) trans-1,3-Dichloroprop...	10.581	79	2570	30.619	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 122.480%	
47) 2-Hexanone-d5	10.922	63	2198	89.988	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 179.980%#	
56) 1,1,2,2-Tetrachloroeth...	12.684	84	3178	22.587	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 90.360%	
66) 1,2-Dichlorobenzene-d4	13.848	152	2878	22.614	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 90.440%	
Target Compounds						
					Qvalue	
8) Chloroethane	2.728	64	122	0.817	ug/L	86
10) 1,1,2-Trichloro-1,2,2-...	4.039	101	138	0.692	ug/L #	19
14) Carbon disulfide	4.393	76	2821	4.341	ug/L	99
15) Methyl Acetate	4.691	43	74	1.043	ug/L #	49
17) trans-1,2-Dichloroethene	5.429	96	312	1.481	ug/L	74
20) cis-1,2-Dichloroethene	7.179	96	128	0.579	ug/L #	25
25) Chloroform	7.679	83	3073	7.626	ug/L #	55
29) Cyclohexane	7.959	56	553	1.897	ug/L #	79
34) Trichloroethene	9.093	95	15386	71.230	ug/L	96
35) Methylcyclohexane	9.331	83	3580	10.415	ug/L #	77
37) 1,2-Dichloropropane	9.337	63	110	0.565	ug/L #	85
40) 4-Methyl-2-pentanone	10.215	43	140	1.605	ug/L #	25
42) Toluene	10.386	91	13810	16.741	ug/L	95
45) 1,1,2-Trichloroethane	10.794	97	112	0.837	ug/L #	40
46) Tetrachloroethene	10.861	164	185570	1158.890	ug/L	92
49) Dibromochloromethane	11.074	129	156	1.058	ug/L	87
50) 1,2-Dibromoethane	11.221	107	52	0.416	ug/L #	1
52) Ethylbenzene	11.727	91	14166	15.155	ug/L	88
53) m,p-Xylene	11.830	106	18285	52.559	ug/L	80

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
 Data File : VW031153.D
 Acq On : 06 Dec 2024 16:12
 Operator : SY/MD
 Sample : P5066-03
 Misc : 3.35g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 06 23:41:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 06 23:31:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


54) o-Xylene	12.160	106	10318	31.880	ug/L	94
55) Styrene	12.166	104	909	1.668	ug/L #	1
57) 1,1,2,2-Tetrachloroethane	12.745	83	676	4.661	ug/L #	52
59) Bromoform	12.355	173	163	3.113	ug/L #	38
60) Isopropylbenzene	12.861	105	31386	54.263	ug/L	94
61) 1,2,3-Trichloropropane	12.781	75	191	2.853	ug/L #	1
62) 1,3,5-Trimethylbenzene	12.940	105	26528	58.244	ug/L	94
63) 1,2,4-Trimethylbenzene	13.245	105	99925	223.333	ug/L	96
64) 1,3-Dichlorobenzene	13.489	146	135	0.535	ug/L #	1
65) 1,4-Dichlorobenzene	13.580	146	313	1.228	ug/L #	1
67) 1,2-Dichlorobenzene	13.873	146	272	1.233	ug/L #	1
68) 1,2-Dibromo-3-chloropr...	14.446	75	1091	75.049	ug/L #	22
70) 1,2,4-trichlorobenzene	15.116	180	132	0.982	ug/L #	1
71) Naphthalene	15.360	128	24653	113.863	ug/L	98
72) 1,2,3-Trichlorobenzene	15.549	180	155	1.347	ug/L #	3


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031153.D
Acq On : 06 Dec 2024 16:12
Operator : SY/MD
Sample : P5066-03
Misc : 3.35g/10mL/MSVOA_W/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 06 23:41:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration




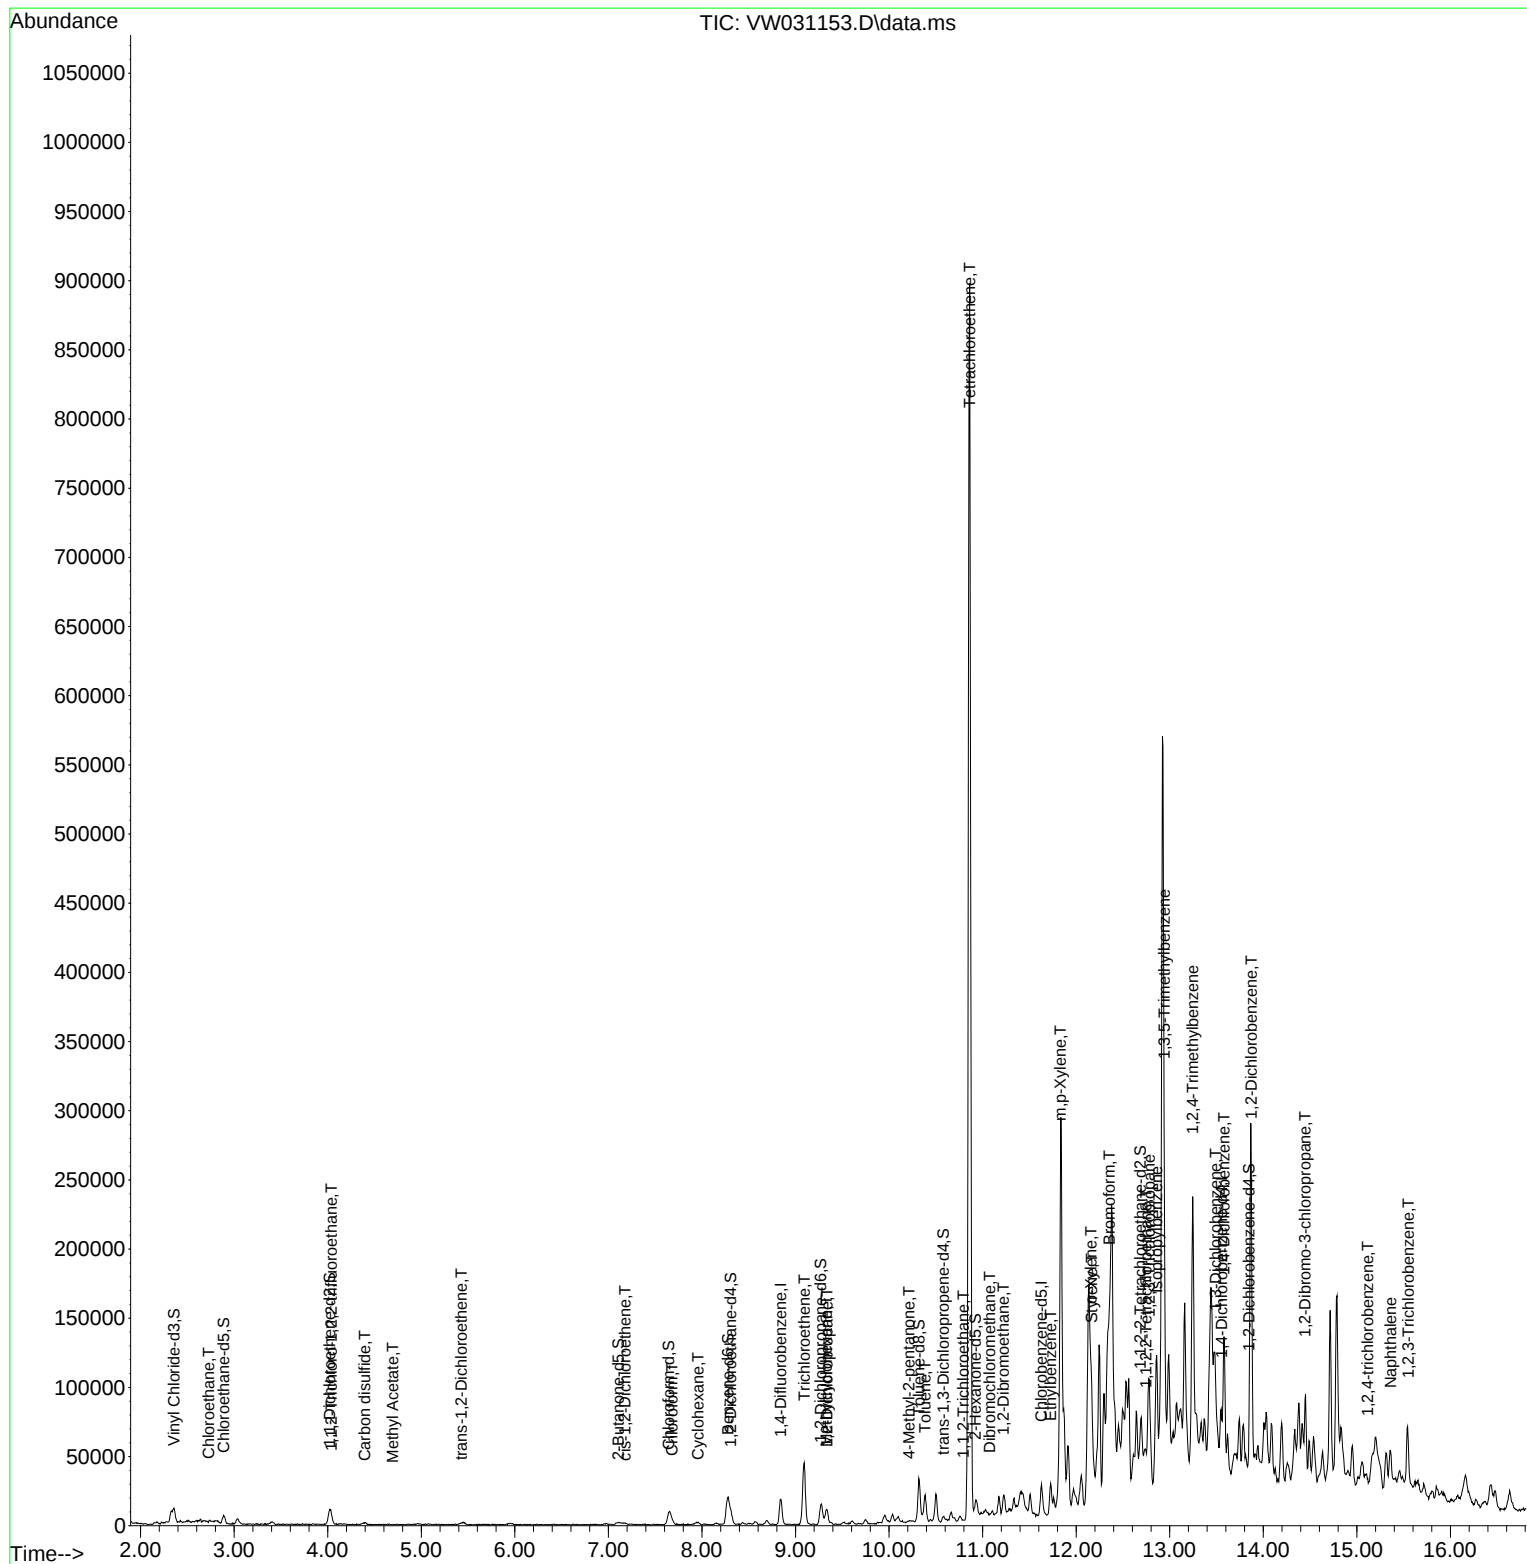




#8
Chloroethane
Concen: 0.817 ug/L
RT: 2.728 min Scan# 11
Delta R.T. -0.201 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 64 Resp: 122
Ion Ratio Lower Upper
64 100
66 41.1 23.2 43.2

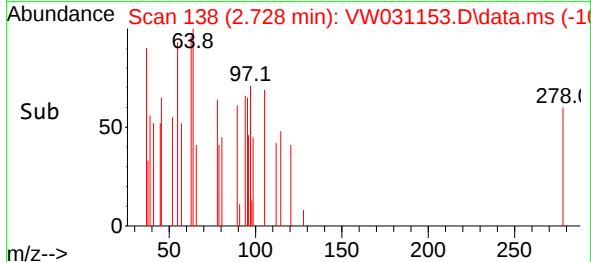

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.692 ug/L
RT: 4.039 min Scan# 353
Delta R.T. -0.037 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12

Tgt Ion: 101 Resp: 138
Ion Ratio Lower Upper
101 100
85 0.0 33.9 50.9#
151 0.0 61.8 92.6#


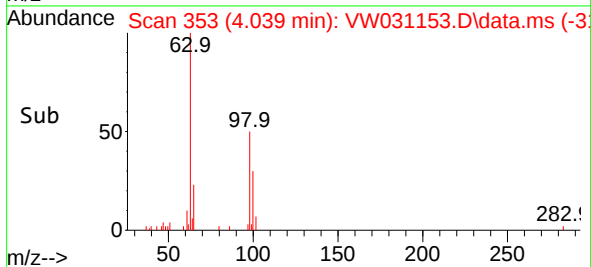

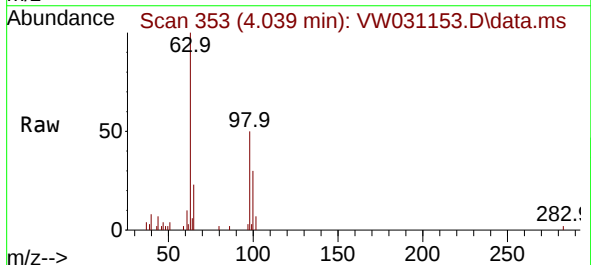


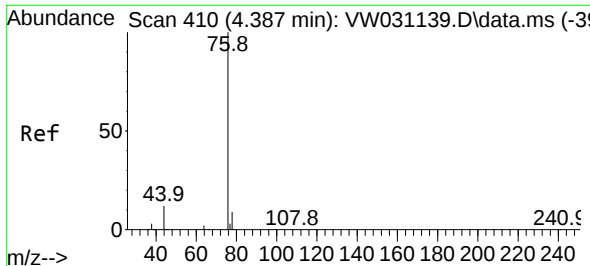

#14
Carbon disulfide
Concen: 4.341 ug/L
RT: 4.393 min Scan# 411
Delta R.T. 0.006 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 76 Resp: 2821
Ion Ratio Lower Upper
76 100
78 9.0 7.4 11.2

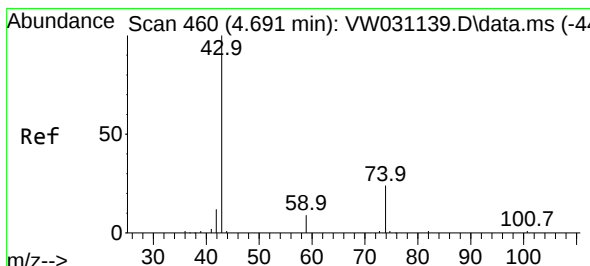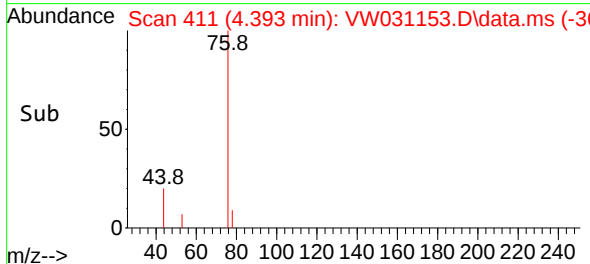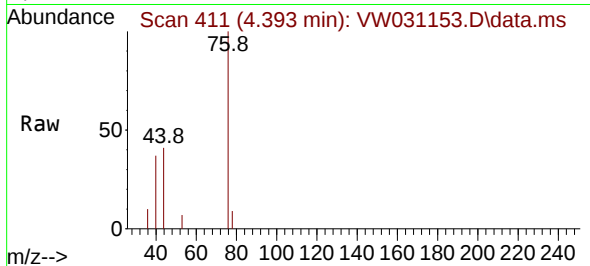

#15
Methyl Acetate
Concen: 1.043 ug/L
RT: 4.691 min Scan# 460
Delta R.T. -0.000 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12

Tgt Ion: 43 Resp: 74
Ion Ratio Lower Upper
43 100
74 0.0 20.8 31.2#

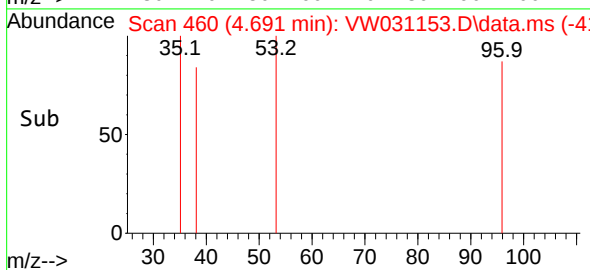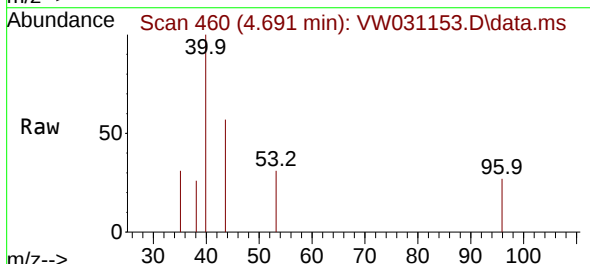



#17

trans-1,2-Dichloroethene

Concen: 1.481 ug/L

RT: 5.429 min Scan# 580

Delta R.T. 0.006 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion: 96 Resp: 312

Ion Ratio Lower Upper

96 100

61 97.9 92.7 172.3

98 49.7 44.4 82.4

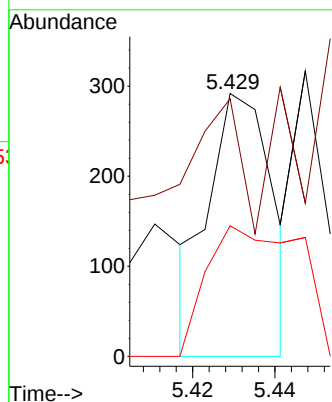

#20

cis-1,2-Dichloroethene

Concen: 0.579 ug/L

RT: 7.179 min Scan# 868

Delta R.T. 0.012 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12




Tgt Ion: 96 Resp: 128


Ion Ratio Lower Upper

96 100

61 245.7 83.7 155.5#

98 62.9 43.9 81.5




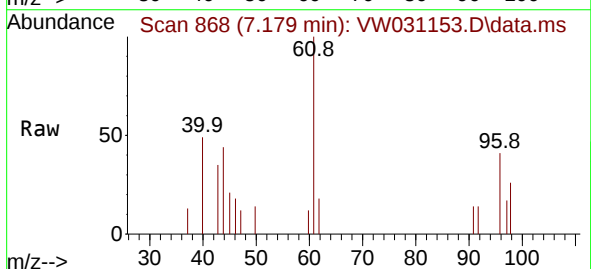




#25
Chloroform
Concen: 7.626 ug/L
RT: 7.679 min Scan# 949
Delta R.T. 0.006 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 83 Resp: 3073
Ion Ratio Lower Upper
83 100
85 30.7 46.5 86.3#

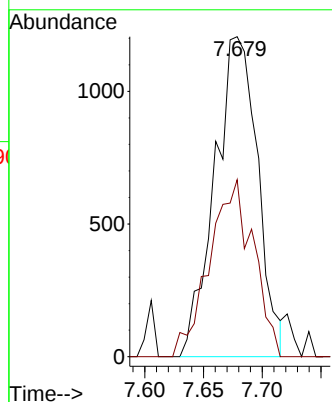

#29
Cyclohexane
Concen: 1.897 ug/L
RT: 7.959 min Scan# 996
Delta R.T. 0.006 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12

Tgt Ion: 56 Resp: 553
Ion Ratio Lower Upper
56 100
69 17.0 25.4 38.2#
84 71.2 71.1 106.7



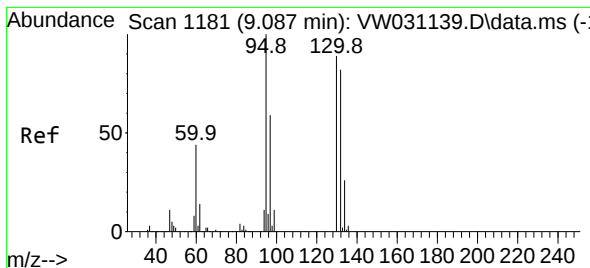

#34

Trichloroethene

Concen: 71.230 ug/L

RT: 9.093 min Scan# 1181

Delta R.T. 0.006 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion: 95 Resp: 15386





Ion Ratio Lower Upper

95 100

97 70.9 48.0 89.2

132 98.8 67.4 125.2

130 93.4 69.5 129.1

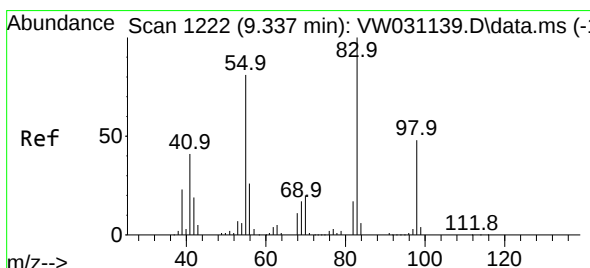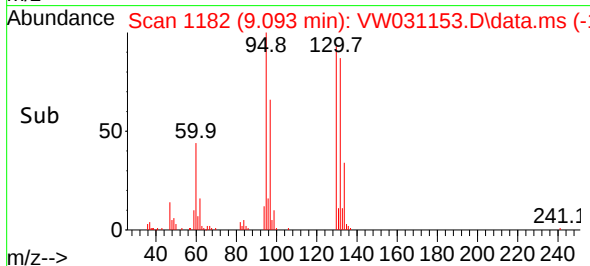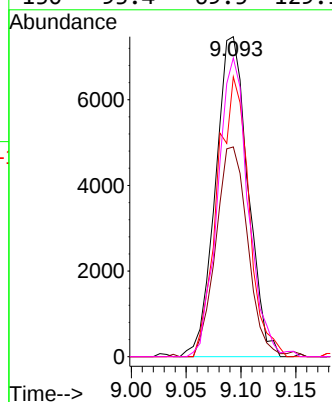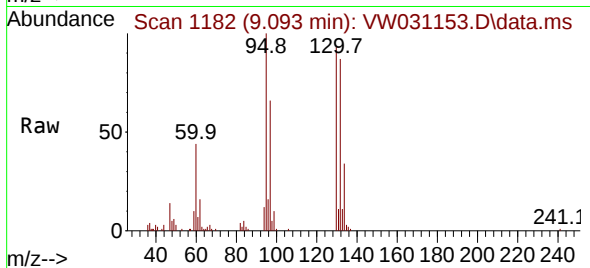

#35

Methylcyclohexane

Concen: 10.415 ug/L

RT: 9.331 min Scan# 1221

Delta R.T. -0.006 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12




Tgt Ion: 83 Resp: 3580


Ion Ratio Lower Upper

83 100

55 103.9 59.5 89.3#

98 44.8 38.7 58.1


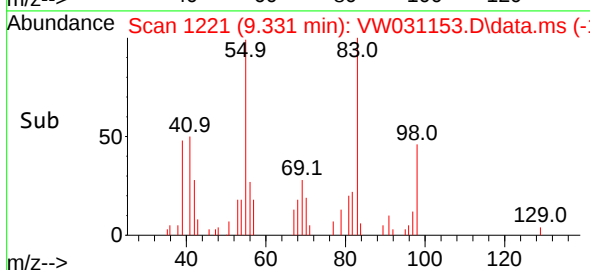

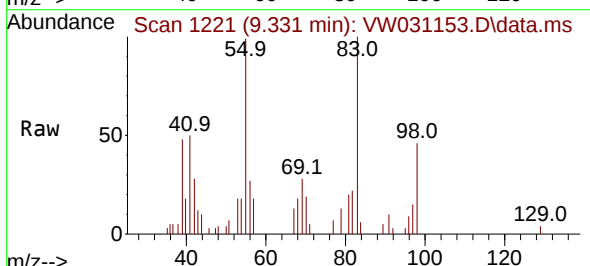




#37
1,2-Dichloropropane
Concen: 0.565 ug/L
RT: 9.337 min Scan# 11
Delta R.T. -0.031 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 63 Resp: 110
Ion Ratio Lower Upper
63 100
112 0.0 3.9 5.9#



#40
4-Methyl-2-pentanone
Concen: 1.605 ug/L
RT: 10.215 min Scan# 1366
Delta R.T. 0.006 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12

Tgt Ion: 43 Resp: 140
Ion Ratio Lower Upper
43 100
58 98.6 33.7 50.5#
100 0.0 14.2 21.2#


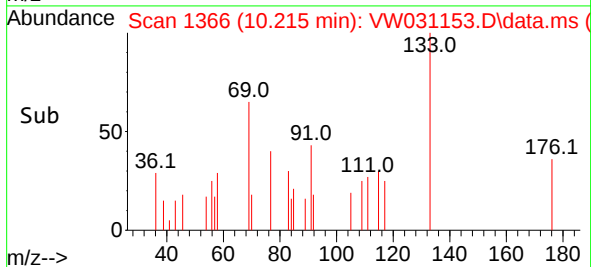

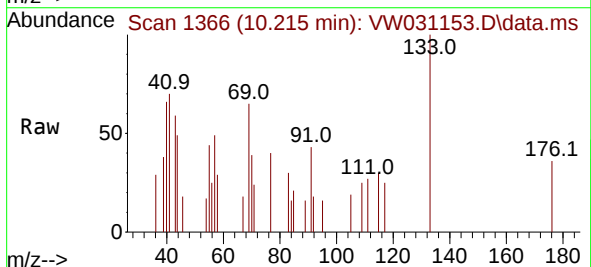




#42
Toluene
Concen: 16.741 ug/L
RT: 10.386 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 91 Resp: 13810
Ion Ratio Lower Upper
91 100
92 54.5 40.8 75.8

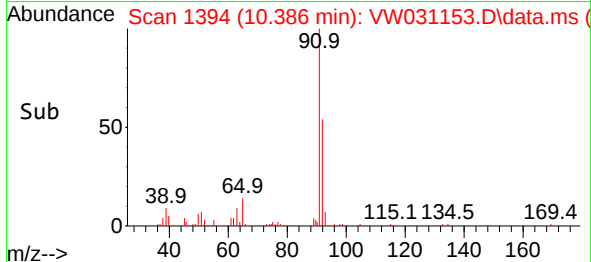

#45
1,1,2-Trichloroethane
Concen: 0.837 ug/L
RT: 10.794 min Scan# 1461
Delta R.T. 0.012 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12

Tgt Ion: 97 Resp: 112
Ion Ratio Lower Upper
97 100
99 0.0 42.4 78.8#
83 115.7 57.8 107.4#
85 0.0 36.6 68.0#

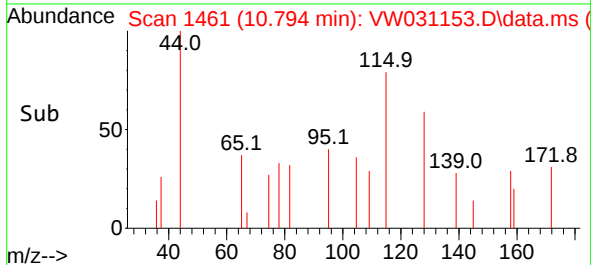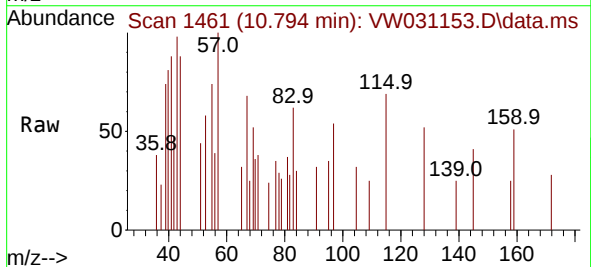



#46

Tetrachloroethene

Concen: 1158.890 ug/L

RT: 10.861 min Scan# 1472

Delta R.T. -0.000 min


Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Instrument :

MSVOA_W

ClientSampleId :



Tgt Ion:164 Resp: 185570




Ion Ratio Lower Upper

164 100

129 103.5 61.9 114.9

131 99.8 67.9 126.1

166 116.3 85.8 159.3

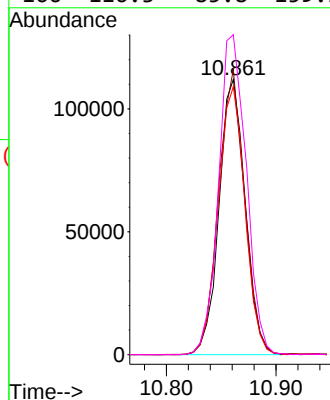

#49

Dibromochloromethane

Concen: 1.058 ug/L

RT: 11.074 min Scan# 1507

Delta R.T. -0.049 min

Lab File: VW031153.D




Acq: 06 Dec 2024 16:12


Tgt Ion:129 Resp: 156

Ion Ratio Lower Upper

129 100

127 84.7 51.4 95.4

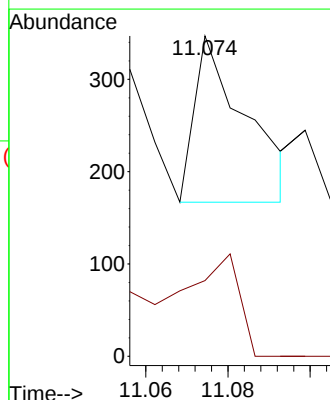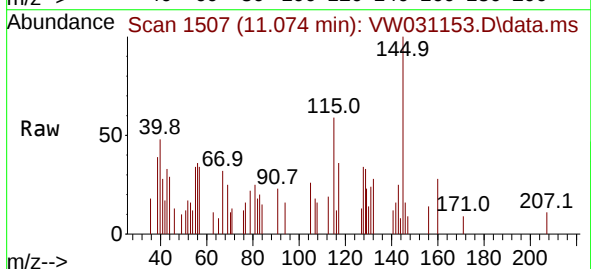



#50

1,2-Dibromoethane

Concen: 0.416 ug/L

RT: 11.221 min Scan# 11

Delta R.T. -0.012 min


Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Instrument :

MSVOA_W

ClientSampleId :






Tgt Ion:107 Resp: 52

Ion Ratio Lower Upper

107 100

109 308.4 71.0 131.9#

188 0.0 3.0 4.4#

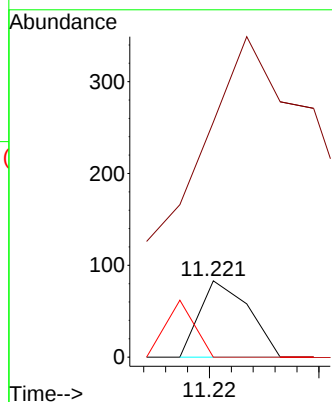

#52

Ethylbenzene

Concen: 15.155 ug/L

RT: 11.727 min Scan# 1614

Delta R.T. -0.000 min

Lab File: VW031153.D




Acq: 06 Dec 2024 16:12


Tgt Ion: 91 Resp: 14166

Ion Ratio Lower Upper

91 100

106 23.8 21.3 39.5

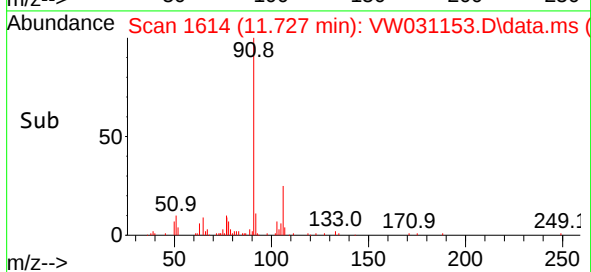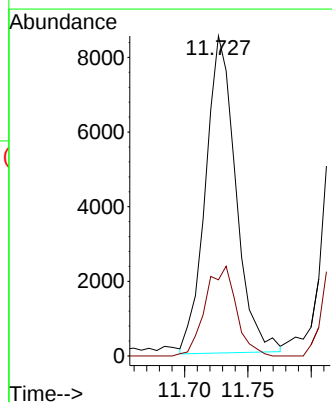



#53

m,p-Xylene

Concen: 52.559 ug/L

RT: 11.830 min Scan# 1

Delta R.T. -0.000 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion:106 Resp: 18285

Ion Ratio Lower Upper

106 100

91 231.8 140.9 261.7

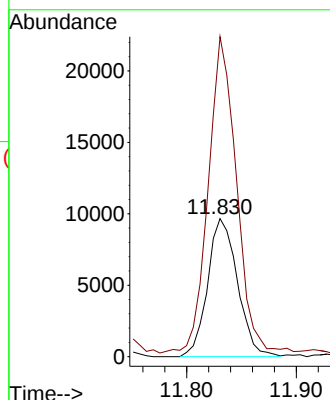

#54

o-Xylene

Concen: 31.880 ug/L

RT: 12.160 min Scan# 1685

Delta R.T. -0.000 min

Lab File: VW031153.D




Acq: 06 Dec 2024 16:12


Tgt Ion:106 Resp: 10318

Ion Ratio Lower Upper

106 100

91 208.1 152.7 283.5

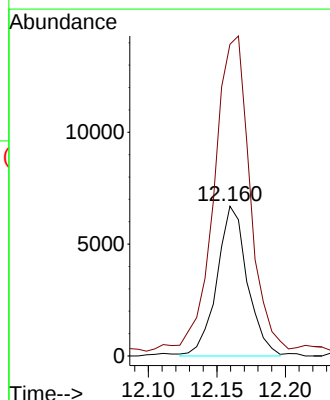



#55

Styrene

Concen: 1.668 ug/L

RT: 12.166 min Scan# 1

Delta R.T. -0.012 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion:104 Resp: 909

Ion Ratio Lower Upper

104 100

78 246.5 30.2 56.0#

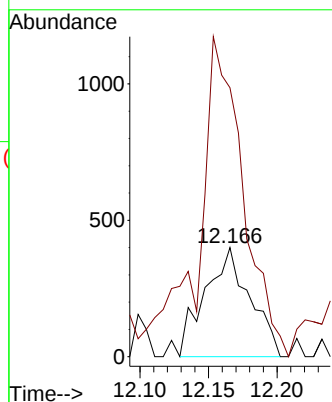

#57

1,1,2,2-Tetrachloroethane

Concen: 4.661 ug/L

RT: 12.745 min Scan# 1781

Delta R.T. 0.030 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12




Tgt Ion: 83 Resp: 676


Ion Ratio Lower Upper

83 100

85 27.4 48.3 89.7#


131 23.3 8.9 13.3#

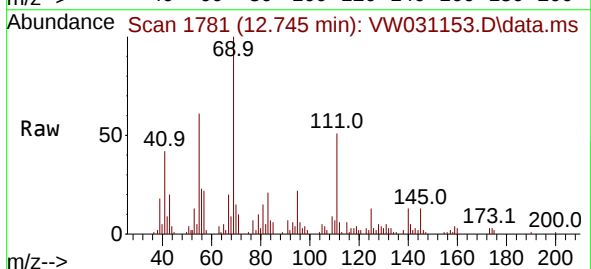






#59
Bromoform
Concen: 3.113 ug/L
RT: 12.355 min Scan# 11
Delta R.T. 0.006 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12

Instrument :
MSVOA_W
ClientSampleId :







Tgt Ion:173 Resp: 163
Ion Ratio Lower Upper
173 100
175 0.0 36.6 54.8#
254 0.0 7.7 11.5#



#60
Isopropylbenzene
Concen: 54.263 ug/L
RT: 12.861 min Scan# 1800
Delta R.T. 0.396 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12

Tgt Ion:105 Resp: 31386
Ion Ratio Lower Upper
105 100
120 31.8 21.5 32.3
77 15.9 12.3 18.5





#61

1,2,3-Trichloropropane

Concen: 2.853 ug/L

RT: 12.781 min Scan# 11

Delta R.T. 0.018 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion: 75 Resp: 191

Ion Ratio Lower Upper

75 100

77 130.4 25.4 38.2#

110 430.9 33.1 49.7#



#62

1,3,5-Trimethylbenzene

Concen: 58.244 ug/L

RT: 12.940 min Scan# 1813

Delta R.T. -0.000 min

Lab File: VW031153.D




Acq: 06 Dec 2024 16:12


Tgt Ion: 105 Resp: 26528

Ion Ratio Lower Upper

105 100

120 46.1 40.5 60.7





#63

1,2,4-Trimethylbenzene

Concen: 223.333 ug/L

RT: 13.245 min Scan# 11

Delta R.T. -0.000 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion:105 Resp: 99925

Ion Ratio Lower Upper

105 100

120 41.4 35.4 53.0

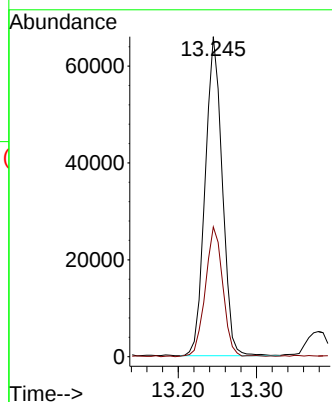

#64

1,3-Dichlorobenzene

Concen: 0.535 ug/L

RT: 13.489 min Scan# 1903

Delta R.T. -0.006 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12




Tgt Ion:146 Resp: 135


Ion Ratio Lower Upper

146 100

111 467.4 28.5 52.9#

148 39.2 44.1 81.9#









#65
1,4-Dichlorobenzene
Concen: 1.228 ug/L
RT: 13.580 min Scan# 1917
Delta R.T. 0.006 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:146 Resp: 313
Ion Ratio Lower Upper
146 100
111 398.5 26.6 49.4#
148 67.2 42.1 78.1

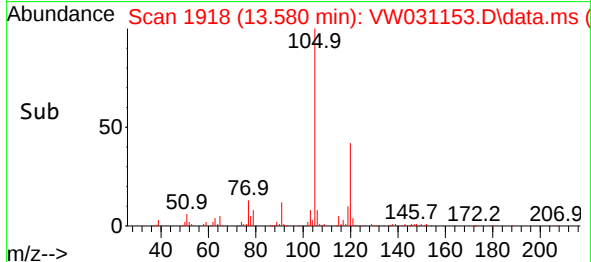

#67
1,2-Dichlorobenzene
Concen: 1.233 ug/L
RT: 13.873 min Scan# 1966
Delta R.T. 0.006 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12

Tgt Ion:146 Resp: 272
Ion Ratio Lower Upper
146 100
111 452.6 30.9 46.3#
148 71.4 50.0 75.0


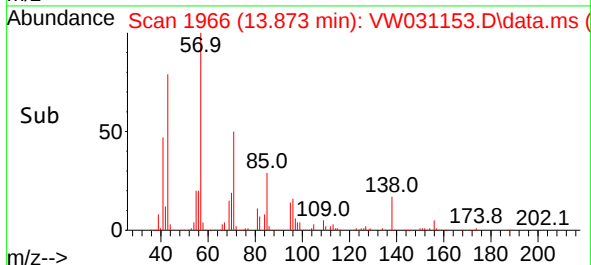
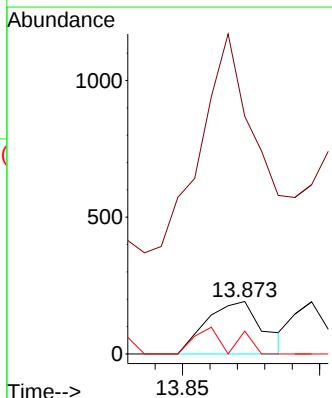
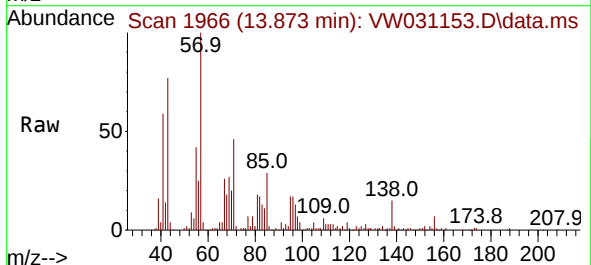




#68
1,2-Dibromo-3-chloropropane
Concen: 75.049 ug/L
RT: 14.446 min Scan# 2065
Delta R.T. -0.031 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 75 Resp: 1091
Ion Ratio Lower Upper
75 100
155 0.0 63.1 94.7#
157 32.4 82.1 123.1#

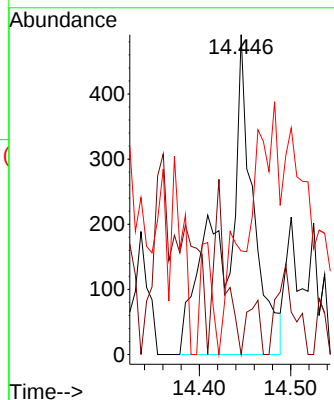

#70
1,2,4-trichlorobenzene
Concen: 0.982 ug/L
RT: 15.116 min Scan# 2170
Delta R.T. -0.006 min
Lab File: VW031153.D
Acq: 06 Dec 2024 16:12

Tgt Ion:180 Resp: 132
Ion Ratio Lower Upper
180 100
182 177.3 76.1 114.1#
145 2140.2 25.7 38.5#

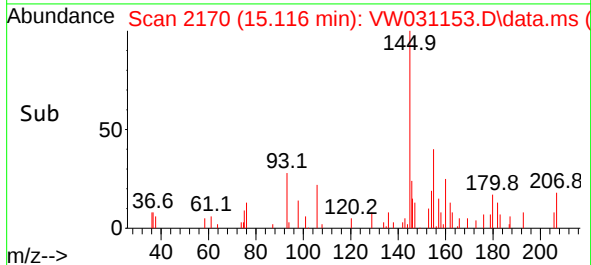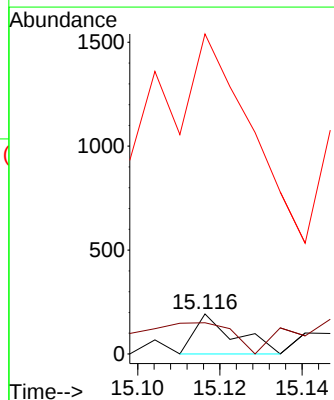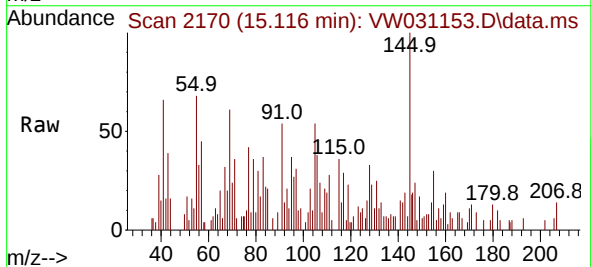



#71

Naphthalene

Concen: 113.863 ug/L

RT: 15.360 min Scan# 21

Delta R.T. -0.000 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion:128 Resp: 24653

Ion Ratio Lower Upper

128 100

127 13.7 10.4 15.6

129 9.9 8.3 12.5

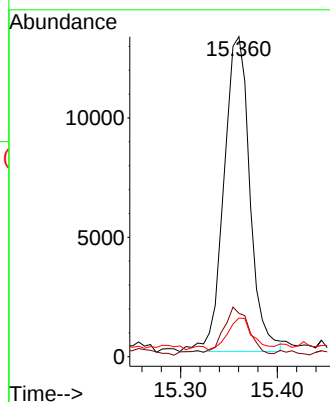

#72

1,2,3-Trichlorobenzene

Concen: 1.347 ug/L

RT: 15.549 min Scan# 2241

Delta R.T. -0.000 min

Lab File: VW031153.D

Acq: 06 Dec 2024 16:12

Tgt Ion:180 Resp: 155

Ion Ratio Lower Upper

180 100

182 207.7 78.7 118.1#

145 0.0 26.3 39.5#

