




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
 Data File : VW031142.D
 Acq On : 06 Dec 2024 11:49
 Operator : SY/MD
 Sample : P5066-08
 Misc : 5.38g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28M7

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:37:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 06 23:31:46 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
 Supervised By :Semsettin Yesilyurt 12/09/2024

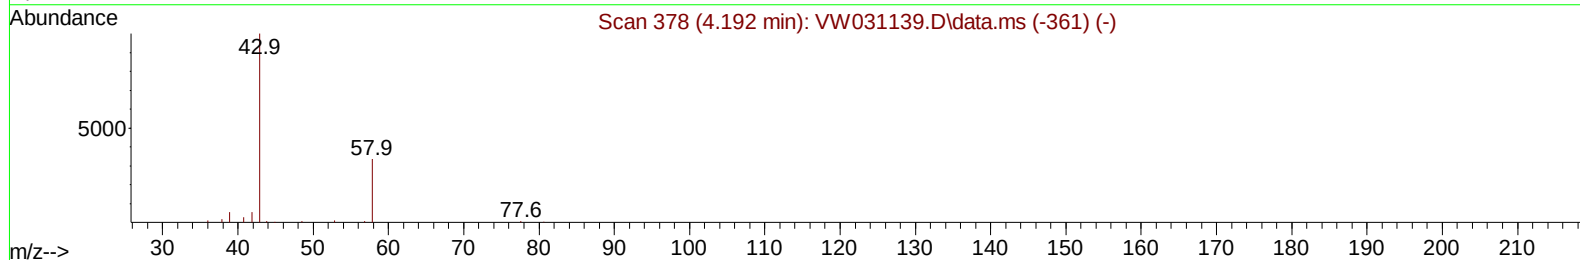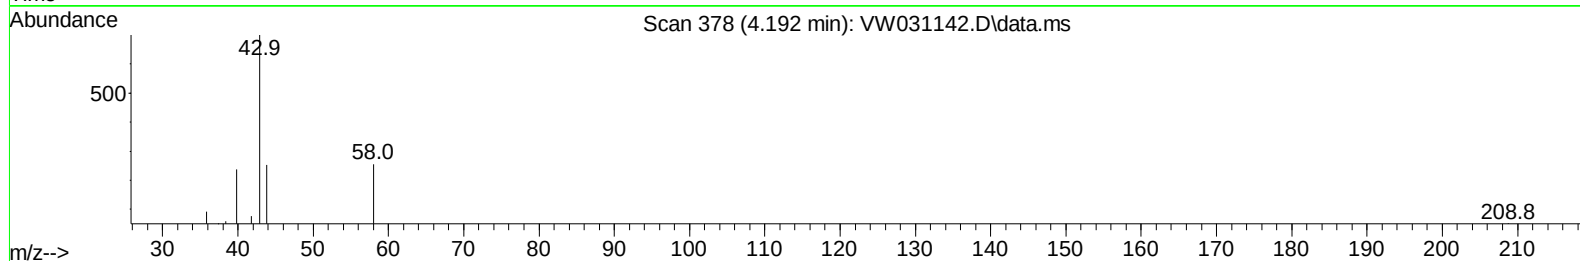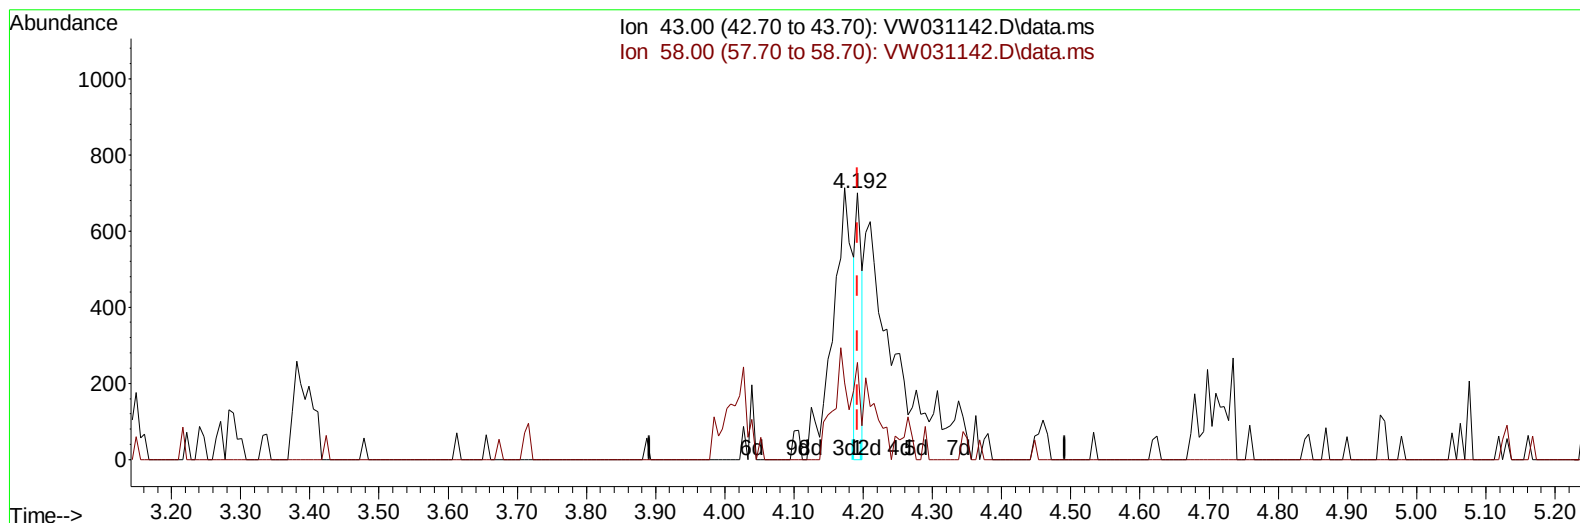

TIC: VW031142.D\data.ms

(13) Acetone (T)

4.192min (+ 0.000) 2.74 ug/L

response 437

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	22.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031142.D
Acq On : 06 Dec 2024 11:49
Operator : SY/MD
Sample : P5066-08
Misc : 5.38g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M7

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:37:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

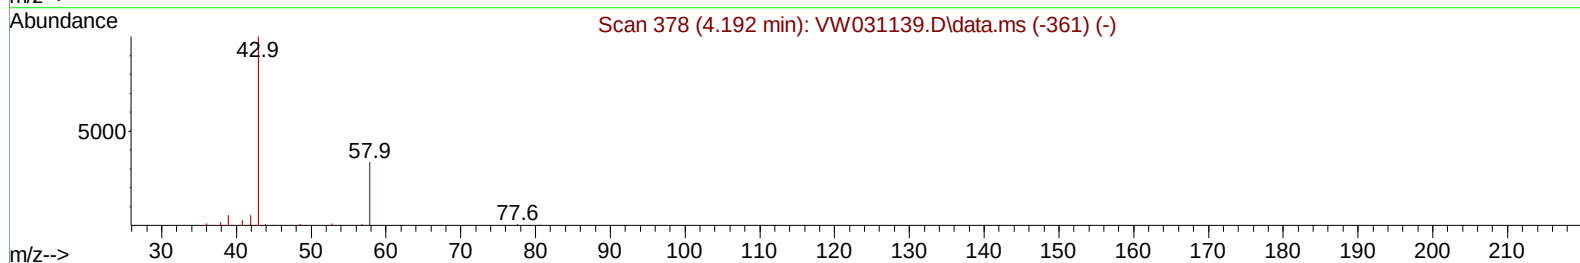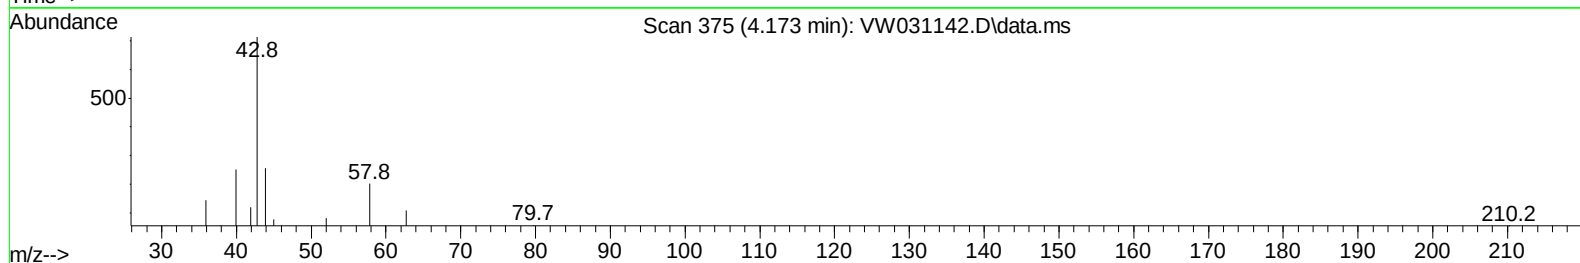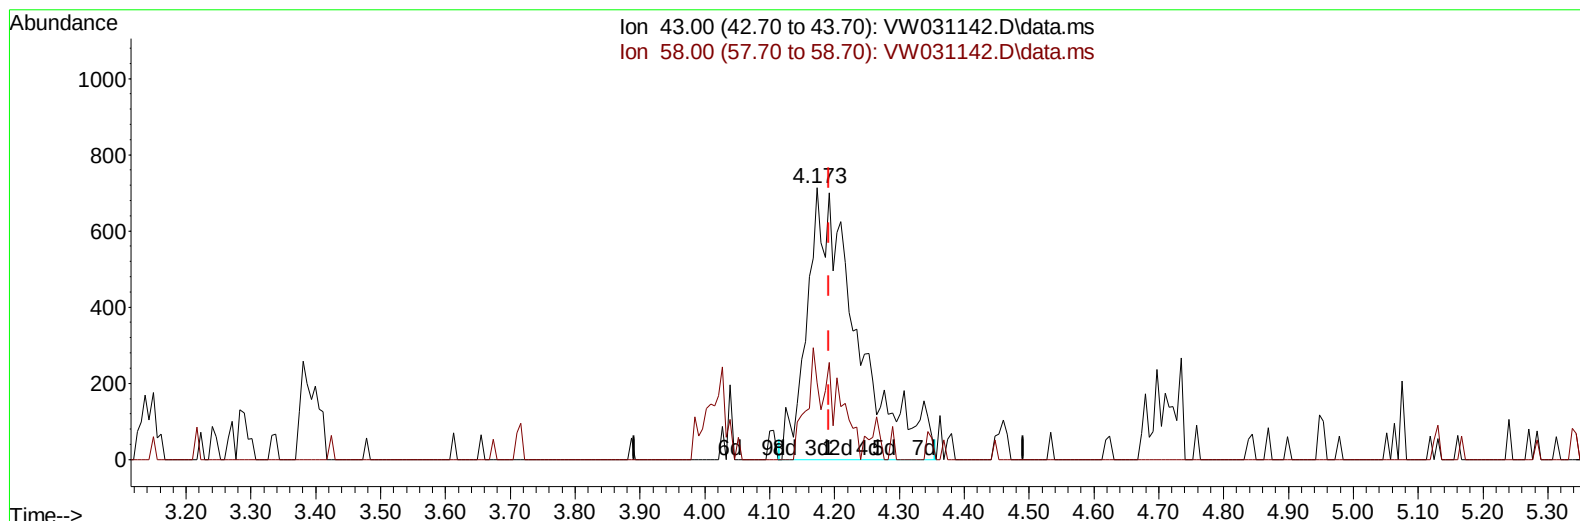

TIC: VW031142.D\data.ms

(13) Acetone (T)

4.173min (-0.018) 24.37 ug/L m

response 3880

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	2.53
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031142.D
Acq On : 06 Dec 2024 11:49
Operator : SY/MD
Sample : P5066-08
Misc : 5.38g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M7

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:37:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

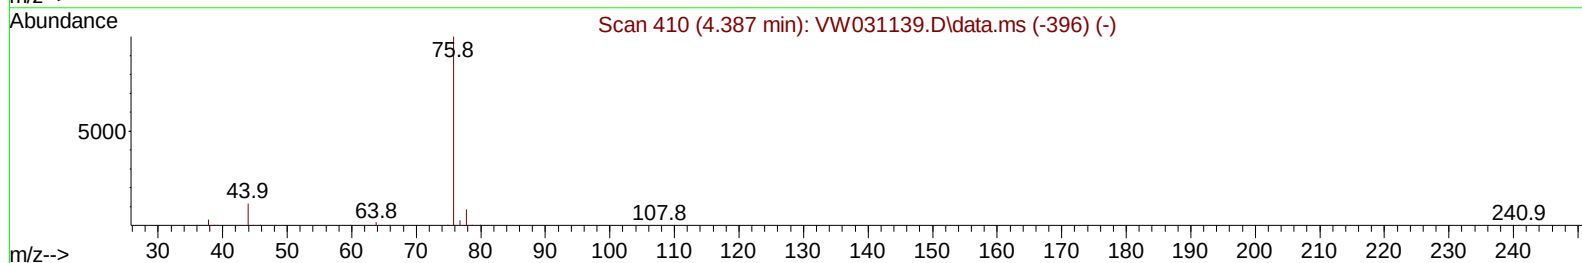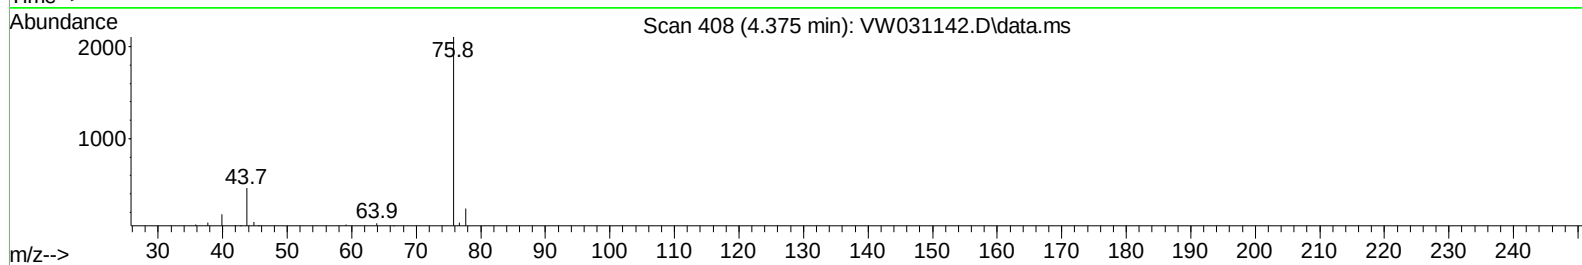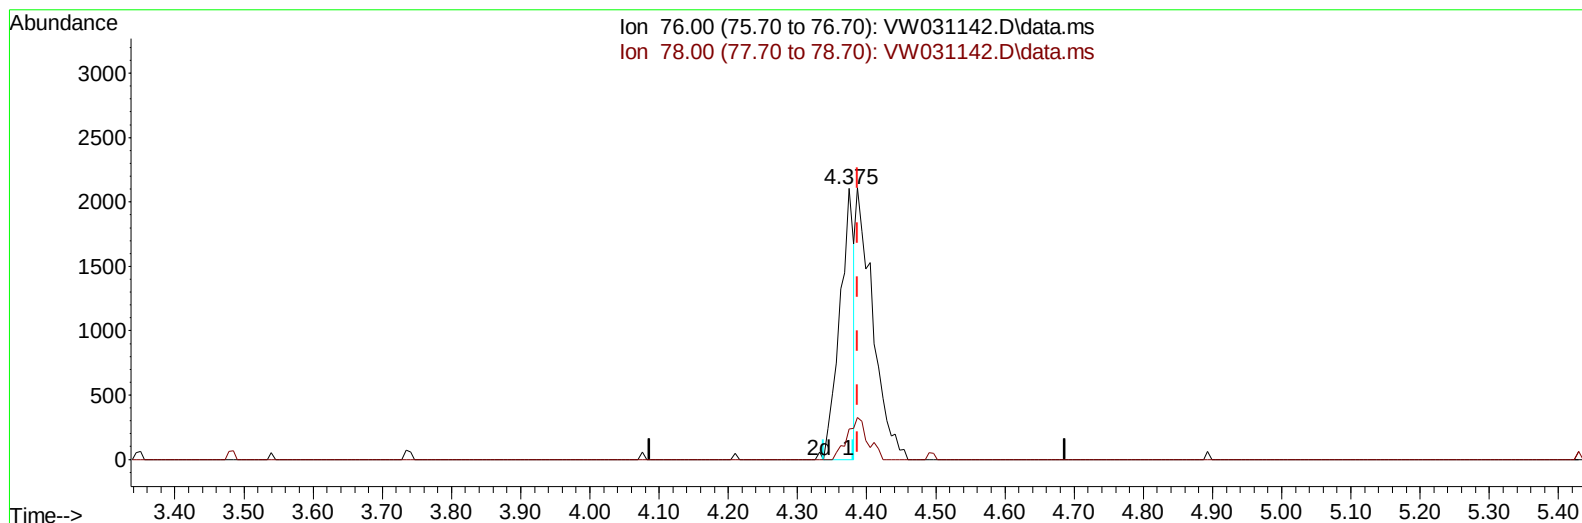

TIC: VW031142.D\data.ms

(14) Carbon disulfide (T)

4.375min (-0.012) 1.92 ug/L

response 2945

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.30	10.91
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031142.D
Acq On : 06 Dec 2024 11:49
Operator : SY/MD
Sample : P5066-08
Misc : 5.38g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M7

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:37:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

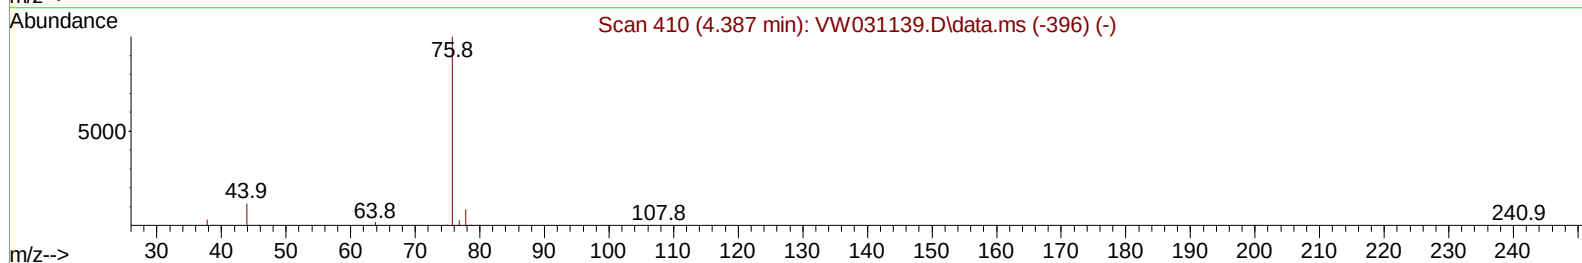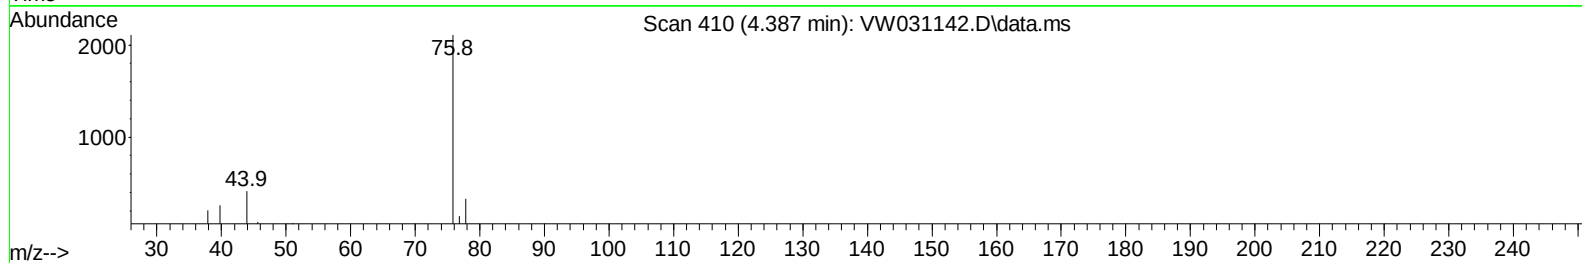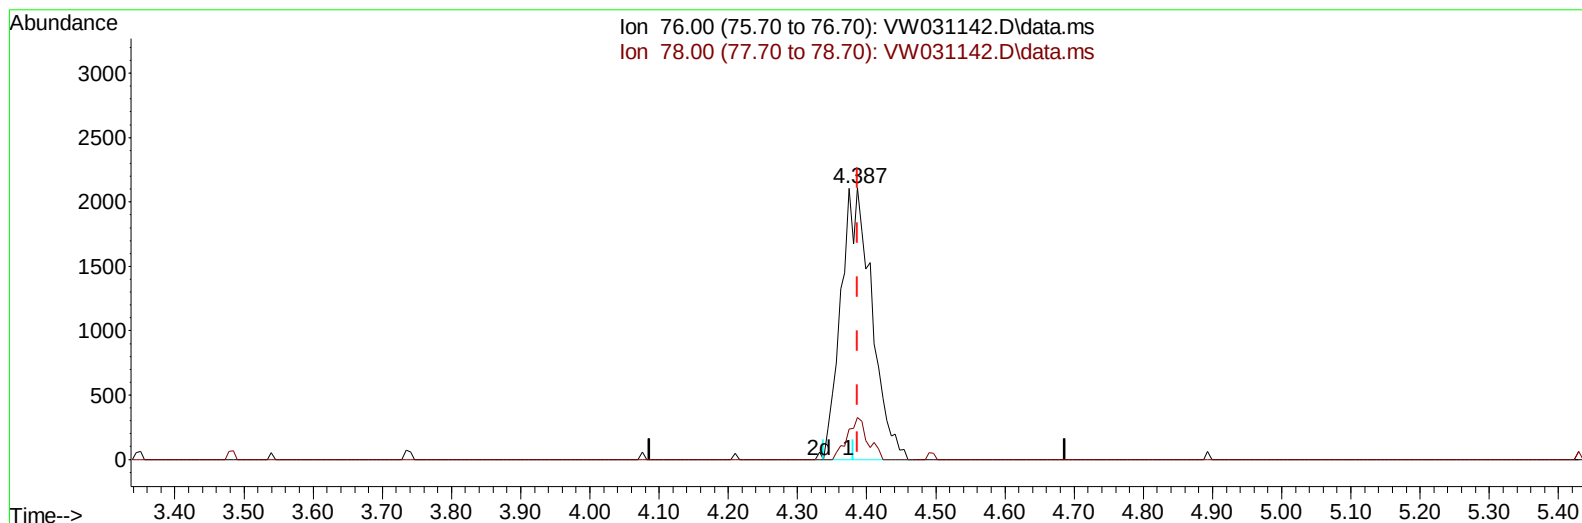

TIC: VW031142.D\data.ms

(14) Carbon disulfide (T)

4.387min (+ 0.000) 4.29 ug/L m

response 6559

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.30	15.55#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw120624\
 Data File : VW031142.D
 Acq On : 06 Dec 2024 11:49
 Operator : SY/MD
 Sample : P5066-08
 Misc : 5.38g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28M7

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:37:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 06 23:31:46 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
 Supervised By :Semsettin Yesilyurt 12/09/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		32862	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		17349	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		2446	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		9917	19.610	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	78.440%		
7) Chloroethane-d5	2.899	69		9164	23.356	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	93.440%		
11) 1,1-Dichloroethene-d2	4.021	65		6343	27.491	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	109.960%		
21) 2-Butanone-d5	7.100	46		30641	346.449	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	692.900%#		
24) Chloroform-d	7.642	84		27663	28.741	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	114.960%		
26) 1,2-Dichloroethane-d4	8.307	65		23402	49.412	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	197.640%#		
32) Benzene-d6	8.276	84		45373	42.552	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	170.200%#		
36) 1,2-Dichloropropane-d6	9.270	67		11165	35.746	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	143.000%#		
41) Toluene-d8	10.319	98		24130	25.076	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	100.320%		
43) trans-1,3-Dichloroprop...	10.581	79		4082	32.461	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	129.840%		
47) 2-Hexanone-d5	10.922	63		5847	159.780	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	319.560%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		9328	44.251	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	177.000%#		
66) 1,2-Dichlorobenzene-d4	13.848	152		2372	27.302	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	109.200%		
Target Compounds							
13) Acetone	4.173	43		3880m	24.367	ug/L	Qvalue
14) Carbon disulfide	4.387	76		6559m	4.285	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031142.D
Acq On : 06 Dec 2024 11:49
Operator : SY/MD
Sample : P5066-08
Misc : 5.38g/10mL/MSVOA_W/SoIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M7

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

Quant Time: Dec 06 23:37:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

