




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031143.D
Acq On : 06 Dec 2024 12:12
Operator : SY/MD
Sample : P5066-09
Misc : 7.23g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M8

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:38:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

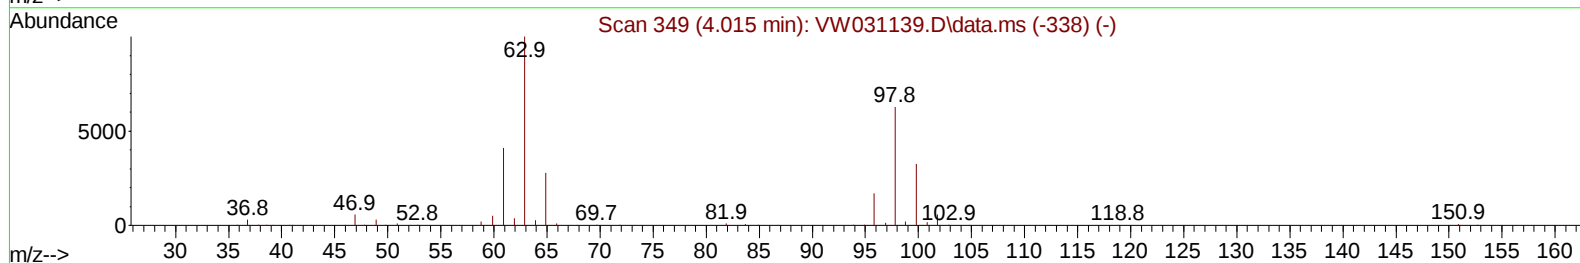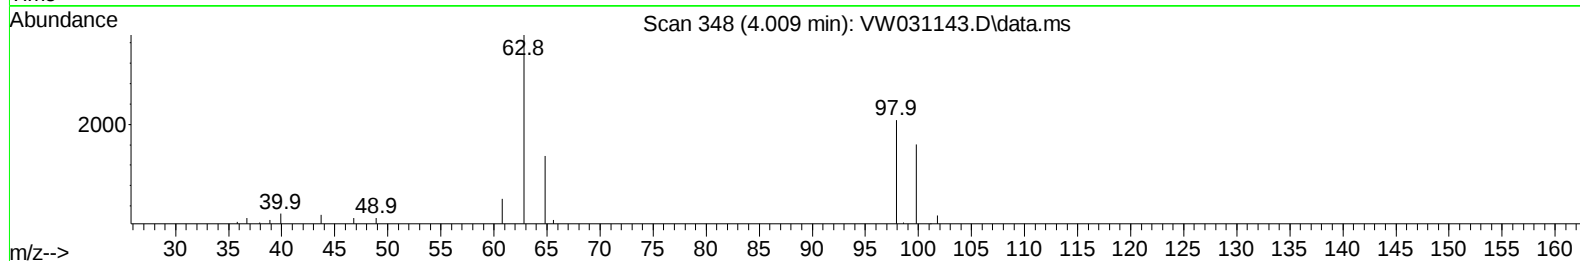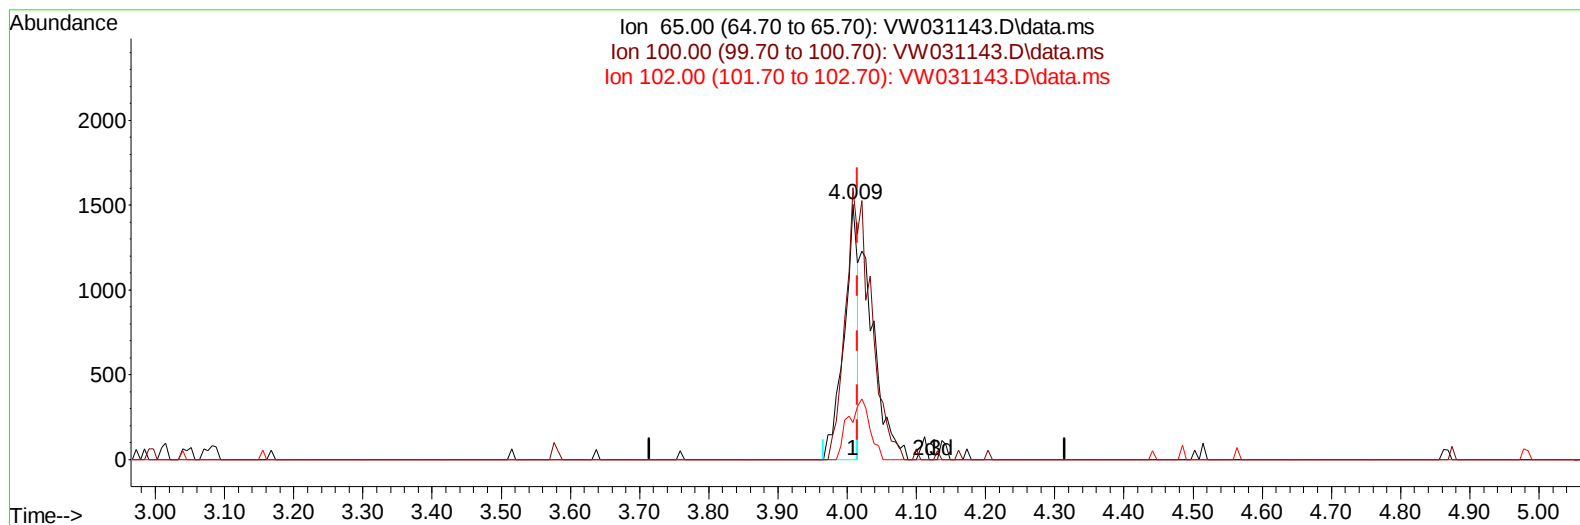

TIC: VW031143.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.009min (-0.006) 11.80 ug/L

response 2074

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	143.20	197.64#
102.00	21.00	13.74#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031143.D
Acq On : 06 Dec 2024 12:12
Operator : SY/MD
Sample : P5066-09
Misc : 7.23g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M8

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:38:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

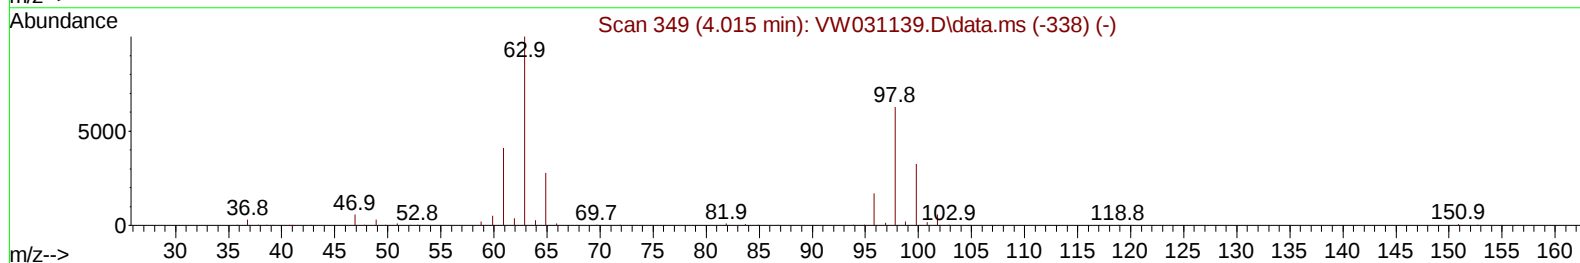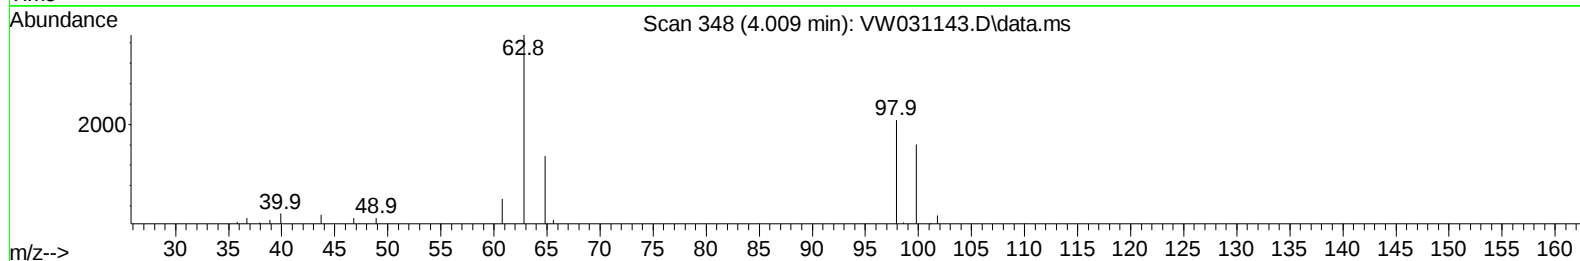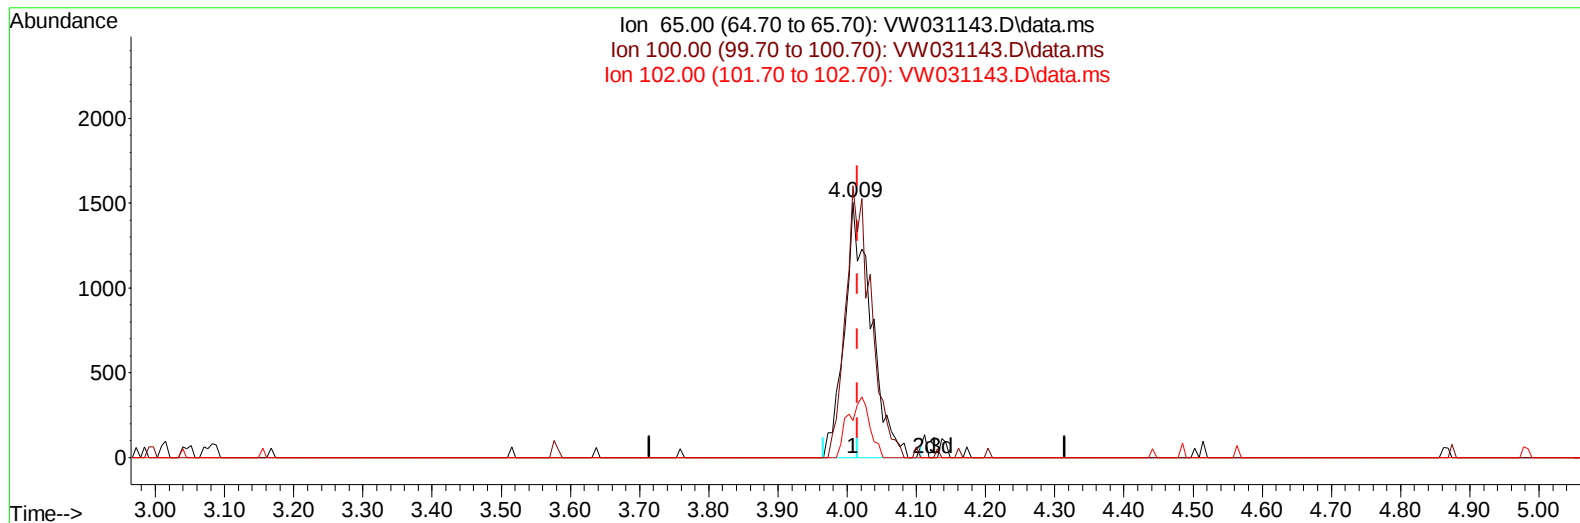

TIC: VW031143.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.009min (-0.006) 23.04 ug/L m

response 4051

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	143.20	101.18
102.00	21.00	7.04#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
 Data File : VW031143.D
 Acq On : 06 Dec 2024 12:12
 Operator : SY/MD
 Sample : P5066-09
 Misc : 7.23g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28M8

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:38:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 06 23:31:46 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
 Supervised By :Semsettin Yesilyurt 12/09/2024

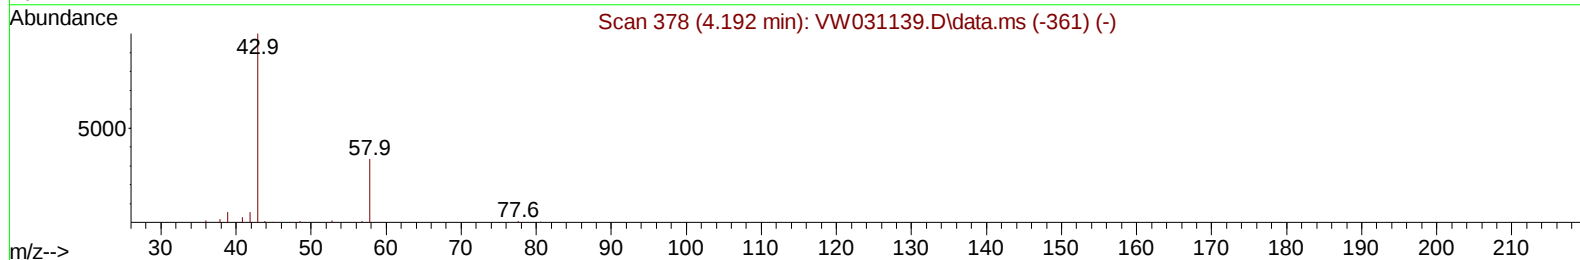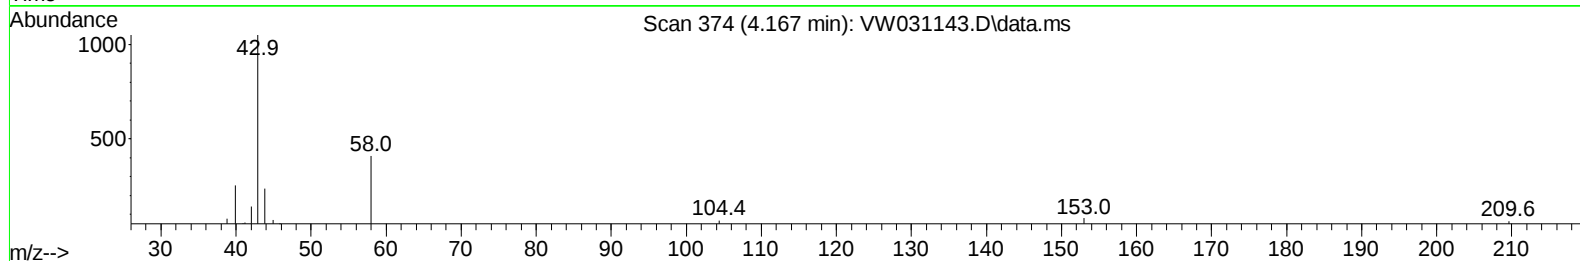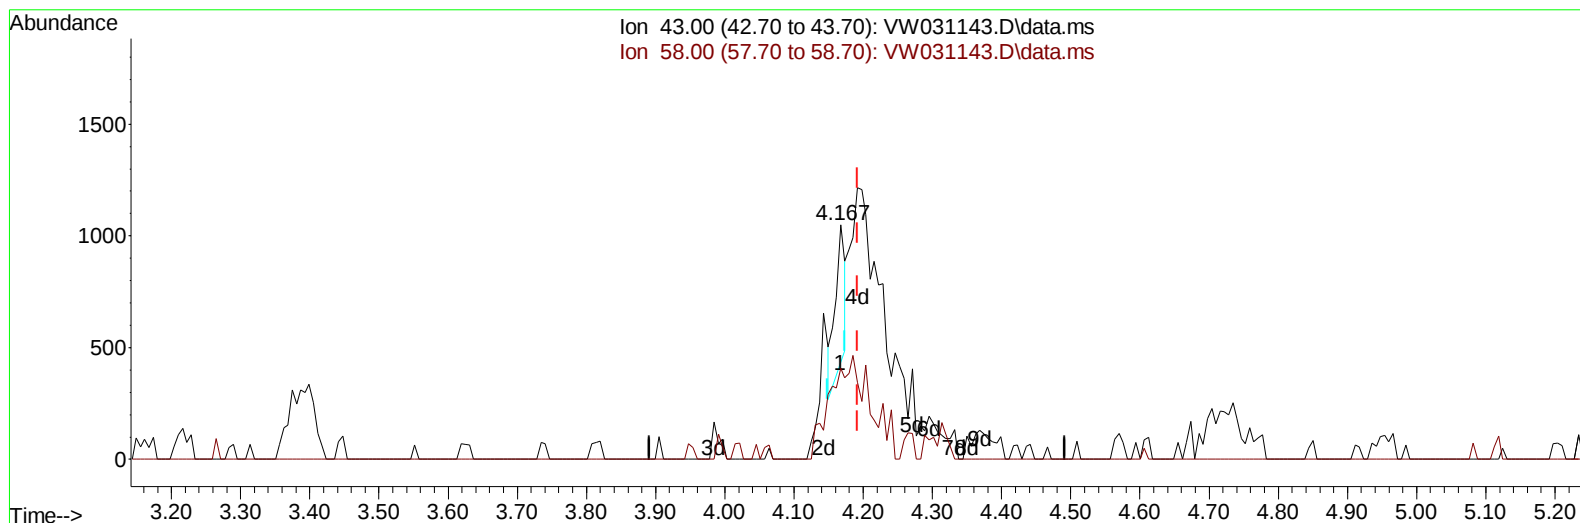

TIC: VW031143.D\data.ms

(13) Acetone (T)

4.167min (-0.024) 5.25 ug/L

response 637

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	44.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031143.D
Acq On : 06 Dec 2024 12:12
Operator : SY/MD
Sample : P5066-09
Misc : 7.23g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M8

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:38:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

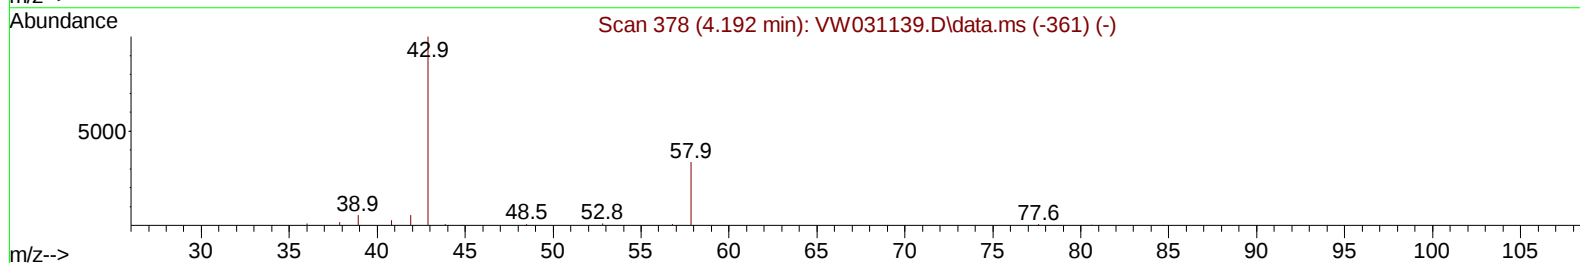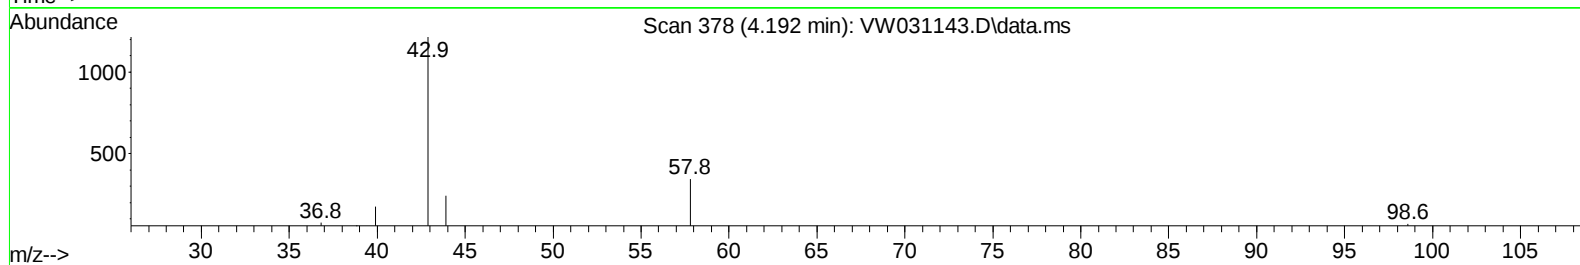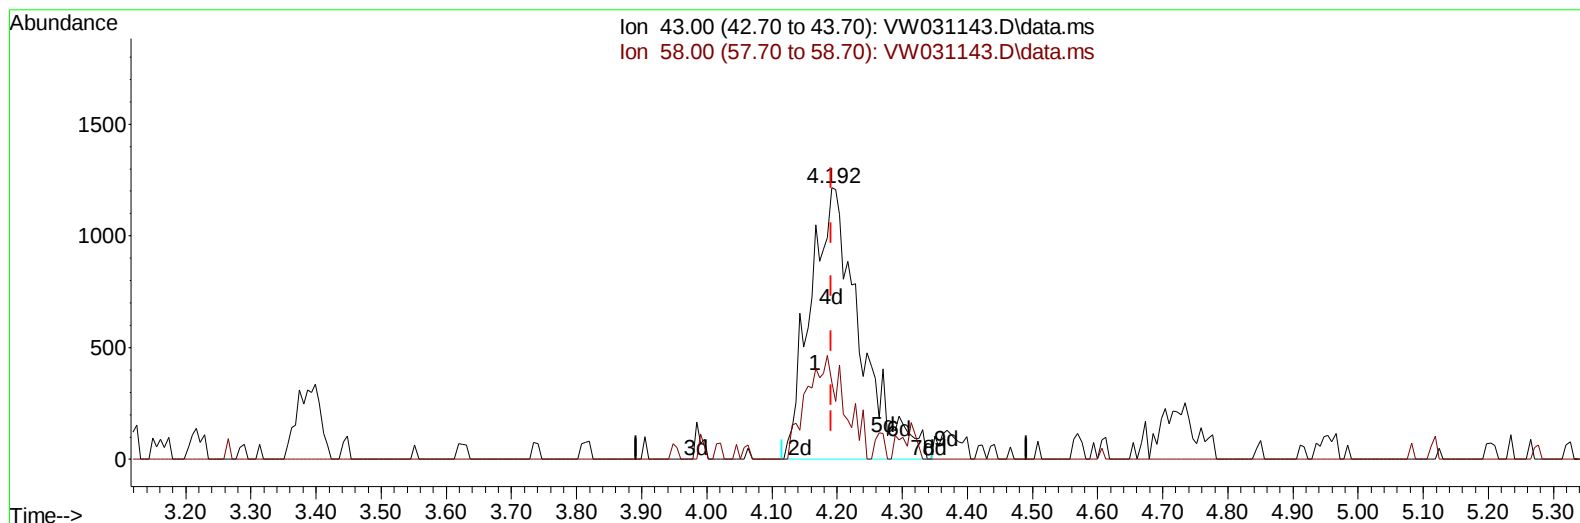

TIC: VW031143.D\data.ms

(13) Acetone (T)

4.192min (+ 0.000) 52.93 ug/L m

response 6421

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	4.39
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031143.D
Acq On : 06 Dec 2024 12:12
Operator : SY/MD
Sample : P5066-09
Misc : 7.23g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M8

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:38:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

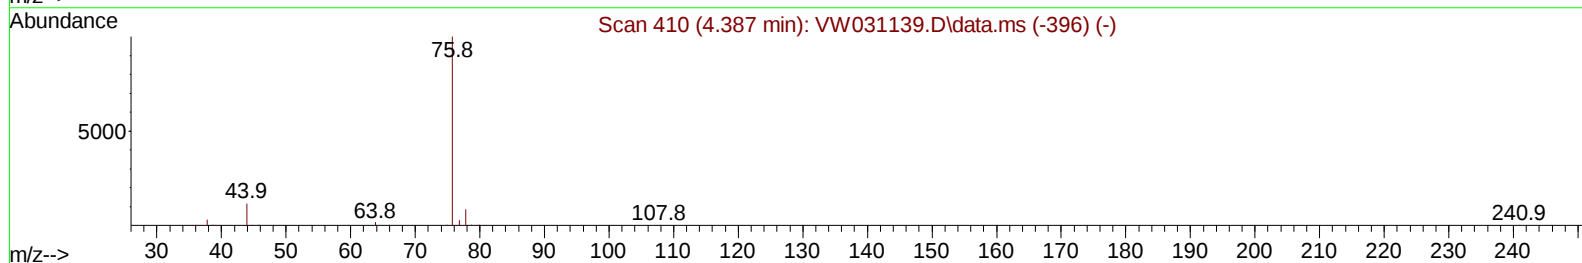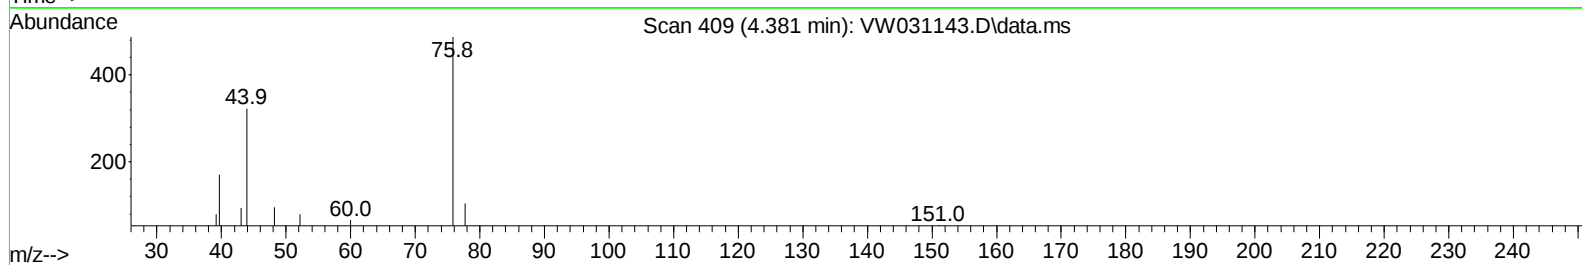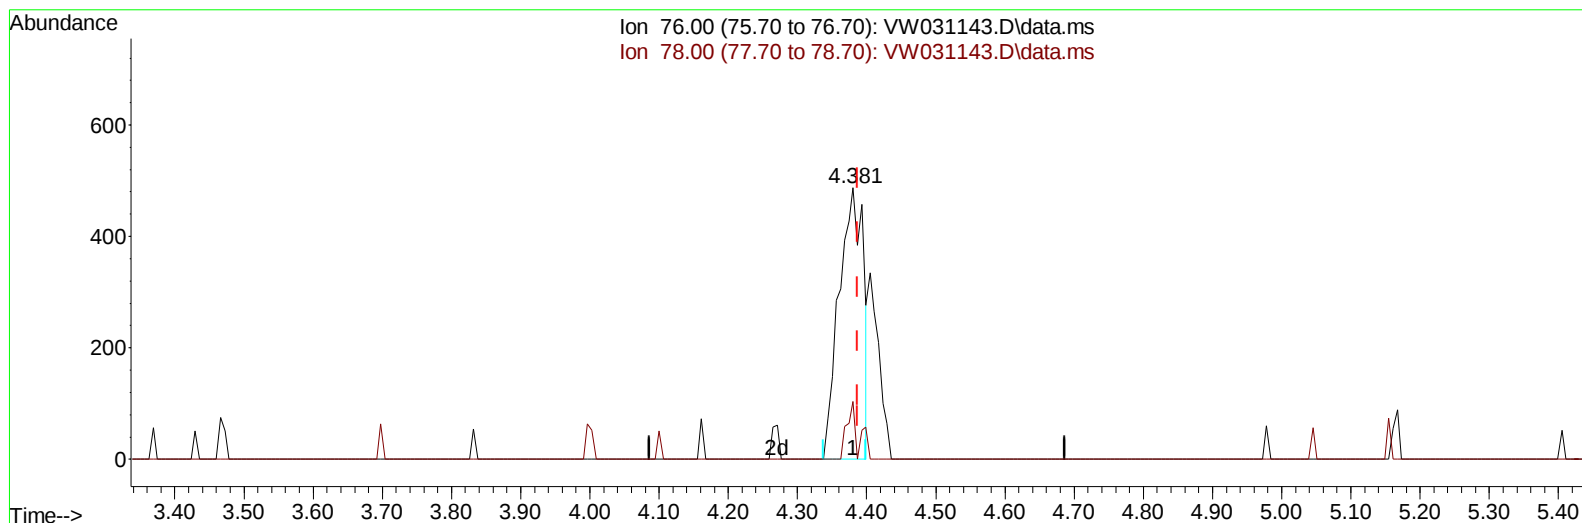

TIC: VW031143.D\data.ms

(14) Carbon disulfide (T)

4.381min (-0.006) 1.02 ug/L

response 1185

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.30	21.36#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031143.D
Acq On : 06 Dec 2024 12:12
Operator : SY/MD
Sample : P5066-09
Misc : 7.23g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M8

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

Quant Time: Dec 06 23:38:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

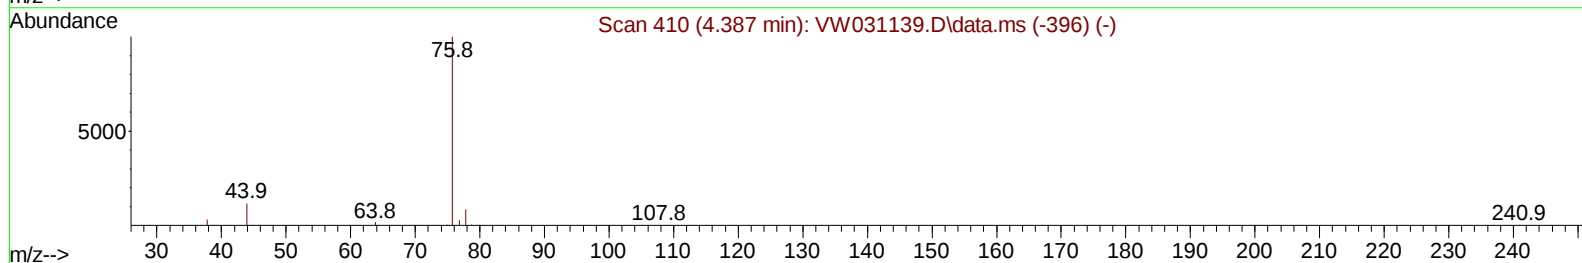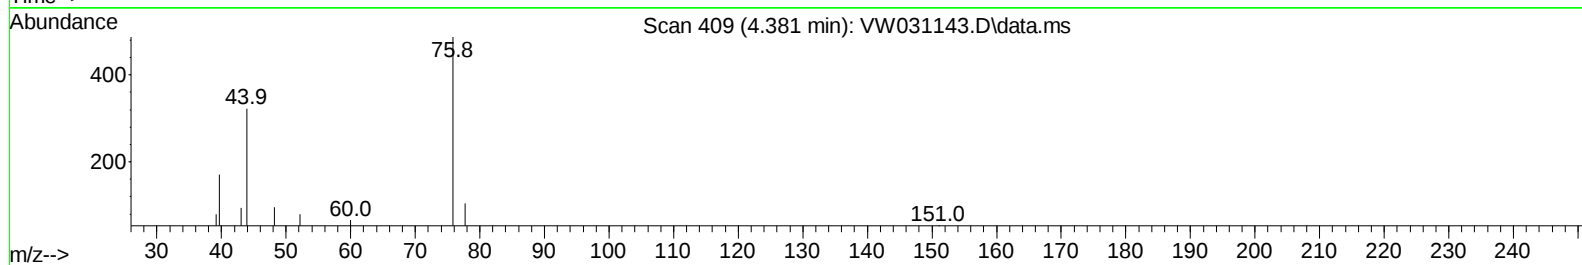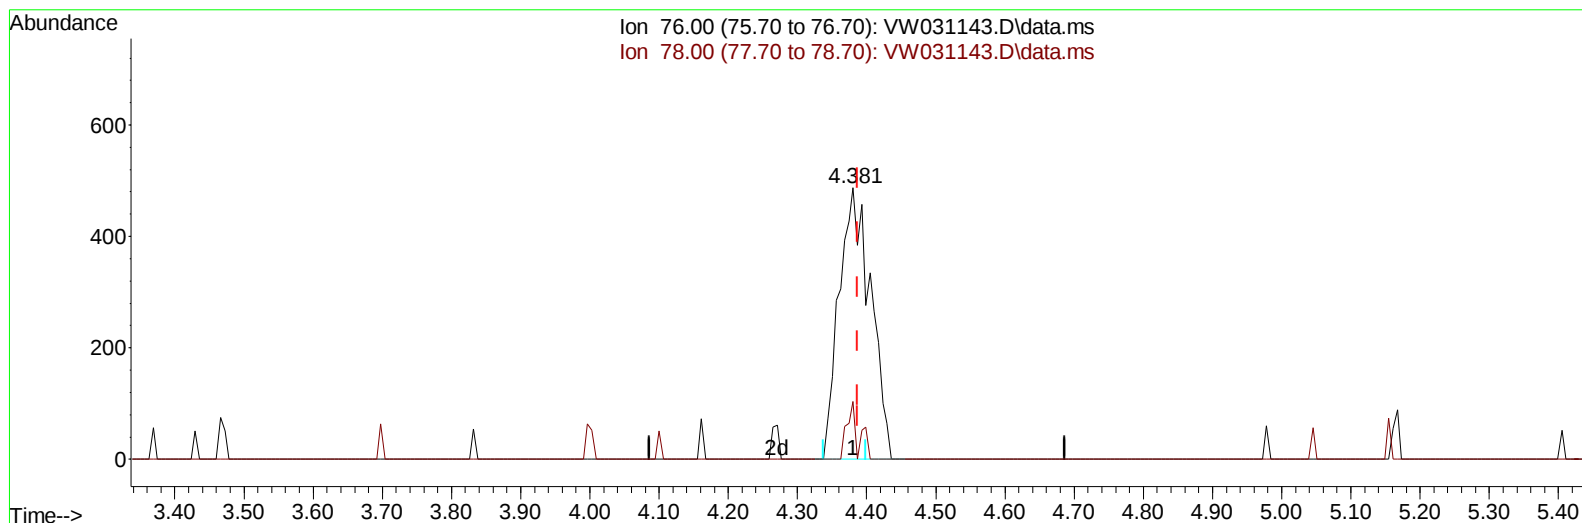

TIC: VW031143.D\data.ms

(14) Carbon disulfide (T)

4.381min (-0.006) 1.32 ug/L m

response 1542

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.30	21.36#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw120624\
 Data File : VW031143.D
 Acq On : 06 Dec 2024 12:12
 Operator : SY/MD
 Sample : P5066-09
 Misc : 7.23g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28M8

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:38:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 06 23:31:46 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
 Supervised By :Semsettin Yesilyurt 12/09/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		25038	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117		24956	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		6502	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		8102	21.027	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	84.120%	
7) Chloroethane-d5	2.887	69		7707	25.781	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	103.120%	
11) 1,1-Dichloroethene-d2	4.009	65		4051m	23.044	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	92.160%	
21) 2-Butanone-d5	7.100	46		34569	513.001	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	1026.000%#	
24) Chloroform-d	7.648	84		29597	40.360	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	161.440%#	
26) 1,2-Dichloroethane-d4	8.307	65		33481	92.784	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	371.120%#	
32) Benzene-d6	8.270	84		41935	27.340	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	109.360%	
36) 1,2-Dichloropropane-d6	9.276	67		18274	40.672	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	162.680%#	
41) Toluene-d8	10.319	98		23203	16.762	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	67.040%	
43) trans-1,3-Dichloroprop...	10.575	79		6943	38.383	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	153.520%#	
47) 2-Hexanone-d5	10.922	63		17374	330.057	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	660.120%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		35145	115.905	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	463.600%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		6356	27.522	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	110.080%	
Target Compounds							
13) Acetone	4.192	43		6421m	52.927	ug/L	Qvalue
14) Carbon disulfide	4.381	76		1542m	1.322	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031143.D
Acq On : 06 Dec 2024 12:12
Operator : SY/MD
Sample : P5066-09
Misc : 7.23g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28M8

Manual IntegrationsAPPROVED

Quant Time: Dec 06 23:38:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 06 23:31:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/09/2024
Supervised By :Semsettin Yesilyurt 12/09/2024

