
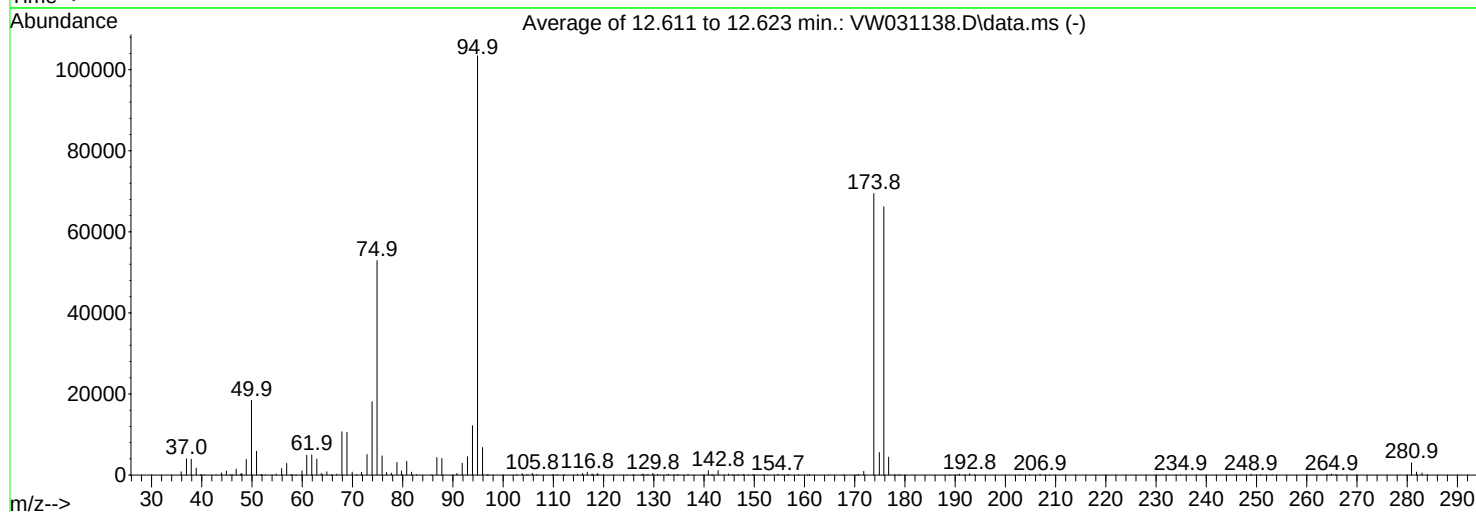


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120624\
Data File : VW031138.D
Acq On : 06 Dec 2024 08:58
Operator : SY/MD
Sample : BFB408
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB408

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Title : SFAM01.0
Last Update : Fri Dec 06 23:31:46 2024

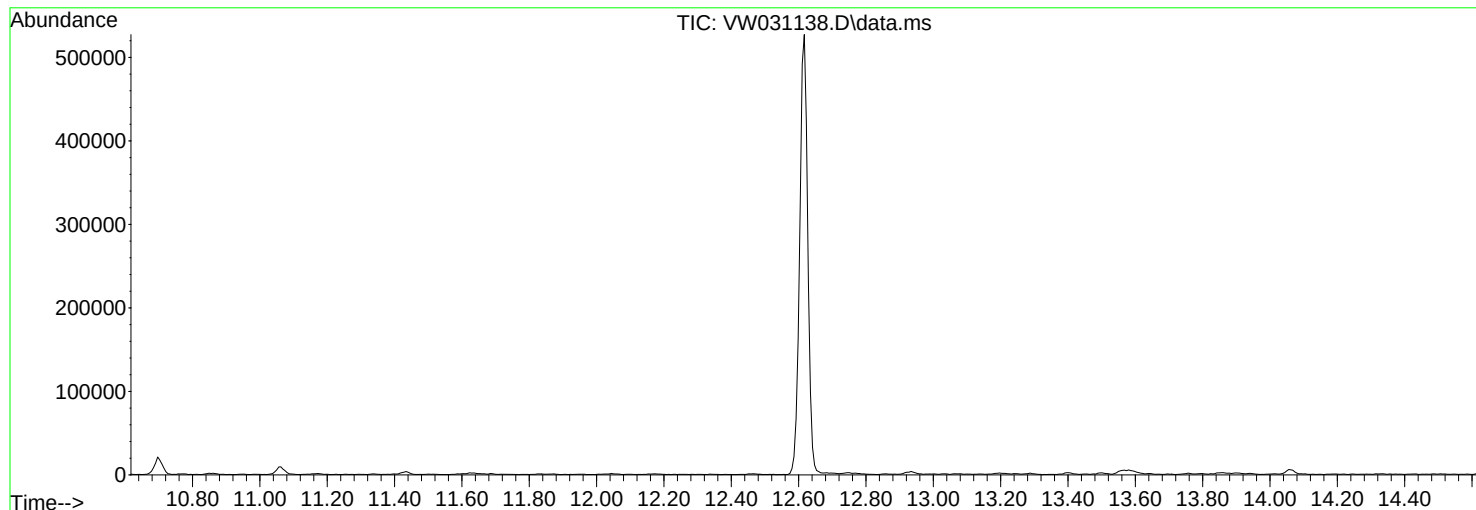

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	18427	PASS
75	95	30	80	51.2	52923	PASS
95	95	100	100	100.0	103440	PASS
96	95	5	9	6.6	6794	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.1	69459	PASS
175	174	5	9	8.0	5560	PASS
176	174	95	101	95.3	66197	PASS
177	176	5	9	6.7	4434	PASS

m/z	Abundance
35.50	103.0
39.70	177.0
43.00	52.0
43.80	89.0

Instrument :
MSVOA_W
ClientSampleId :
BFB408

m/z	Abundance
35.90	757.0
36.90	4394.0
37.90	4437.0
38.90	2007.0
39.90	296.0
42.80	77.0
43.90	673.0
44.80	1188.0
45.70	109.0
46.10	68.0
46.80	1697.0
48.00	503.0
48.80	4297.0
49.90	19856.0
50.90	6222.0
51.80	216.0
52.70	75.0
54.80	409.0
55.90	1807.0
56.90	3242.0
58.00	188.0
58.90	115.0
60.00	1057.0
60.90	4637.0
61.90	5222.0
62.90	4588.0
63.80	497.0
64.90	1062.0
65.90	156.0
67.00	318.0
67.90	10954.0
68.90	10624.0
70.00	885.0
70.80	103.0
71.80	904.0
72.90	5748.0
73.90	18776.0
74.90	56616.0
75.90	5019.0
76.80	616.0
77.80	611.0
78.90	3299.0
79.80	1151.0
80.80	3416.0
81.80	783.0
82.70	152.0
85.90	93.0
86.80	4755.0
87.80	4120.0
90.80	511.0
91.90	2766.0
92.90	4574.0
93.90	12357.0
94.90	106056.0
95.90	7332.0
96.80	259.0
102.70	192.0
103.70	384.0
104.60	181.0
105.80	440.0
106.60	81.0
109.90	144.0
110.80	131.0
112.20	66.0
114.80	155.0
115.80	436.0
116.70	649.0
117.70	335.0
118.70	695.0
124.60	56.0
125.80	157.0
127.90	387.0
128.60	132.0
129.00	101.0
129.80	429.0
130.90	148.0
132.90	389.0
134.00	60.0
134.70	134.0
134.90	133.0
136.80	260.0
140.90	1152.0
141.50	98.0
142.80	1007.0
144.90	306.0
145.80	163.0
146.90	116.0
147.70	192.0
148.80	154.0
149.70	151.0
152.70	73.0
154.60	201.0

Instrument :
MSVOA_W
ClientSampleId :
BFB408

155.60	52.0
156.60	116.0
158.80	155.0
161.00	182.0
164.80	99.0
170.70	256.0
171.70	1032.0
173.80	62232.0
174.90	5472.0
175.80	64632.0
176.70	3738.0
177.90	133.0
178.60	98.0
179.00	175.0
188.90	142.0
190.80	478.0
191.80	76.0
192.80	593.0
193.90	122.0
204.80	108.0
206.90	282.0
207.90	132.0
208.80	67.0
248.90	432.0
250.00	84.0
250.90	222.0
253.10	55.0
264.10	94.0
264.90	487.0
265.80	242.0
267.00	75.0
280.80	5149.0
281.80	1277.0
283.00	818.0
284.00	128.0

Instrument :
MSVOA_W
ClientSampleId :
BFB408

m/z	Abundance
35.90	986.0
37.00	4159.0
37.90	4322.0
38.90	1938.0
39.90	274.0
40.50	111.0
42.80	129.0
43.90	712.0
44.90	856.0
45.80	155.0
46.90	1642.0
47.90	719.0
48.90	3993.0
49.90	21192.0
50.90	6644.0
52.00	329.0
54.80	225.0
56.00	1556.0
56.90	3339.0
57.90	216.0
58.60	60.0
59.90	1101.0
60.90	5467.0
61.90	5684.0
62.90	4019.0
63.80	576.0
64.90	801.0
65.70	79.0
65.90	80.0
66.80	265.0
67.90	11849.0
68.90	11187.0
70.00	659.0
70.90	207.0
71.80	546.0
72.90	5760.0
73.90	20400.0
74.90	59664.0
75.90	5381.0
76.80	689.0
77.70	232.0
78.80	3627.0
79.80	1148.0
80.80	3650.0
81.70	743.0
82.80	174.0
86.80	4723.0
87.80	4859.0
90.90	357.0
91.80	3379.0
92.90	5332.0
93.90	14001.0
94.90	114624.0
95.90	7383.0
97.00	303.0
102.70	161.0
103.80	366.0
104.90	191.0
105.80	531.0
106.70	141.0
109.90	94.0
110.70	164.0
112.20	58.0
114.80	144.0
115.80	465.0
116.80	754.0
117.70	533.0
118.90	668.0
120.00	54.0
126.30	55.0
127.70	457.0
128.80	205.0
129.80	547.0
130.70	249.0
131.30	54.0
132.90	266.0
134.10	97.0
134.80	131.0
136.80	165.0
139.80	55.0
140.90	922.0
142.80	1211.0
144.90	275.0
145.80	110.0
146.80	115.0
147.80	234.0
149.80	240.0
151.80	65.0
154.70	271.0
156.80	212.0
158.80	165.0
160.90	221.0

Instrument :
MSVOA_W
ClientSampleId :
BFB408

170.80	211.0
171.80	837.0
173.80	78424.0
174.90	5842.0
175.80	68136.0
176.80	5540.0
177.90	71.0
190.90	181.0
192.90	213.0
202.80	63.0
204.90	100.0
207.00	174.0
249.00	188.0
250.80	182.0
265.00	286.0
265.80	153.0
280.90	2307.0
281.90	706.0
282.90	474.0
284.10	96.0

Instrument :
MSVOA_W
ClientSampleId :
BFB408

m/z	Abundance
35.90	708.0
36.90	3483.0
37.90	3033.0
38.90	1245.0
39.80	208.0
42.80	82.0
44.00	483.0
45.00	809.0
46.10	153.0
46.90	1137.0
47.70	648.0
48.90	3270.0
49.90	14233.0
50.90	4771.0
51.90	224.0
54.80	157.0
55.80	1486.0
56.90	2045.0
57.70	145.0
59.90	966.0
60.90	4599.0
61.90	4013.0
62.90	3242.0
64.00	336.0
64.90	599.0
66.90	226.0
67.90	9247.0
68.90	9910.0
69.80	661.0
70.80	76.0
71.80	640.0
73.00	3673.0
73.90	15125.0
74.90	42488.0
75.90	3824.0
76.80	639.0
77.70	581.0
78.80	2471.0
79.70	781.0
80.80	3109.0
81.70	648.0
85.70	65.0
86.80	3520.0
87.80	3397.0
90.70	413.0
91.90	2583.0
92.90	3671.0
93.90	10245.0
94.90	89640.0
95.90	5667.0
96.80	219.0
103.90	379.0
105.00	165.0
105.80	327.0
106.80	181.0
109.90	78.0
110.60	52.0
114.80	127.0
115.80	273.0
116.80	767.0
117.90	332.0
118.80	550.0
126.10	59.0
127.50	131.0
128.00	112.0
128.80	137.0
129.70	267.0
130.70	137.0
132.60	93.0
134.60	202.0
136.80	178.0
140.80	1172.0
141.70	225.0
142.80	1132.0
144.90	245.0
145.60	75.0
146.60	94.0
147.90	159.0
149.70	114.0
151.70	75.0
154.80	260.0
155.70	70.0
156.80	135.0
158.70	116.0
160.60	96.0
161.10	56.0
167.70	78.0
170.40	127.0
170.80	115.0
171.90	904.0
173.80	67720.0
174.90	5365.0

Instrument :
MSVOA_W
ClientSampleId :
BFB408

175.80	65824.0
176.80	4025.0
177.90	77.0
190.50	78.0
191.00	99.0
192.80	192.0
206.80	204.0
234.90	50.0
248.80	129.0
251.00	55.0
264.60	147.0
280.90	1673.0
282.00	223.0
282.90	251.0

Instrument :
MSVOA_W
ClientSampleId :
BFB408