

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120821\
 Data File : VW021230.D
 Acq On : 08 Dec 2021 15:18
 Operator : SY/VA
 Sample : VIBLK517
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK517

Quant Time: Dec 08 23:02:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120321SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 08 22:58:53 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	90120	25.000	ug/L	# 0.00
28) Chlorobenzene-d5		11.628	117	90845	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	50328	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.355	65	38915	30.993	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	123.960%	
7) Chloroethane-d5		2.885	69	27811	33.087	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	132.360%	
11) 1,1-Dichloroethene-d2		4.019	63	42130	21.003	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.000%	
21) 2-Butanone-d5		7.074	46	13445	46.945	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.900%	
24) Chloroform-d		7.653	84	64796	28.710	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	114.840%	
26) 1,2-Dichloroethane-d4		8.305	65	34964	28.318	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	113.280%	
32) Benzene-d6		8.275	84	126711	27.279	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.120%	
36) 1,2-Dichloropropane-d6		9.275	67	35069	27.168	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.680%	
41) Toluene-d8		10.323	98	125791	26.411	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.640%	
43) trans-1,3-Dichloroprop...		10.579	79	13560	23.135	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.520%	
47) 2-Hexanone-d5		10.921	63	11091	44.908	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.820%	
56) 1,1,2,2-Tetrachloroeth...		12.689	84	27135	22.722	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.880%	
66) 1,2-Dichlorobenzene-d4		13.853	152	46536	25.807	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.240%	
Target Compounds							
13) Acetone		4.123	43	937	3.592	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120821\
Data File : VW021230.D
Acq On : 08 Dec 2021 15:18
Operator : SY/VA
Sample : VIBLK517
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK517

Quant Time: Dec 08 23:02:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120321SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 08 22:58:53 2021
Response via : Initial Calibration

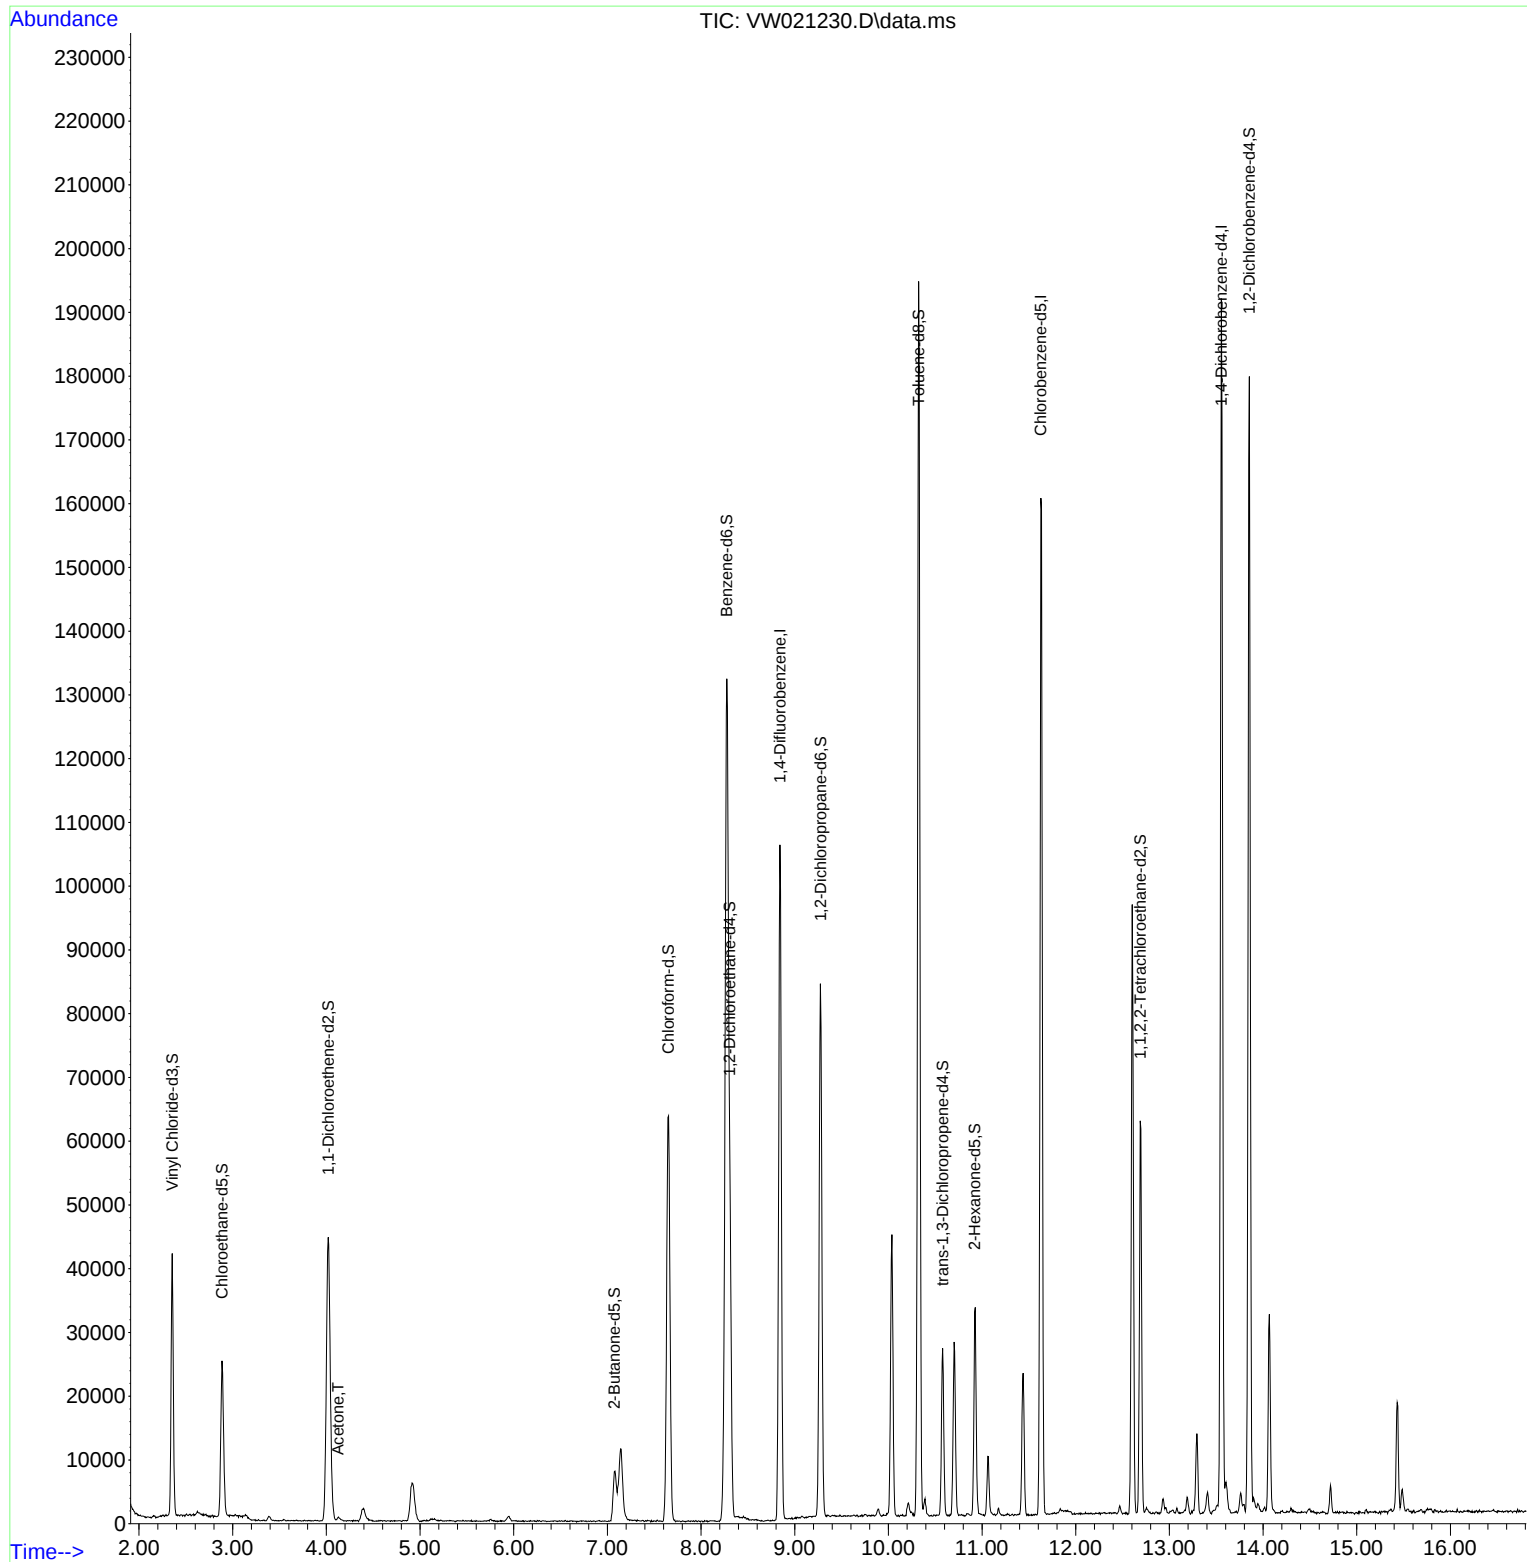

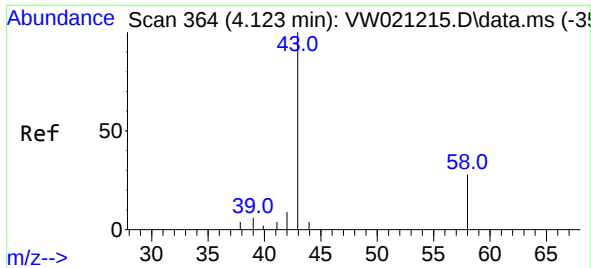

#13
 Acetone
 Concen: 3.592 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW021230.D
 Acq: 08 Dec 2021 15:18

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK517

Tgt Ion: 43 Resp: 937
 Ion Ratio Lower Upper
 43 100
 58 21.7 0.0 52.8

