


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW121018\
 Data File : VW007350.D
 Acq On : 10 Dec 2018 09:16
 Operator : SY/AP
 Sample : BFB84
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
 Title : VOC Analysis
 Last Update : Tue Dec 11 01:18:15 2018

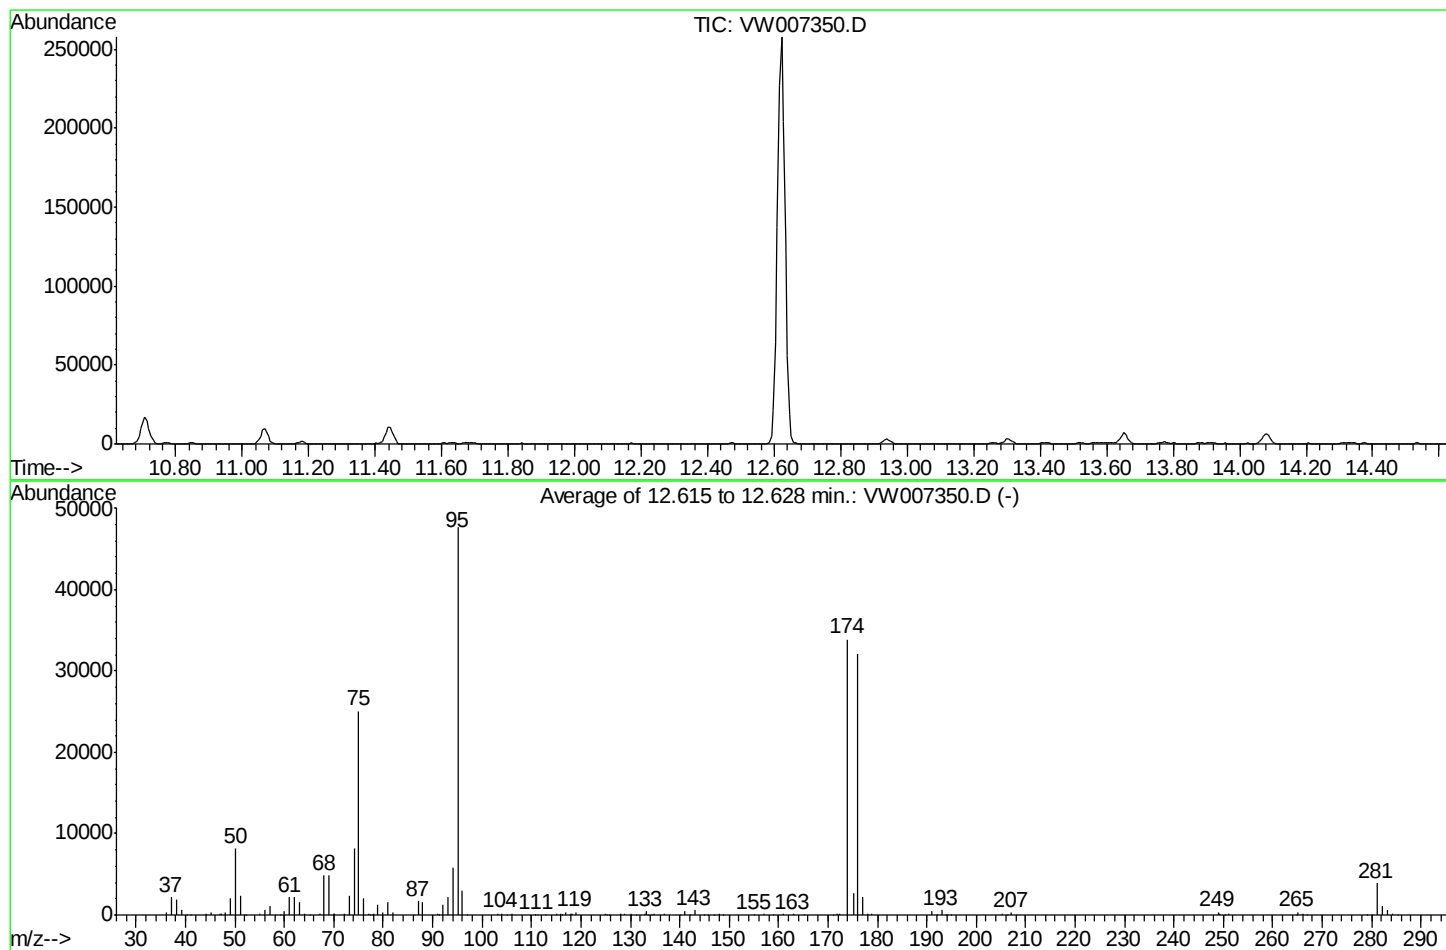

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	8179	PASS
75	95	30	80	52.7	25106	PASS
95	95	100	100	100.0	47666	PASS
96	95	5	9	6.3	3001	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.0	33850	PASS
175	174	5	9	7.8	2625	PASS
176	174	95	101	95.1	32176	PASS
177	176	5	9	7.0	2241	PASS

m/z	Abundance
36.10	510.0
37.10	2438.0
38.00	1888.0
39.10	604.0
40.30	52.0
41.00	61.0
44.00	281.0
45.00	404.0
47.10	288.0
48.00	379.0
49.00	1792.0
50.10	9061.0
51.10	2383.0
52.00	106.0
54.90	149.0
56.00	626.0
57.00	1172.0
58.00	57.0
59.20	73.0
60.00	347.0
61.00	2176.0
62.10	2250.0
63.00	1595.0
64.10	156.0
65.00	83.0
67.10	124.0
68.00	5078.0
69.10	4869.0
70.00	360.0
72.00	222.0
73.00	2647.0
74.00	8234.0
75.10	23624.0
76.10	2549.0
77.00	179.0
77.90	121.0
78.90	1398.0
80.00	473.0
80.90	1587.0
81.90	344.0
87.00	1500.0
88.00	1732.0
90.90	181.0
92.00	1266.0
93.00	2019.0
94.00	6164.0
95.10	47888.0
96.00	3319.0
97.20	52.0
103.10	173.0
103.90	252.0
104.90	60.0
106.00	263.0
112.90	51.0
115.00	51.0
115.80	140.0
116.10	114.0
116.90	320.0
118.10	216.0
118.90	413.0
124.90	148.0
125.40	86.0
127.90	136.0
128.80	54.0
130.10	200.0
131.20	71.0
133.10	639.0
134.20	154.0
134.80	129.0
137.10	108.0
141.00	482.0
143.00	447.0
144.90	69.0
145.70	82.0
146.90	128.0
147.90	120.0
148.90	52.0
155.00	94.0
157.10	76.0
159.00	73.0
161.00	79.0
163.00	173.0
165.10	81.0
171.00	53.0
172.00	200.0
174.00	32552.0
175.10	2354.0
176.00	27712.0
177.00	1979.0
178.00	146.0
179.00	199.0
191.00	673.0

Instrument :
MSVOA_W
ClientSampleId :
BFB84

192.10	214.0
193.00	726.0
193.80	106.0
195.00	121.0
205.10	138.0
207.10	341.0
208.00	87.0
249.00	391.0
250.20	146.0
251.00	296.0
265.00	389.0
266.20	169.0
267.00	113.0
281.10	4891.0
282.10	1410.0
283.20	901.0
284.10	171.0
285.20	104.0

Instrument :
MSVOA_W
ClientSampleId :
BFB84

Scan 1750 (12.573 min): VW007350.D
BFB84

m/z	Abundance
36.00	105.0
38.10	51.0
44.00	65.0

Instrument :
MSVOA_W
ClientSampleId :
BFB84

m/z	Abundance
36.10	374.0
37.10	1848.0
38.10	1614.0
39.10	554.0
44.10	311.0
45.00	411.0
47.00	264.0
48.10	262.0
49.10	1766.0
50.10	6860.0
51.10	2121.0
52.10	121.0
54.90	114.0
56.00	489.0
57.00	1043.0
60.10	418.0
61.10	1797.0
62.00	1734.0
63.10	1354.0
64.10	92.0
65.10	56.0
67.20	179.0
68.10	4071.0
69.10	4177.0
70.10	339.0
72.00	355.0
73.00	2004.0
74.10	7086.0
75.00	23008.0
76.00	1518.0
77.20	207.0
78.10	256.0
78.90	1263.0
80.00	282.0
80.90	1397.0
82.00	298.0
87.10	1544.0
87.90	1356.0
90.90	145.0
92.00	1173.0
93.00	2075.0
94.00	5038.0
95.10	39584.0
96.10	2449.0
97.00	94.0
103.10	64.0
103.80	243.0
105.00	58.0
105.90	183.0
110.80	81.0
115.00	96.0
115.90	136.0
117.00	313.0
117.90	238.0
119.00	387.0
125.20	70.0
128.00	169.0
129.00	87.0
129.90	214.0
131.00	52.0
132.90	348.0
133.60	56.0
135.00	104.0
136.90	137.0
139.80	55.0
141.00	529.0
142.00	88.0
143.00	667.0
145.90	98.0
148.00	65.0
155.10	73.0
157.00	97.0
159.10	57.0
160.90	92.0
171.80	163.0
174.00	33208.0
175.10	2485.0
176.00	32432.0
177.00	2181.0
178.00	75.0
178.80	56.0
191.20	276.0
193.00	399.0
205.10	90.0
207.10	184.0
249.00	268.0
264.80	159.0
265.20	194.0
266.10	67.0
280.20	129.0
281.20	2559.0
282.10	723.0

Instrument :
MSVOA_W
ClientSampleId :
BFB84

283.10496.0

284.1080.0

Instrument :
MSVOA_W
ClientSampleId :
BFB84

m/z	Abundance
36.00	625.0
37.10	2221.0
38.10	2110.0
39.10	694.0
44.00	250.0
45.10	371.0
47.30	394.0
48.10	307.0
49.10	2394.0
50.10	8618.0
51.10	2809.0
52.20	119.0
54.90	130.0
56.10	781.0
57.00	1192.0
59.20	82.0
60.00	488.0
61.00	2629.0
62.00	2626.0
63.10	1912.0
64.10	230.0
65.00	82.0
67.10	161.0
68.10	5408.0
69.00	5781.0
70.20	327.0
72.20	236.0
73.10	2652.0
74.10	9286.0
75.10	28688.0
76.10	2192.0
77.00	324.0
79.00	1354.0
80.00	394.0
81.00	1557.0
82.00	403.0
86.20	70.0
87.00	1973.0
88.00	1842.0
91.20	171.0
92.10	1384.0
93.00	2388.0
94.10	6400.0
95.10	55528.0
96.00	3236.0
97.00	70.0
103.10	125.0
103.90	225.0
105.00	69.0
105.90	229.0
111.10	86.0
112.90	53.0
115.00	110.0
115.80	150.0
117.00	426.0
117.80	260.0
118.20	248.0
118.90	351.0
124.90	188.0
125.70	54.0
128.00	272.0
128.90	118.0
130.00	184.0
131.00	77.0
133.20	574.0
134.90	207.0
136.90	169.0
139.90	76.0
141.10	550.0
142.20	87.0
143.00	644.0
144.90	83.0
145.80	64.0
147.00	102.0
147.90	138.0
155.10	70.0
157.10	85.0
158.90	83.0
160.90	109.0
162.90	154.0
165.00	92.0
172.30	276.0
174.00	35792.0
175.10	3038.0
176.00	36384.0
177.00	2564.0
177.90	124.0
178.90	151.0
191.10	419.0
193.00	759.0
194.10	163.0
194.90	75.0

Instrument :
MSVOA_W
ClientSampleId :
BFB84

205.20	160.0
206.30	80.0
207.10	304.0
208.10	74.0
248.90	289.0
249.20	292.0
250.20	101.0
251.10	171.0
265.10	409.0
266.10	91.0
267.00	74.0
279.20	63.0
281.10	4355.0
282.10	1386.0
283.10	731.0
284.20	117.0

Instrument :
MSVOA_W
ClientSampleId :
BFB84