

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121024\
 Data File : VW031197.D
 Acq On : 10 Dec 2024 17:30
 Operator : SY/MD
 Sample : P5155-02
 Misc : 4.93g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 11 00:32:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 11 00:26:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	453696	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117	277941	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	48600	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	83140	11.908	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	47.640%
7) Chloroethane-d5	2.893	69	76195	14.066	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.280%
11) 1,1-Dichloroethene-d2	4.015	65	37395	11.739	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.960%
21) 2-Butanone-d5	6.953	46	92	0.075	ug/L	-0.15
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.160%#
24) Chloroform-d	7.648	84	201066	15.131	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	60.520%
26) 1,2-Dichloroethane-d4	8.410	65	271	0.041	ug/L	0.11
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.160%#
32) Benzene-d6	8.270	84	329445	19.285	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.160%
36) 1,2-Dichloropropane-d6	9.270	67	122850	24.551	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.200%
41) Toluene-d8	10.325	98	228578	14.827	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	59.320%
43) trans-1,3-Dichloroprop...	10.574	79	38437	19.079	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.320%
47) 2-Hexanone-d5	10.922	63	35686	60.871	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.740%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	89435	26.483	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.920%
66) 1,2-Dichlorobenzene-d4	13.848	152	30210	17.501	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	70.000%#
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3152	0.447	ug/L	# 33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121024\
Data File : VW031197.D
Acq On : 10 Dec 2024 17:30
Operator : SY/MD
Sample : P5155-02
Misc : 4.93g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 11 00:32:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 11 00:26:57 2024
Response via : Initial Calibration

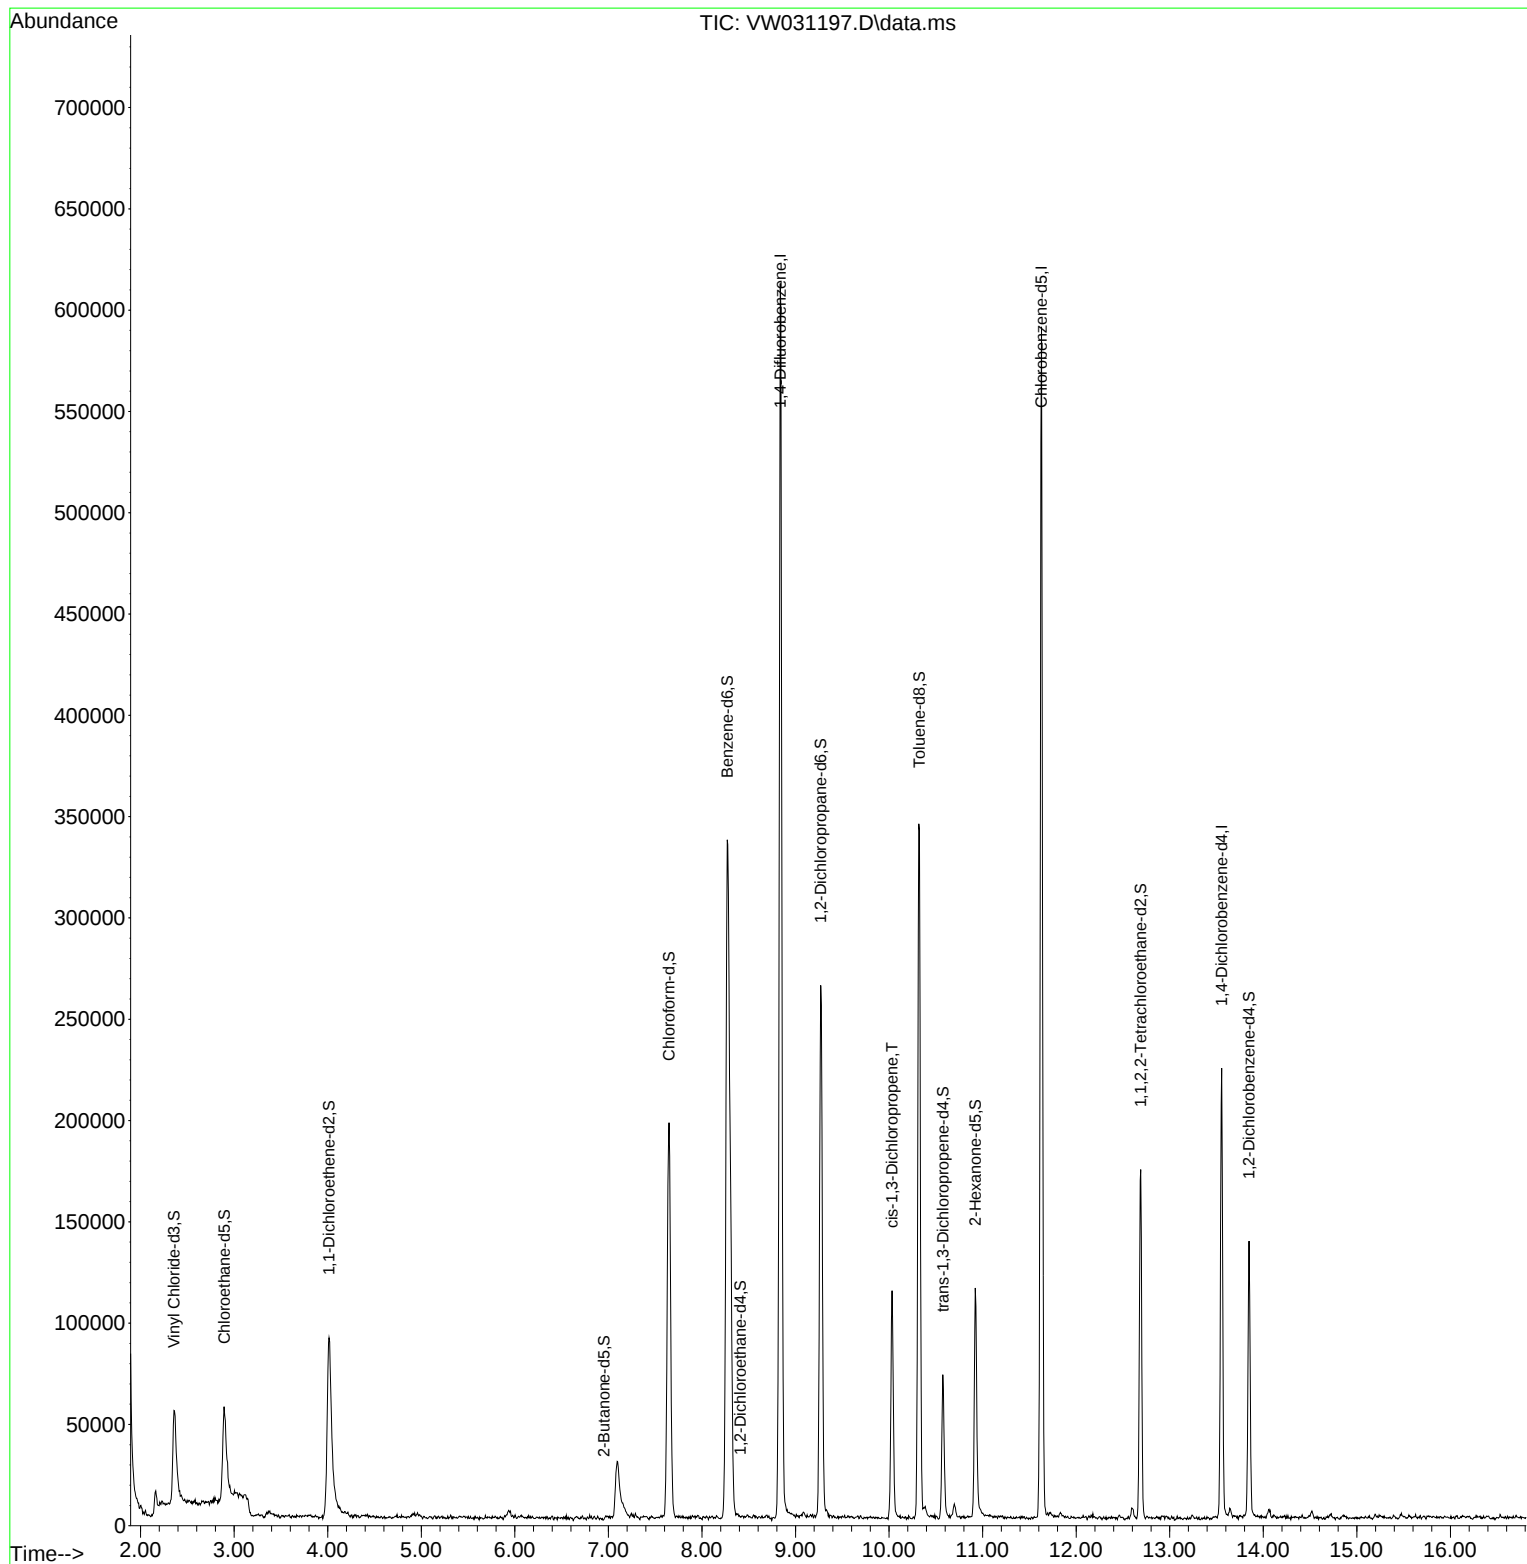

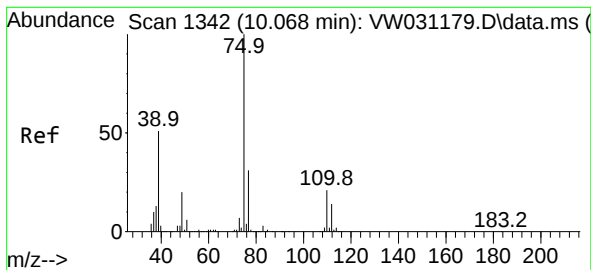

#39
 cis-1,3-Dichloropropene
 Concen: 0.447 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW031197.D
 Acq: 10 Dec 2024 17:30

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3152
 Ion Ratio Lower Upper
 75 100
 77 67.8 21.6 40.2#

