




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121024\
 Data File : VW031195.D
 Acq On : 10 Dec 2024 16:42
 Operator : SY/MD
 Sample : P5153-07
 Misc : 6.08g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28P5

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:32:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 11 00:26:57 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2024
 Supervised By :Semsettin Yesilyurt 12/11/2024

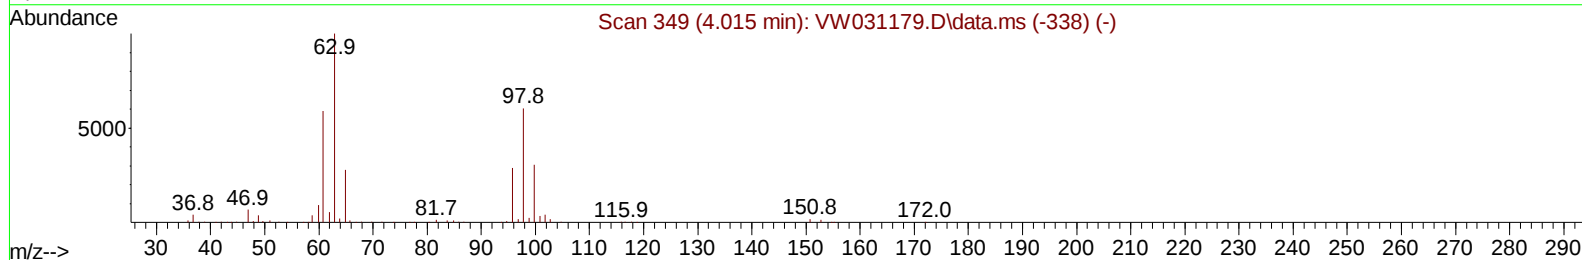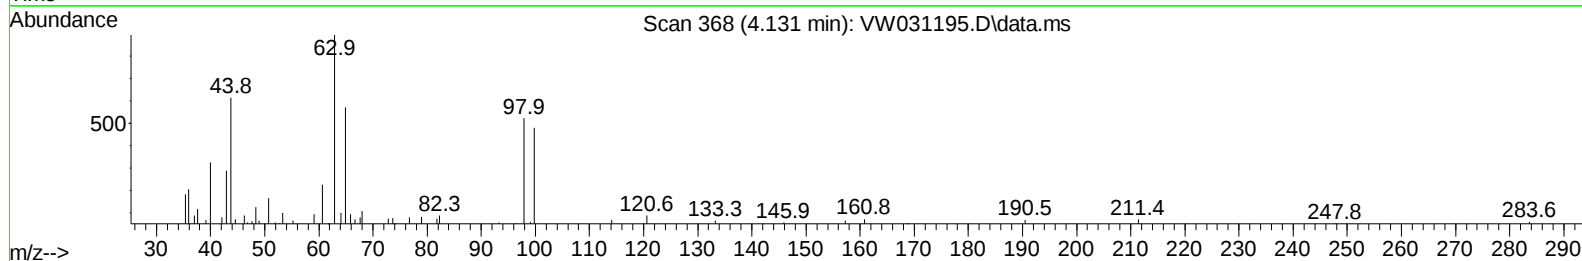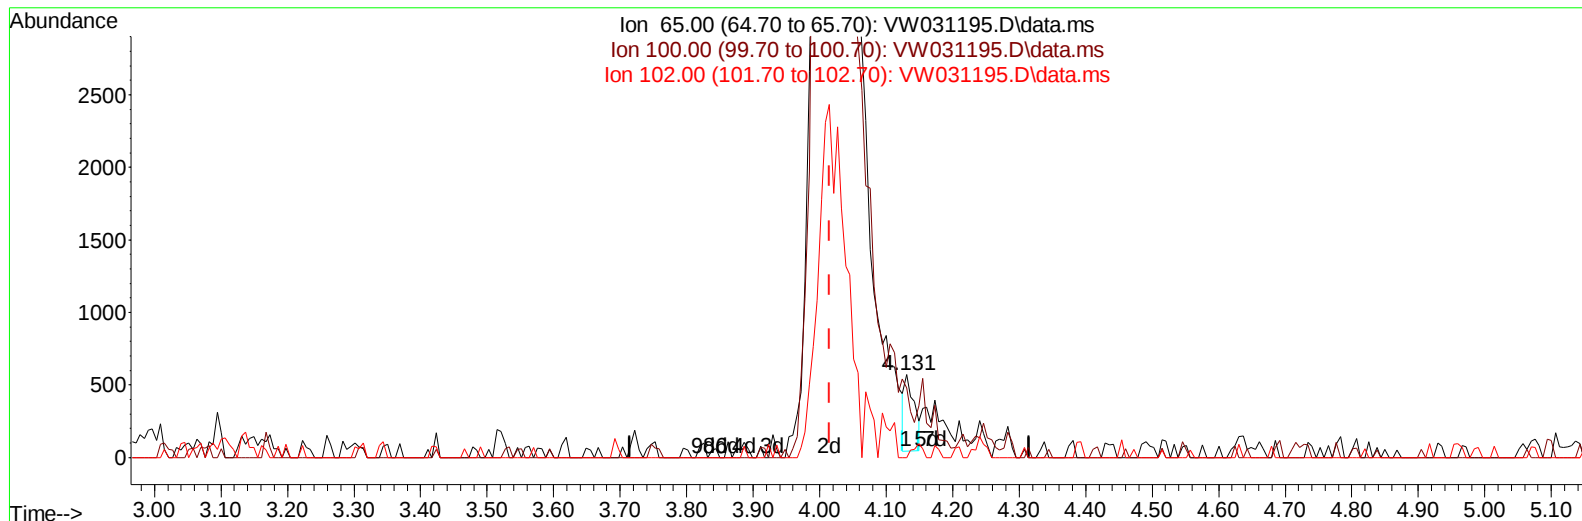

TIC: VW031195.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.131min (+ 0.116) 0.17 ug/L

response 529

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	143.20	123.44
102.00	21.00	16.45
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121024\
Data File : VW031195.D
Acq On : 10 Dec 2024 16:42
Operator : SY/MD
Sample : P5153-07
Misc : 6.08g/10mL/MSVOA_W/SOIL/B
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28P5

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:32:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 11 00:26:57 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2024
Supervised By :Semsettin Yesilyurt 12/11/2024

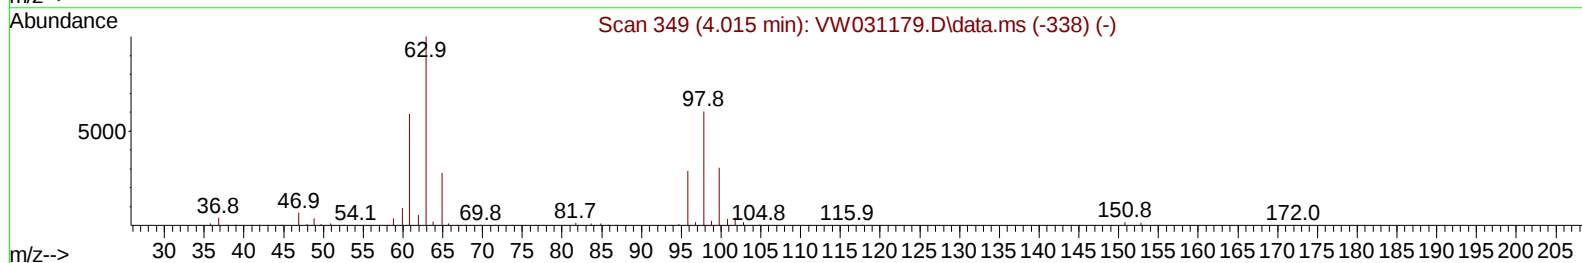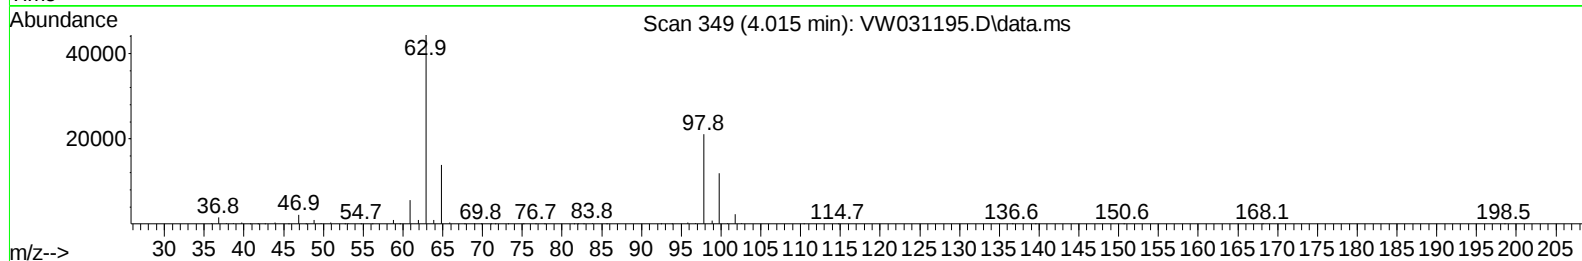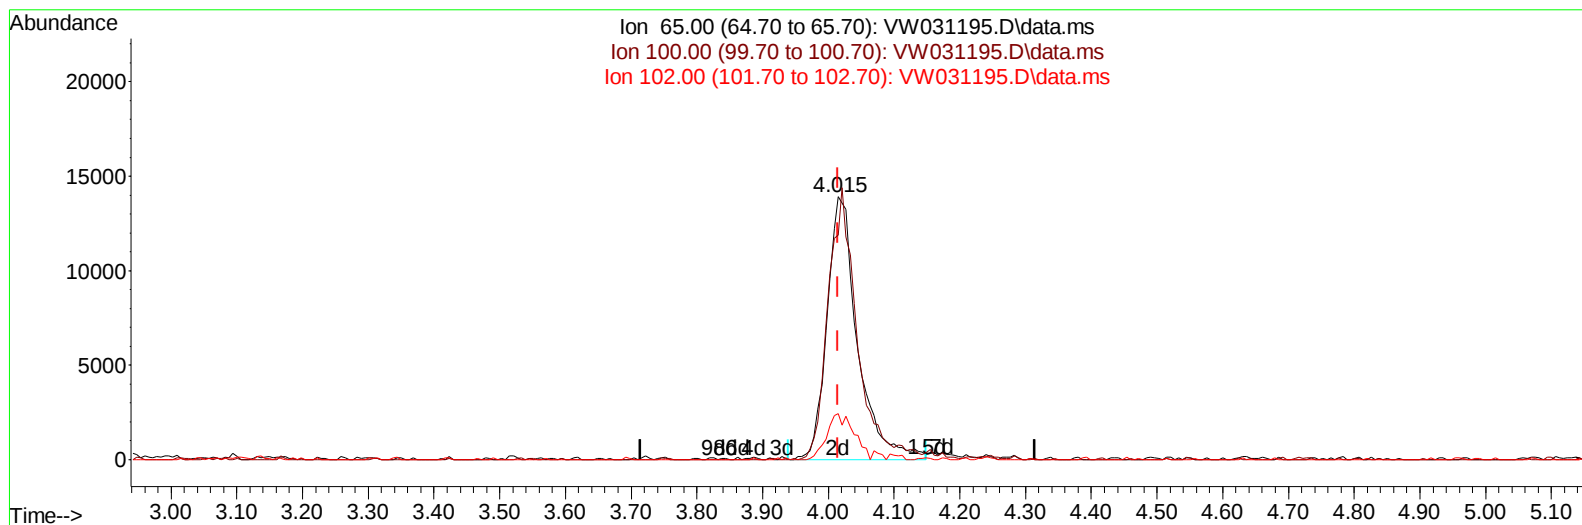

TIC: VW031195.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.015min (+ 0.000) 14.56 ug/L m

response 44961

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	143.20	1.45#
102.00	21.00	0.19#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121024\
 Data File : VW031195.D
 Acq On : 10 Dec 2024 16:42
 Operator : SY/MD
 Sample : P5153-07
 Misc : 6.08g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28P5

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:32:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 11 00:26:57 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2024
 Supervised By :Semsettin Yesilyurt 12/11/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		439737	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117		307912	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		63554	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		96582	14.272	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	57.080%		
7) Chloroethane-d5	2.899	69		82238	15.664	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	62.640%		
11) 1,1-Dichloroethene-d2	4.015	65		44961m	14.563	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	58.240%		
21) 2-Butanone-d5	7.093	46		14061	11.881	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	23.760%		
24) Chloroform-d	7.648	84		227492	17.663	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	70.640%		
26) 1,2-Dichloroethane-d4	8.307	65		133462	21.059	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	84.240%		
32) Benzene-d6	8.276	84		366398	19.361	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	77.440%		
36) 1,2-Dichloropropane-d6	9.270	67		135509	24.445	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	97.760%		
41) Toluene-d8	10.325	98		276731	16.203	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	64.800%		
43) trans-1,3-Dichloroprop...	10.575	79		33475	14.999	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	60.000%		
47) 2-Hexanone-d5	10.922	63		14316	22.042	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	44.080%		
56) 1,1,2,2-Tetrachloroeth...	12.684	84		95934	25.642	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	102.560%		
66) 1,2-Dichlorobenzene-d4	13.848	152		44048	19.513	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	78.040%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121024\
Data File : VW031195.D
Acq On : 10 Dec 2024 16:42
Operator : SY/MD
Sample : P5153-07
Misc : 6.08g/10mL/MSVOA_W/SOIL/B
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28P5

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:32:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 11 00:26:57 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2024
Supervised By :Semsettin Yesilyurt 12/11/2024

