

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121121\
 Data File : VW021328.D
 Acq On : 11 Dec 2021 15:41
 Operator : SY/VA
 Sample : M5062-05
 Misc : 6.80g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGL04

Manual IntegrationsAPPROVED

Quant Time: Dec 12 08:08:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 23:12:45 2021
 Response via : Initial Calibration




Reviewed By :Semsettin
 Yesilyurt

12/13/2021

Supervised By :Mahesh

Dadoda

12/15/2021

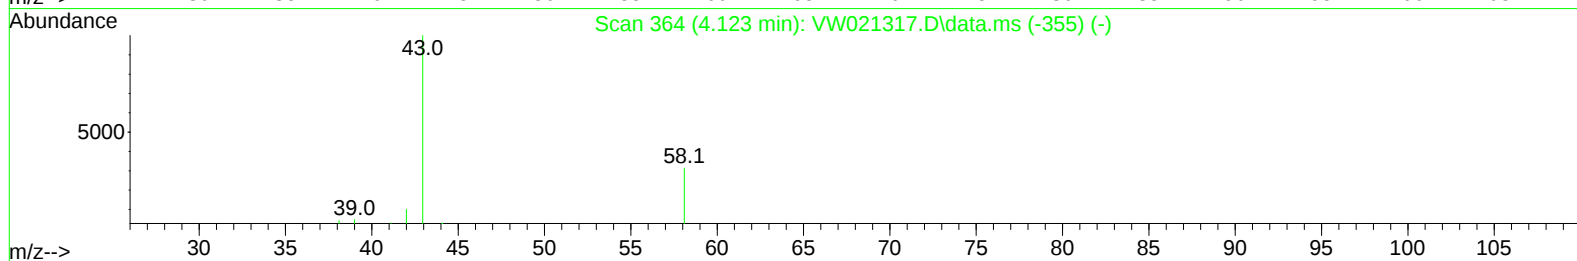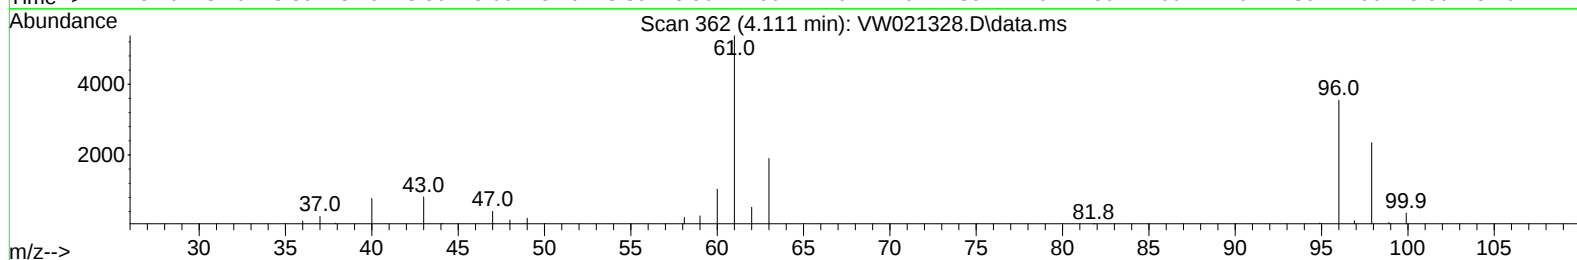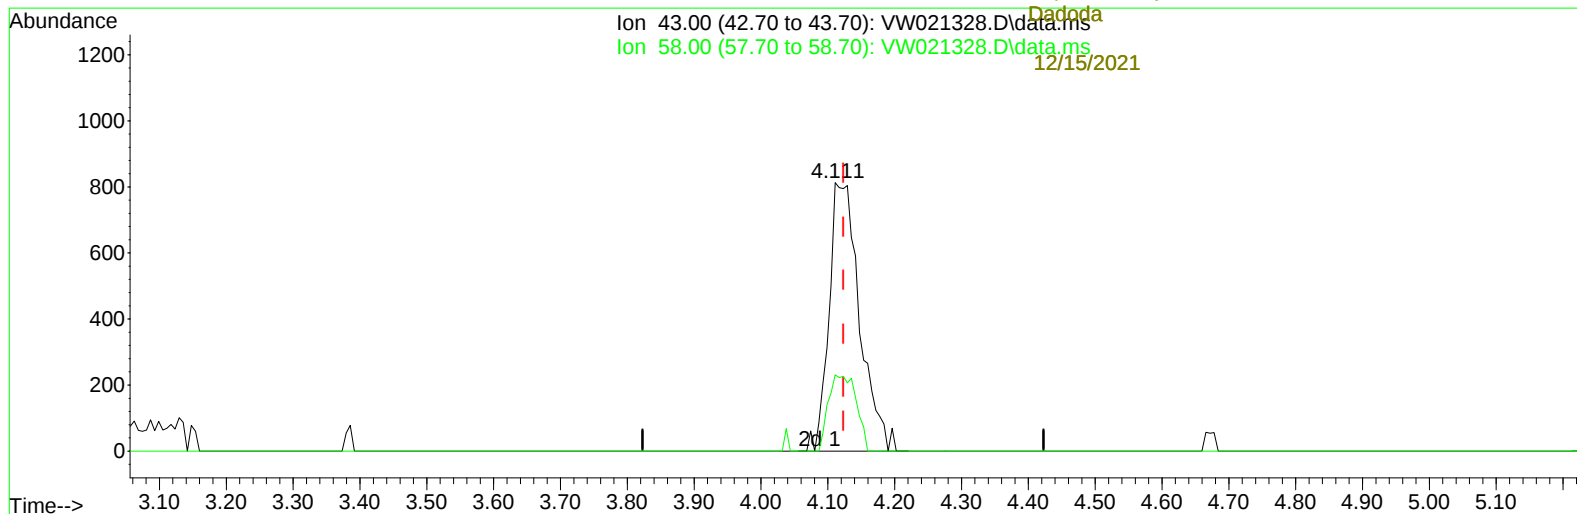

TIC: VW021328.D\data.ms

(13) Acetone (T)

4.111min (-0.012) 12.48 ug/L m

response 2589

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	17.77
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121121\
 Data File : VW021328.D
 Acq On : 11 Dec 2021 15:41
 Operator : SY/VA
 Sample : M5062-05
 Misc : 6.80g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGL04




Manual IntegrationsAPPROVED

Quant Time: Dec 12 08:08:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 23:12:45 2021
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

12/13/2021
 Supervised By :Mahesh
 Dadoda

12/15/2021

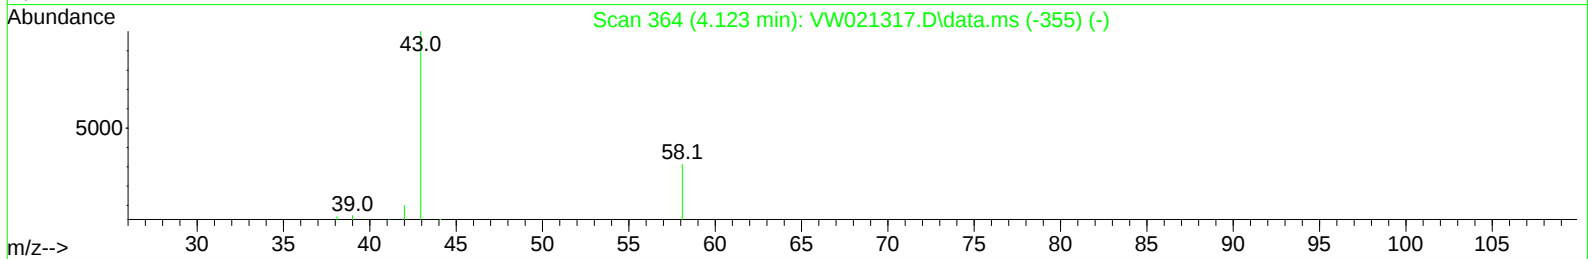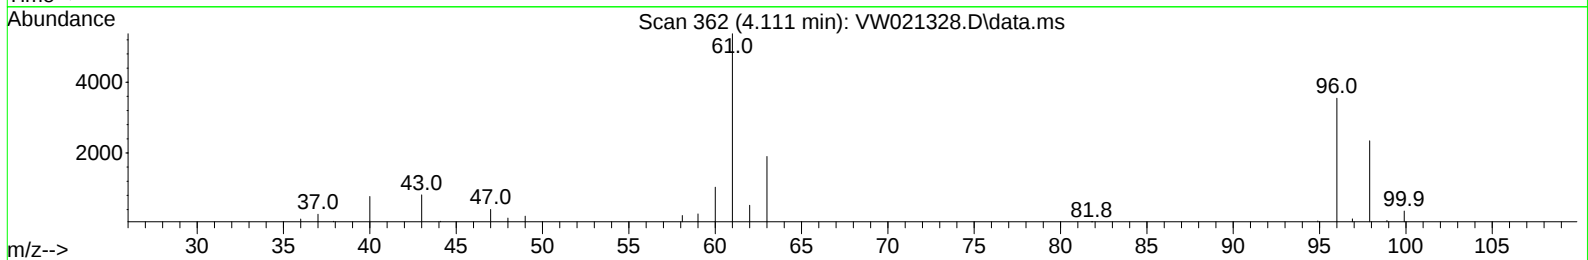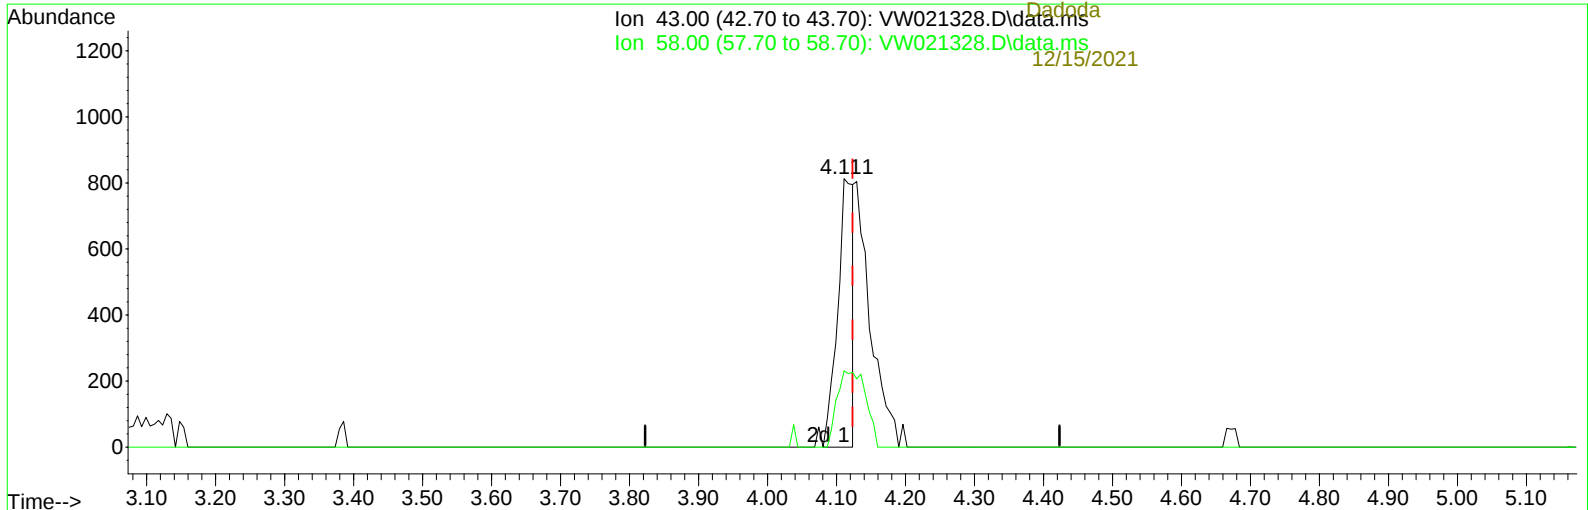

TIC: VW021328.D\data.ms

(13) Acetone (T)

4.111min (-0.012) 6.19 ug/L

response	1285	
Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	35.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121121\
 Data File : VW021328.D
 Acq On : 11 Dec 2021 15:41
 Operator : SY/VA
 Sample : M5062-05
 Misc : 6.80g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGL04

Manual IntegrationsAPPROVED

Quant Time: Dec 12 08:08:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 23:12:45 2021
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

12/13/2021
 Supervised By :Mahesh
 Dadoda

12/15/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	90173	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	88463	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	47918	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	36301	22.104	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.400%
7) Chloroethane-d5	2.879	69	28848	26.571	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.280%
11) 1,1-Dichloroethene-d2	4.032	63	138608	63.307	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	253.240%#
21) 2-Butanone-d5	7.074	46	15070	65.098	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	130.200%
24) Chloroform-d	7.647	84	62271	24.780	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.120%
26) 1,2-Dichloroethane-d4	8.305	65	32830	24.561	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.240%
32) Benzene-d6	8.275	84	112386	23.177	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.720%
36) 1,2-Dichloropropane-d6	9.275	67	32847	25.258	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.040%
41) Toluene-d8	10.323	98	108057	21.810	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.240%
43) trans-1,3-Dichloroprop...	10.579	79	15622	26.090	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	104.360%
47) 2-Hexanone-d5	10.921	63	12161	63.240	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.480%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	29893	26.740	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.960%
66) 1,2-Dichlorobenzene-d4	13.847	152	38636	20.805	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.200%
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	4.038	96	211482	189.207	ug/L #	60
13) Acetone	4.111	43	2589m	12.475	ug/L	
19) 1,1-Dichloroethane	6.214	63	325787	171.549	ug/L	96
30) 1,1,1-Trichloroethane	7.878	97	8162841	4112.558	ug/L #	89
34) Trichloroethene	9.086	95	509236	376.438	ug/L	97
42) Toluene	10.390	91	349122	61.944	ug/L	99
45) 1,1,2-Trichloroethane	10.793	97	5096	5.792	ug/L	88
46) Tetrachloroethene	10.872	164	5335541	4151.898	ug/L	90
53) m,p-Xylene	11.835	106	6698	2.578	ug/L	88
54) o-Xylene	12.164	106	2847	1.155	ug/L	84
57) 1,1,2,2-Tetrachloroethane	12.713	83	1134	1.124	ug/L #	89
63) 1,2,4-Trimethylbenzene	13.249	105	5021	0.919	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

