

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121121\
 Data File : VW021322.D
 Acq On : 11 Dec 2021 13:16
 Operator : SY/VA
 Sample : M5023-08RE
 Misc : 6.47g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGKY4RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/13/2021
 Supervised By :Mahesh Dadoda 12/15/2021

Quant Time: Dec 12 08:07:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 23:12:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	42398	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	37997	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	15597	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	19220	24.891	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	99.560%	
7) Chloroethane-d5	2.879	69	15421	30.209	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	120.840%	
11) 1,1-Dichloroethene-d2	4.013	63	19714	19.150	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	76.600%	
21) 2-Butanone-d5	7.080	46	9356	85.956	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	171.920%#	
24) Chloroform-d	7.647	84	32735	27.705	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	110.840%	
26) 1,2-Dichloroethane-d4	8.305	65	18567	29.542	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	118.160%	
32) Benzene-d6	8.275	84	59226	28.436	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	113.760%	
36) 1,2-Dichloropropane-d6	9.274	67	17556	31.430	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	125.720%#	
41) Toluene-d8	10.323	98	52176	24.518	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	98.080%	
43) trans-1,3-Dichloroprop...	10.579	79	7206	28.018	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	112.080%	
47) 2-Hexanone-d5	10.921	63	6461	78.223	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	156.440%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	15881	33.074	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	132.280%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	15058	24.911	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	99.640%	
Target Compounds						
13) Acetone	4.135	43	847m	8.680	ug/L	
16) Methylene chloride	4.915	84	3639	5.194	ug/L	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121121\
Data File : VW021322.D
Acq On : 11 Dec 2021 13:16
Operator : SY/VA
Sample : M5023-08RE
Misc : 6.47g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BGKY4RE

Quant Time: Dec 12 08:07:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 10 23:12:45 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 12/13/2021
Supervised By :Mahesh Dadoda 12/15/2021

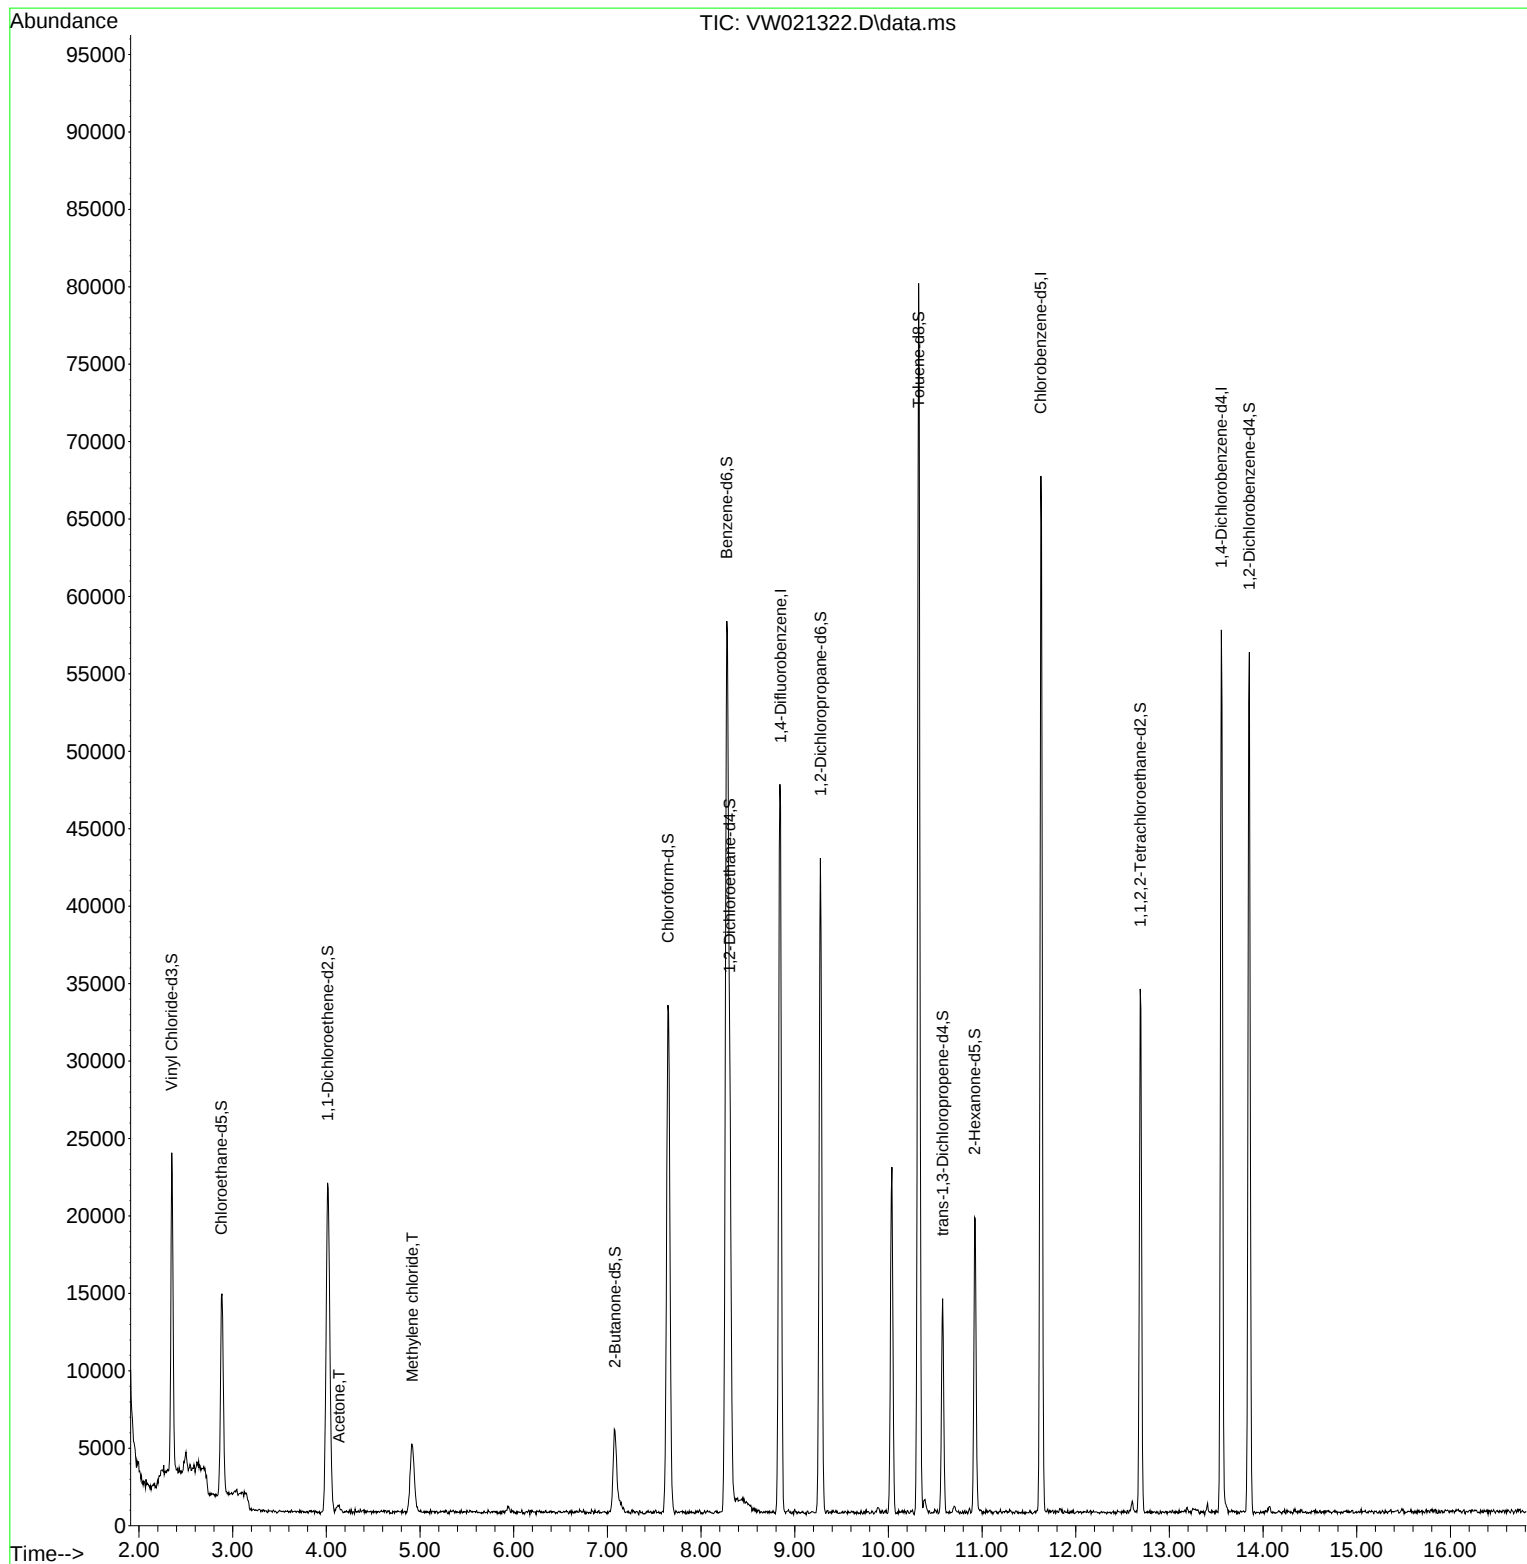

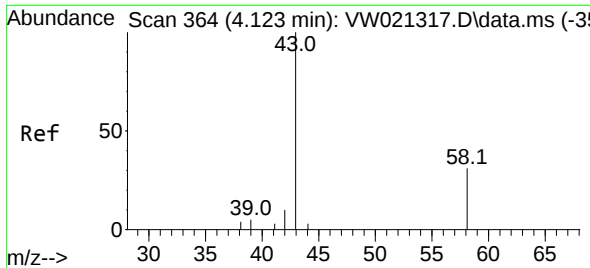

#13

Acetone

Concen: 8.680 ug/L m

RT: 4.135 min Scan# 3

Delta R.T. 0.012 min

Lab File: VW021322.D

Acq: 11 Dec 2021 13:16

Instrument :

MSVOA_W

ClientSampleId :





BGKY4RE

Tgt Ion: 43 Resp: 84
 Ion Ratio Lower Upper
 43 100
 58 15.6 0.0 52.8

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 12/13/2021
 Supervised By :Mahesh Dadoda 12/15/2021

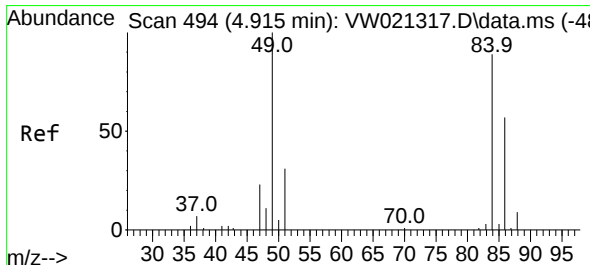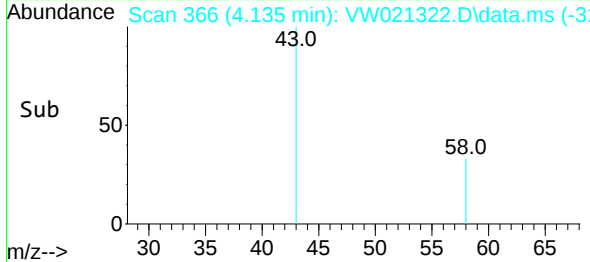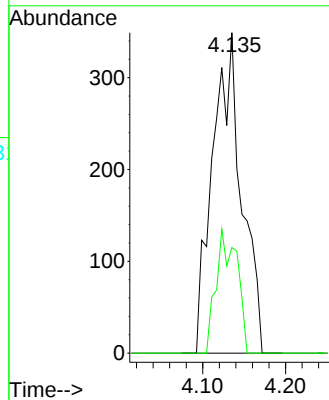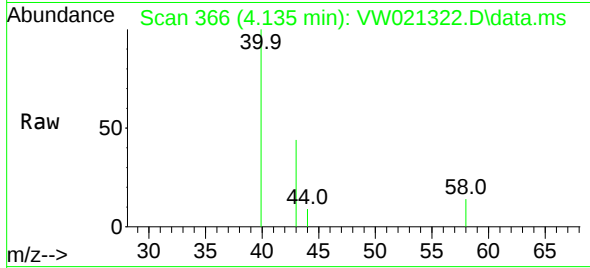

#16

Methylene chloride

Concen: 5.194 ug/L

RT: 4.915 min Scan# 494

Delta R.T. -0.000 min

Lab File: VW021322.D

Acq: 11 Dec 2021 13:16

Tgt Ion: 84 Resp: 3639
 Ion Ratio Lower Upper
 84 100
 86 71.3 45.5 84.5
 49 111.3 100.5 186.7

