
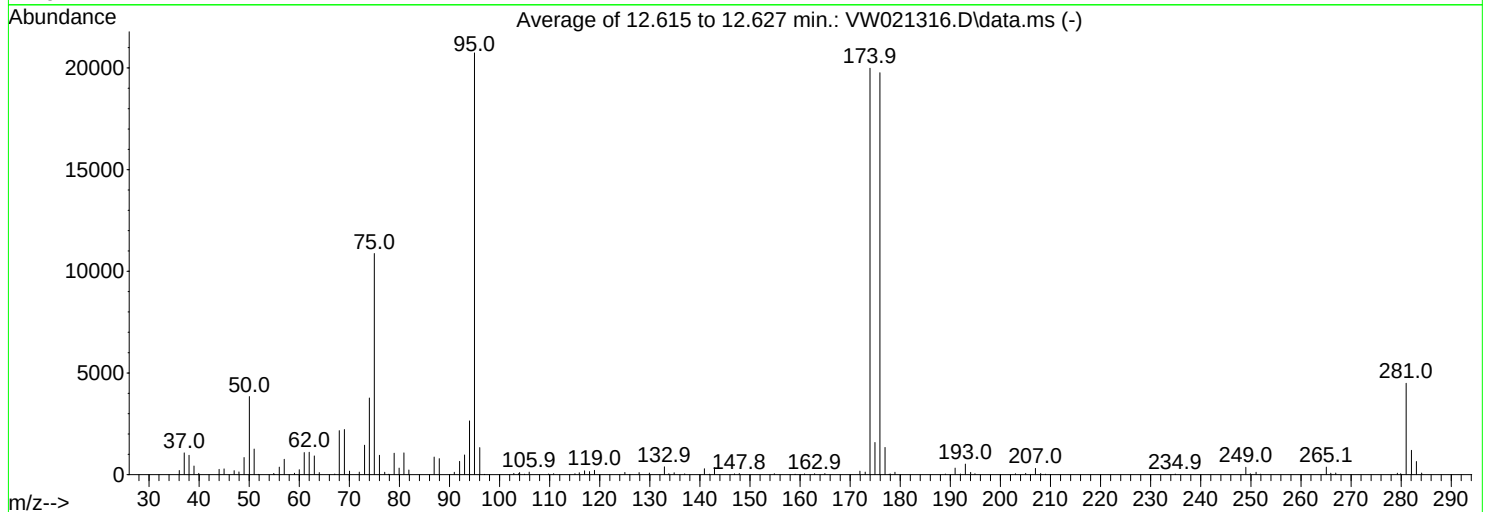


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121121\
 Data File : VW021316.D
 Acq On : 11 Dec 2021 08:46
 Operator : SY/VA
 Sample : BFB477
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB477

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Title : SFAM01.0
 Last Update : Fri Dec 17 00:58:26 2021

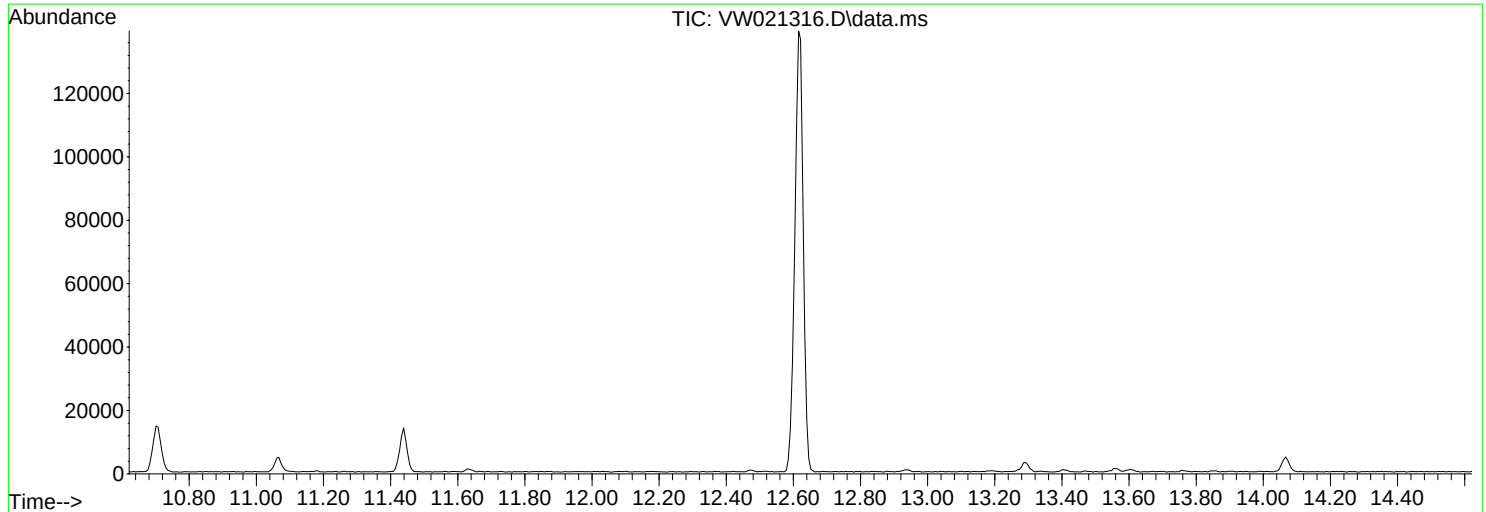

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	3840	PASS
75	95	30	80	52.4	10872	PASS
95	95	100	100	100.0	20744	PASS
96	95	5	9	6.4	1331	PASS
173	174	0.00	2	0.6	129	PASS
174	95	50	120	96.3	19984	PASS
175	174	5	9	7.9	1581	PASS
176	174	95	105	98.9	19768	PASS
177	176	5	10	6.8	1341	PASS

Scan 1750 (12.573 min): VW021316.D\data.ms
BFB477

m/z	Abundance
40.00	627.0
281.00	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

m/z	Abundance
36.00	208.0
37.10	1236.0
38.00	1149.0
39.00	526.0
39.90	740.0
44.00	341.0
45.00	332.0
47.10	197.0
48.00	149.0
49.00	1007.0
50.00	4616.0
51.00	1532.0
51.90	58.0
54.90	72.0
56.00	414.0
57.00	825.0
59.00	137.0
60.10	307.0
61.00	1365.0
62.00	1241.0
63.00	1023.0
64.00	123.0
67.10	105.0
68.00	2594.0
69.00	2540.0
70.10	190.0
72.00	191.0
73.10	1879.0
74.00	4307.0
75.00	12423.0
76.00	1082.0
77.00	159.0
78.90	1191.0
80.00	355.0
80.90	1243.0
81.90	237.0
86.90	1023.0
88.00	806.0
90.90	106.0
92.00	796.0
93.00	1102.0
94.00	3011.0
95.00	22872.0
96.00	1473.0
102.90	123.0
103.80	150.0
105.00	77.0
105.90	138.0
109.80	88.0
110.80	84.0
115.00	85.0
116.00	109.0
116.90	184.0
118.00	196.0
119.00	223.0
125.00	219.0
126.00	58.0
127.80	86.0
129.90	80.0
132.90	701.0
134.80	122.0
136.90	58.0
140.90	322.0
142.90	341.0
146.90	69.0
147.90	62.0
159.00	65.0
160.90	107.0
162.90	134.0
165.00	112.0
172.00	193.0
173.90	20944.0
175.00	1606.0
176.00	18528.0
176.90	1561.0
177.80	81.0
179.00	259.0
189.00	101.0
191.00	444.0
193.00	937.0
194.00	186.0
194.90	152.0
203.00	89.0
205.00	146.0
207.00	524.0
208.00	99.0
209.00	64.0
234.90	104.0
249.00	680.0
249.90	150.0
251.00	237.0
251.90	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

265.10	603.0
266.00	114.0
267.00	113.0
279.30	145.0
281.00	7037.0
282.10	2065.0
283.10	1017.0
284.10	173.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

m/z	Abundance
36.10	249.0
37.00	1205.0
38.00	1061.0
39.00	419.0
39.90	673.0
44.00	246.0
45.00	333.0
46.90	245.0
48.00	146.0
49.00	984.0
50.10	4090.0
51.00	1375.0
55.10	80.0
56.10	457.0
57.00	888.0
59.10	75.0
59.90	279.0
61.00	1086.0
62.00	1228.0
63.00	1089.0
64.00	119.0
68.00	2438.0
69.00	2502.0
70.00	217.0
72.00	107.0
73.00	1617.0
74.00	4231.0
75.00	12209.0
76.00	1045.0
77.10	129.0
77.90	76.0
79.00	1174.0
79.90	357.0
80.90	1217.0
81.90	263.0
87.00	911.0
87.90	997.0
91.00	176.0
91.90	647.0
93.00	1057.0
94.00	2912.0
95.00	23200.0
96.10	1554.0
97.00	52.0
102.80	66.0
104.00	216.0
105.90	135.0
110.80	62.0
115.10	52.0
115.90	112.0
117.00	194.0
117.90	162.0
118.90	208.0
125.00	124.0
127.90	117.0
129.90	151.0
132.90	332.0
133.80	153.0
134.80	89.0
137.00	52.0
140.90	320.0
141.90	59.0
142.90	377.0
146.90	51.0
147.80	56.0
154.90	102.0
164.90	58.0
171.90	163.0
174.00	21624.0
174.90	1963.0
175.90	23368.0
176.90	1414.0
178.00	83.0
178.90	87.0
190.90	362.0
192.00	92.0
193.00	464.0
194.10	142.0
203.00	55.0
205.10	54.0
206.00	53.0
207.00	276.0
208.10	59.0
249.00	317.0
251.10	128.0
265.00	344.0
265.90	98.0
266.90	118.0
279.20	69.0
279.90	145.0
281.10	5046.0
282.00	1141.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

283.00665.0

284.1074.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

m/z	Abundance
36.00	148.0
37.10	772.0
38.10	655.0
39.00	328.0
40.00	648.0
44.00	199.0
45.00	194.0
47.00	158.0
47.90	110.0
49.00	538.0
50.00	2813.0
51.00	865.0
54.90	85.0
55.90	238.0
57.10	560.0
60.00	156.0
61.00	807.0
62.00	835.0
63.00	648.0
64.00	59.0
68.00	1468.0
69.10	1615.0
70.00	125.0
71.90	92.0
73.00	857.0
74.00	2778.0
75.00	7983.0
76.00	724.0
77.00	75.0
78.90	807.0
79.90	250.0
81.00	756.0
81.90	180.0
86.90	655.0
87.90	563.0
90.90	76.0
92.10	524.0
93.00	746.0
94.00	2012.0
95.00	16161.0
96.00	966.0
104.00	102.0
105.90	108.0
115.80	69.0
116.90	194.0
117.90	100.0
118.90	208.0
127.90	104.0
132.80	127.0
134.90	82.0
140.90	240.0
142.90	294.0
147.80	54.0
154.80	52.0
172.00	156.0
173.00	388.0
173.90	17384.0
174.90	1174.0
175.90	17408.0
177.00	1048.0
191.00	157.0
193.00	150.0
207.00	122.0
249.00	100.0
264.90	155.0
281.10	1561.0
282.10	379.0
283.00	256.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477