

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
 Data File : VW031215.D
 Acq On : 11 Dec 2024 15:40
 Operator : SY/MD
 Sample : P5155-09
 Misc : 4.43g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 12 03:04:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 12 03:01:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	64490	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117	50833	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	11458	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	18909	19.053	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.200%
7) Chloroethane-d5	2.893	69	17340	22.520	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.080%
11) 1,1-Dichloroethene-d2	4.027	65	7550	16.674	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.680%
21) 2-Butanone-d5	7.081	46	2995	17.256	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	34.520%
24) Chloroform-d	7.648	84	43526	23.044	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.160%
26) 1,2-Dichloroethane-d4	8.075	65	85	0.091	ug/L	-0.23
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.360%#
32) Benzene-d6	8.270	84	58166	18.617	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.480%
36) 1,2-Dichloropropane-d6	9.276	67	24661	26.947	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.800%
41) Toluene-d8	10.325	98	40692	14.432	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	57.720%
43) trans-1,3-Dichloroprop...	10.581	79	5721	15.527	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	62.120%
47) 2-Hexanone-d5	10.873	63	51	0.476	ug/L	-0.05
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.960%#
56) 1,1,2,2-Tetrachloroeth...	12.684	84	18543	30.022	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	120.080%#
66) 1,2-Dichlorobenzene-d4	13.855	152	8618	21.176	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.720%
Target Compounds						Qvalue
15) Methyl Acetate	4.686	43	332	1.013	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
Data File : VW031215.D
Acq On : 11 Dec 2024 15:40
Operator : SY/MD
Sample : P5155-09
Misc : 4.43g/10mL/MSVOA_W/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 12 03:04:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 12 03:01:22 2024
Response via : Initial Calibration

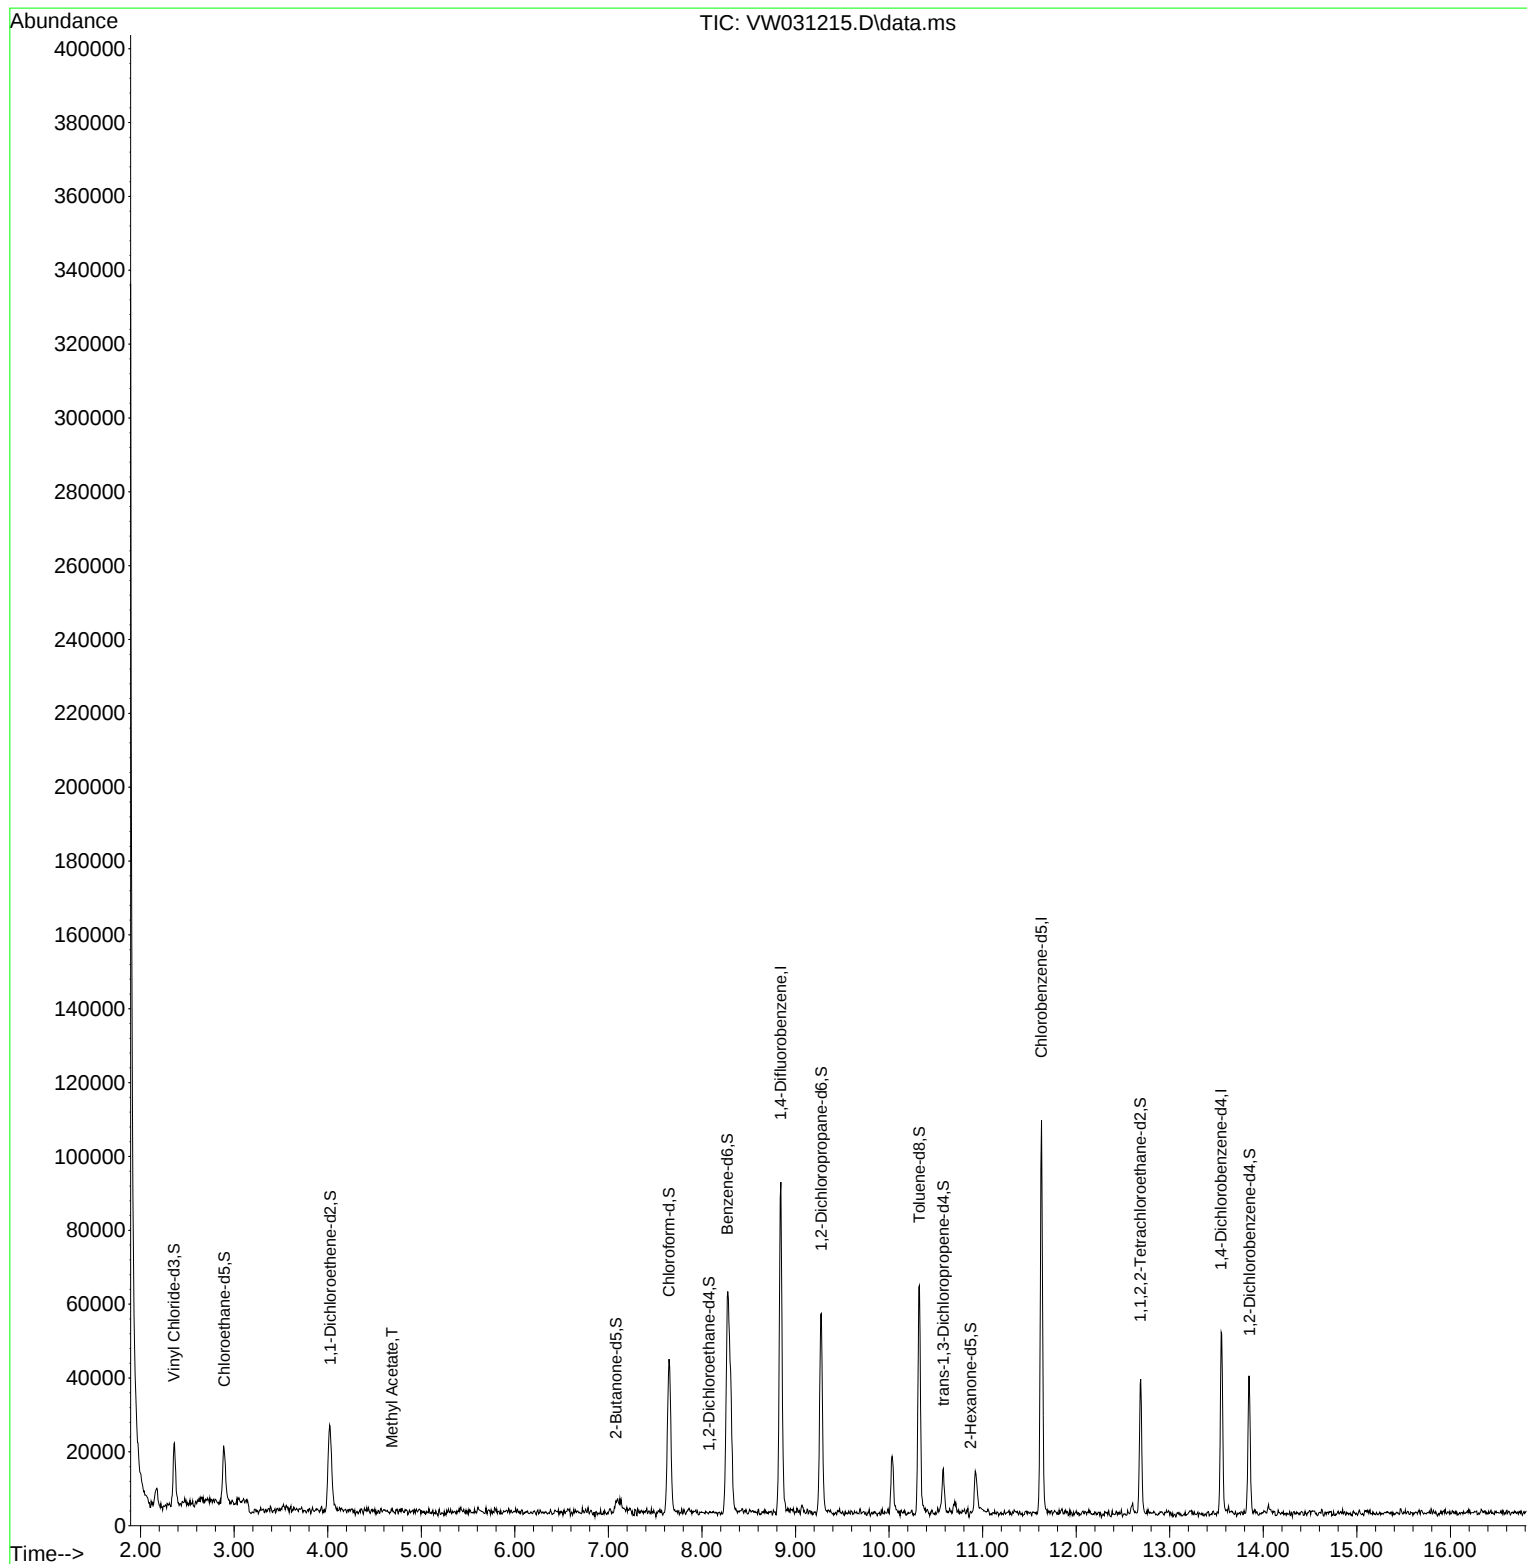

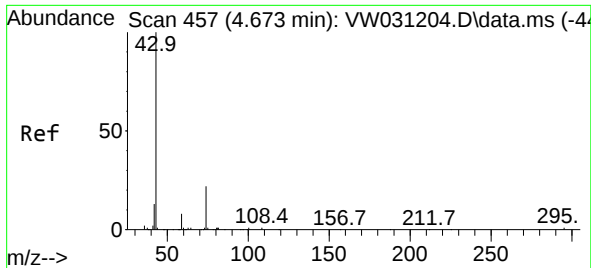

#15

Methyl Acetate

Concen: 1.013 ug/L

RT: 4.686 min Scan# 4

Delta R.T. 0.012 min


Lab File: VW031215.D

Acq: 11 Dec 2024 15:40

Instrument :

MSVOA_W

ClientSampleId :

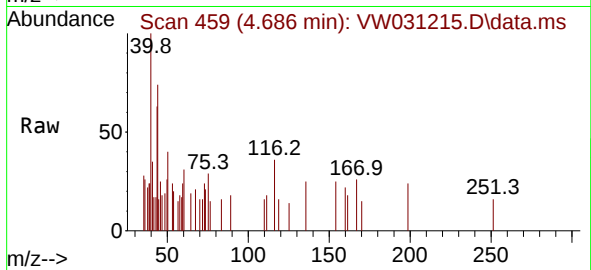

Tgt Ion: 43 Resp: 332

Ion Ratio Lower Upper

43 100

74 10.2 20.8 31.2#

