

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
 Data File : VW031222.D
 Acq On : 11 Dec 2024 18:27
 Operator : SY/MD
 Sample : P5155-15
 Misc : 4.50g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 12 03:06:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 12 03:01:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	486090	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117	318837	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	65118	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	93471	12.495	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.000%
7) Chloroethane-d5	2.905	69	81592	14.059	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.240%
11) 1,1-Dichloroethene-d2	4.021	65	39284	11.511	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.040%
21) 2-Butanone-d5	6.990	46	65	0.050	ug/L	-0.10
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.100%#
24) Chloroform-d	7.648	84	244138	17.148	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	68.600%
26) 1,2-Dichloroethane-d4	8.307	65	124577	17.783	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	71.120%
32) Benzene-d6	8.276	84	341568	17.430	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	69.720%
36) 1,2-Dichloropropane-d6	9.270	67	142458	24.818	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.280%
41) Toluene-d8	10.319	98	242362	13.705	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	54.800%
43) trans-1,3-Dichloroprop...	10.575	79	25172	10.892	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	43.560%
47) 2-Hexanone-d5	10.928	63	8006	11.904	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	23.800%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	85219	21.998	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.000%
66) 1,2-Dichlorobenzene-d4	13.849	152	42057	18.183	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	72.720%#
Target Compounds					Qvalue	
48) 2-Hexanone	10.947	43	5992	2.758	ug/L	# 35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
Data File : VW031222.D
Acq On : 11 Dec 2024 18:27
Operator : SY/MD
Sample : P5155-15
Misc : 4.50g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 12 03:06:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 12 03:01:22 2024
Response via : Initial Calibration

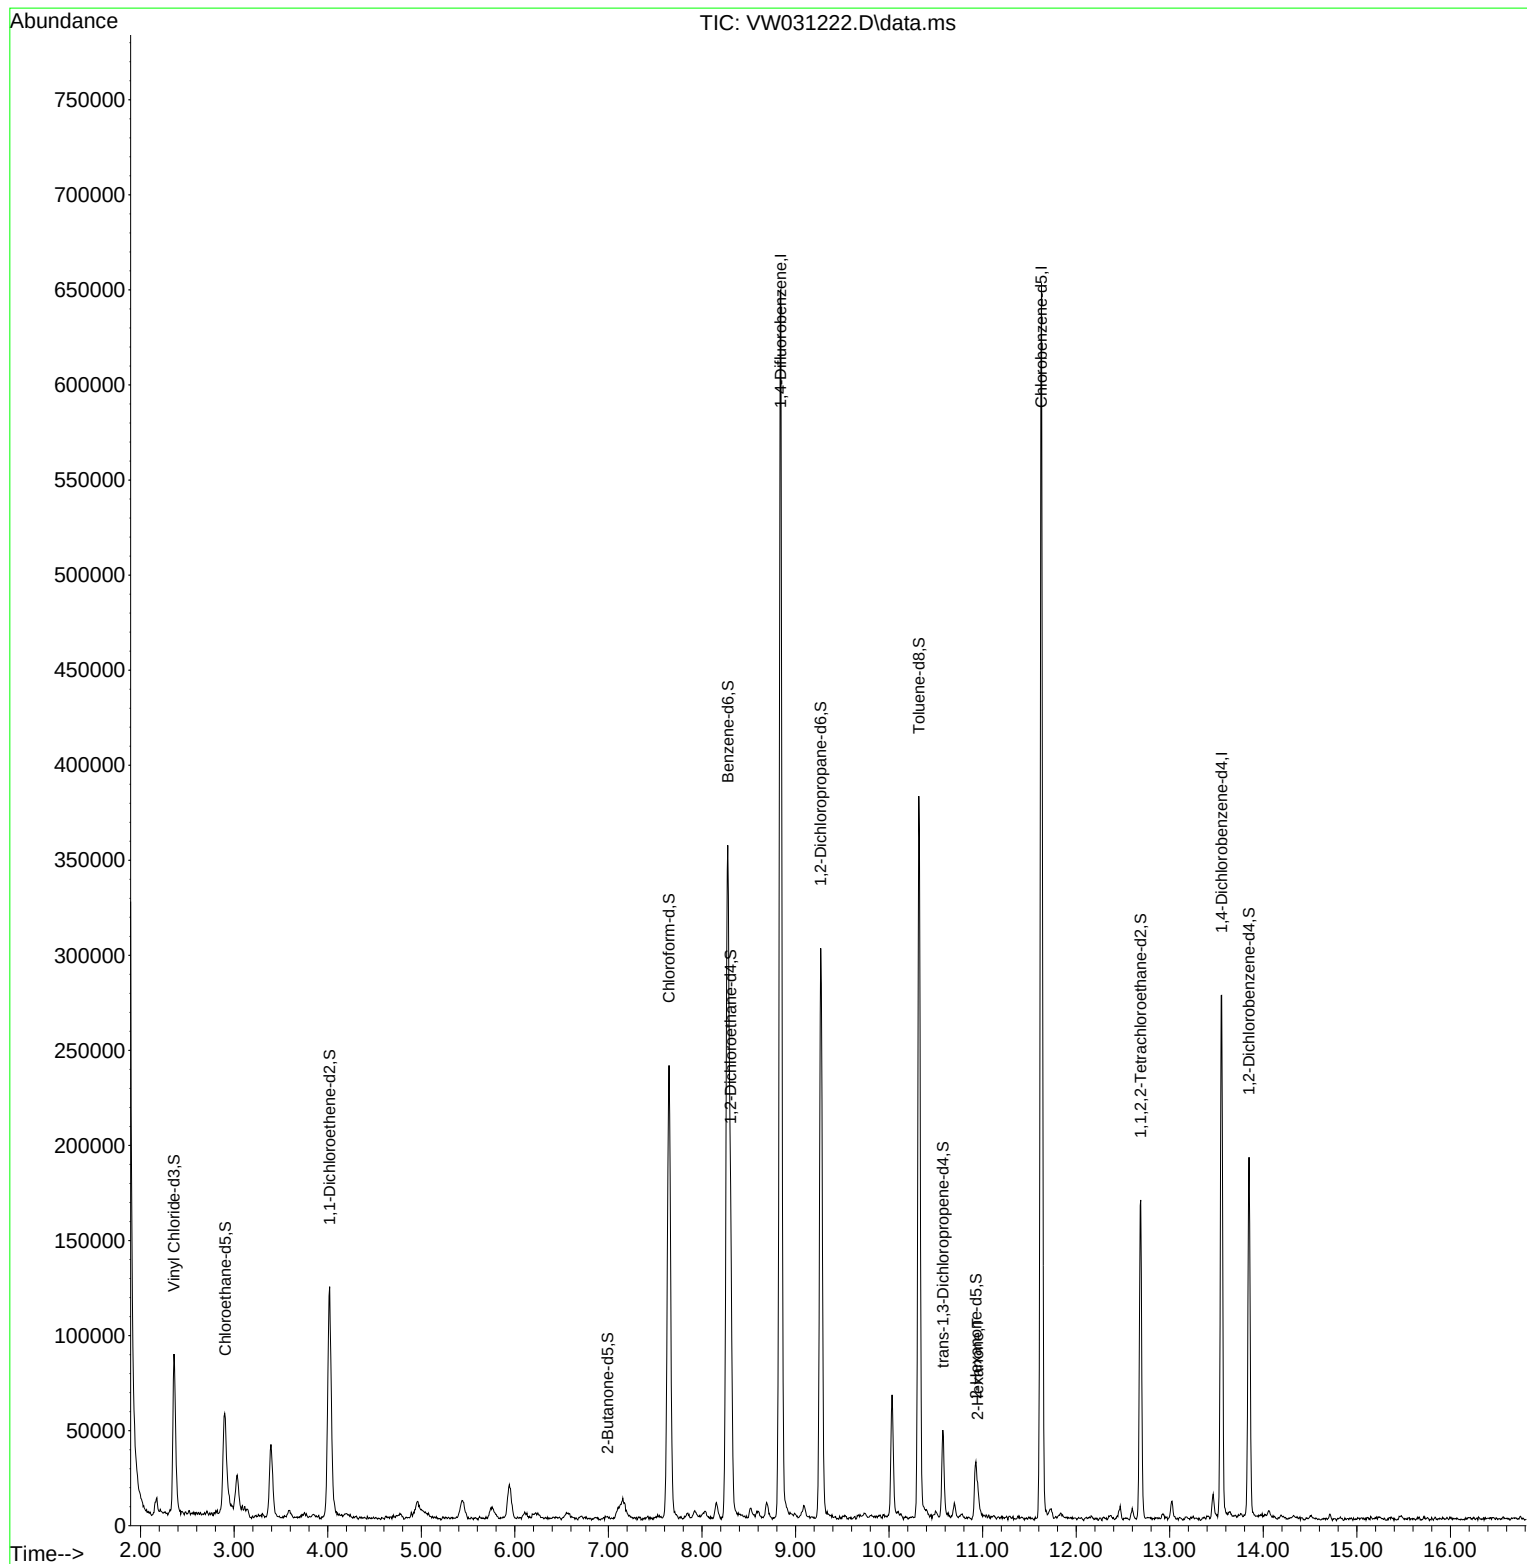

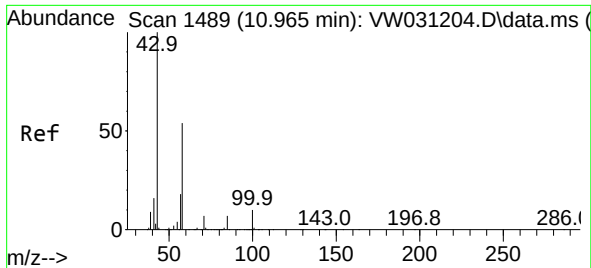

#48
2-Hexanone
Concen: 2.758 ug/L
RT: 10.947 min Scan# 1486
Delta R.T. -0.018 min
Lab File: VW031222.D
Acq: 11 Dec 2024 18:27

Instrument :
MSVOA_W
ClientSampleId :

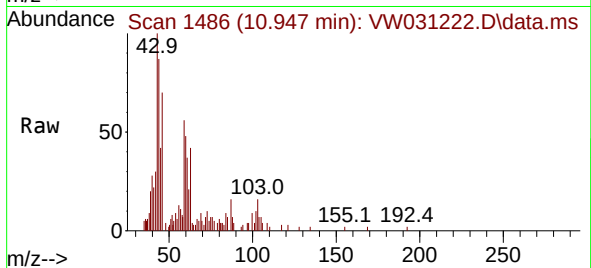

Tgt Ion:	43	Resp:	5992
Ion	Ratio	Lower	Upper
43	100		
58	0.0	49.8	74.6#
57	0.0	16.6	24.8#
100	3.0	11.4	17.2#

