




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
 Data File : VW031211.D
 Acq On : 11 Dec 2024 14:05
 Operator : SY/MD
 Sample : P5153-16
 Misc : 8.66g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28Q3

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:03:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 12 03:01:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/12/2024
 Supervised By :Mahesh Dadoda 12/13/2024

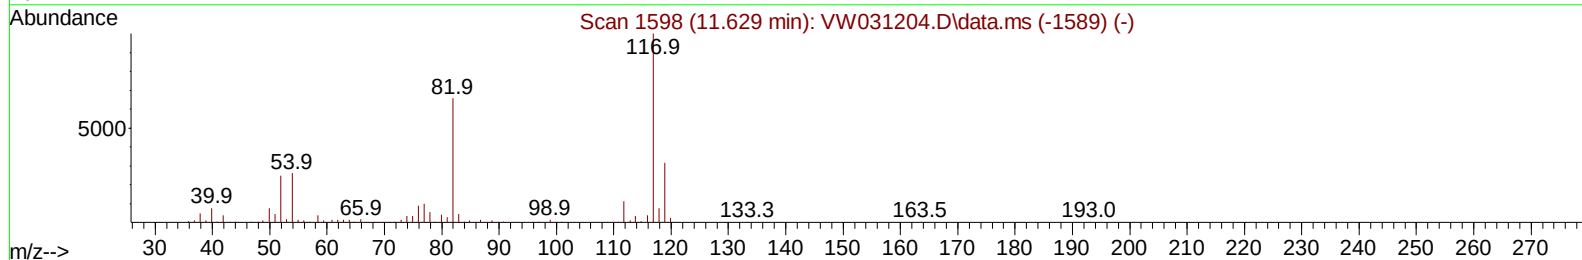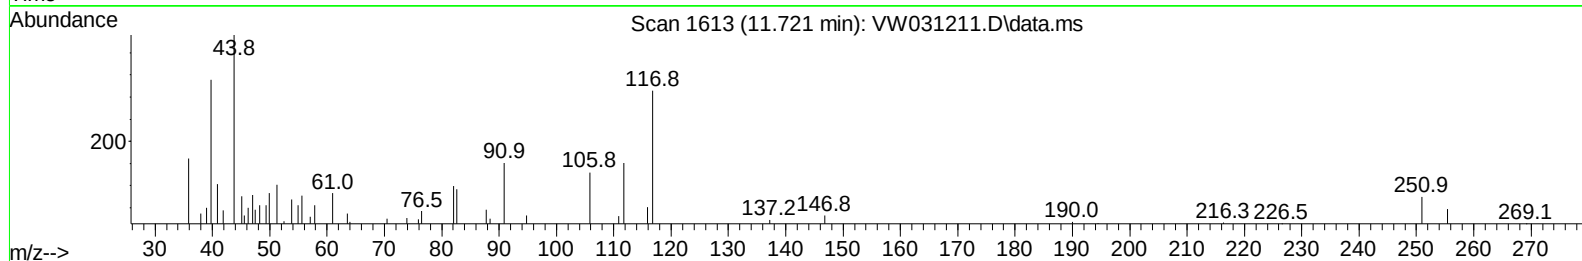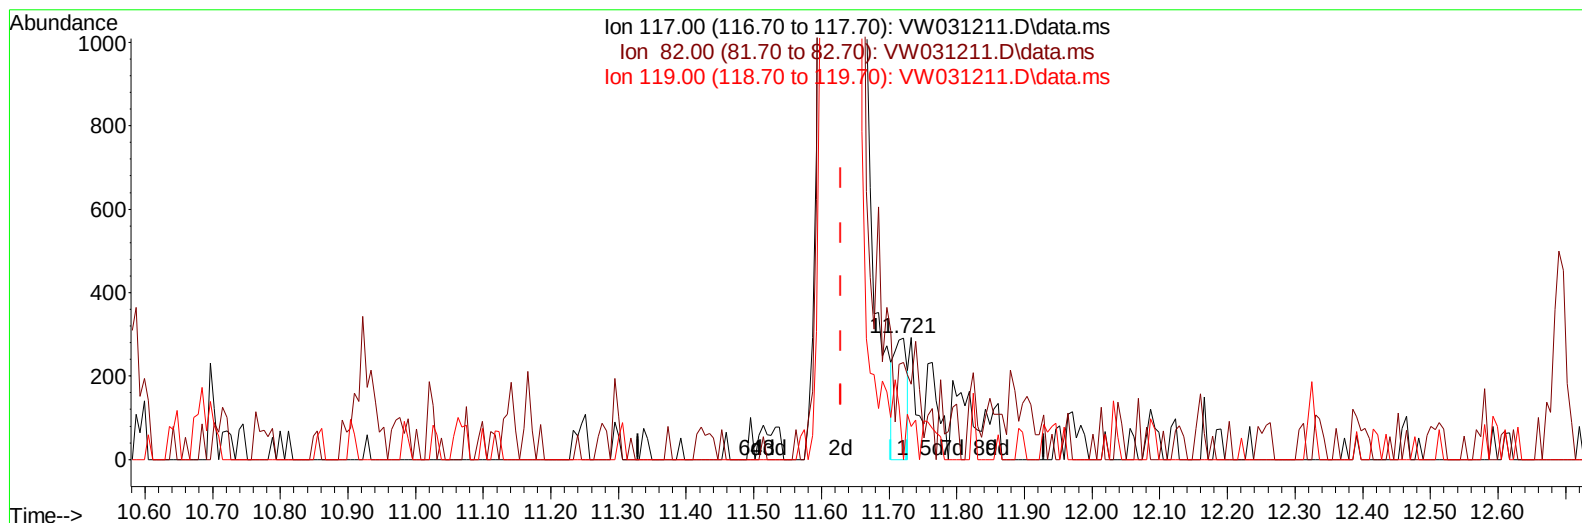

TIC: VW031211.D\data.ms

(28) Chlorobenzene-d5 (I)

11.721min (+ 0.091) 25.00 ug/L

response 384

Ion	Exp%	Act%
117.00	100.00	100.00
82.00	55.10	64.32
119.00	31.90	27.08
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
Data File : VW031211.D
Acq On : 11 Dec 2024 14:05
Operator : SY/MD
Sample : P5153-16
Misc : 8.66g/10mL/MSVOA_W/SOIL/B
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Q3

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:03:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 12 03:01:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 12/12/2024
Supervised By :Mahesh Dadoda 12/13/2024

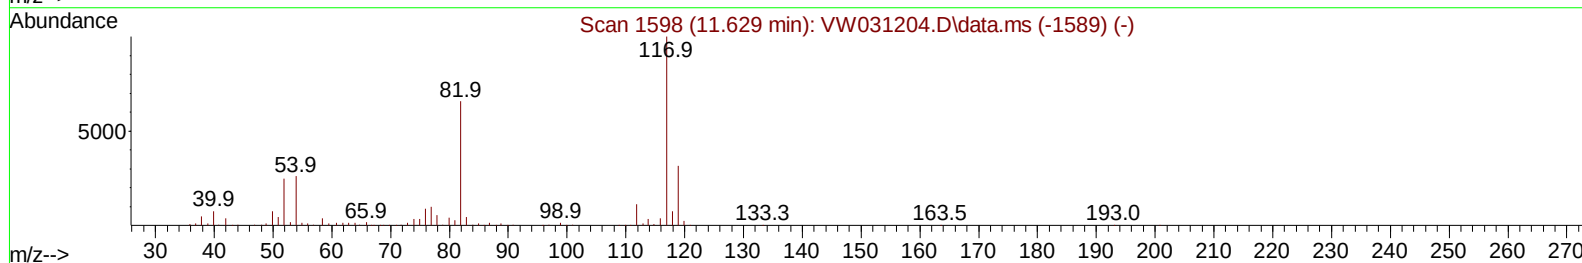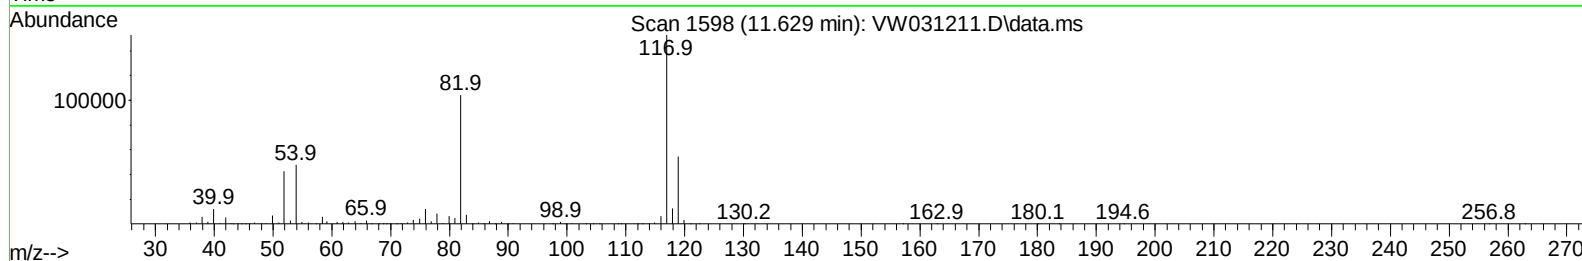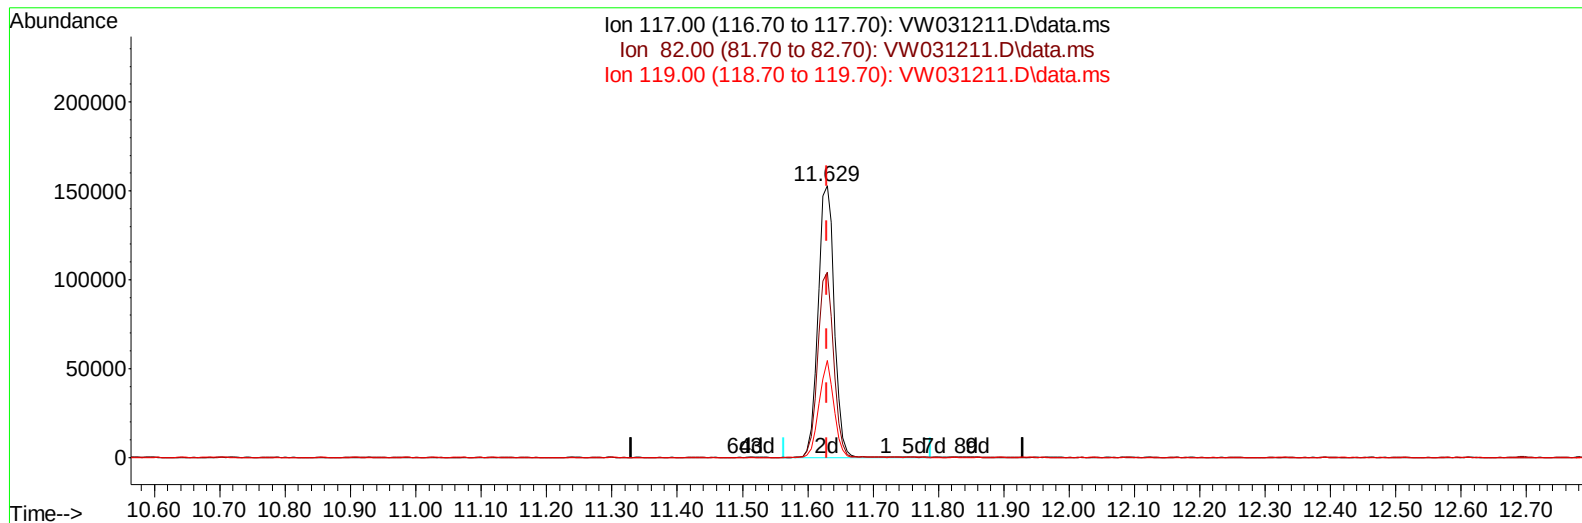

TIC: VW031211.D\data.ms

(28) Chlorobenzene-d5 (I)

11.629min (+ 0.000) 25.00 ug/L m

response 262253

Ion	Exp%	Act%
117.00	100.00	100.00
82.00	55.10	0.09#
119.00	31.90	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121124\
 Data File : VW031211.D
 Acq On : 11 Dec 2024 14:05
 Operator : SY/MD
 Sample : P5153-16
 Misc : 8.66g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28Q3

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:03:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 12 03:01:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/12/2024
 Supervised By :Mahesh Dadoda 12/13/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		278513	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117		262253m	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		107428	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		89078	20.783	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.120%	
7) Chloroethane-d5	2.899	69		77134	23.196	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	92.800%	
11) 1,1-Dichloroethene-d2	4.015	65		40715	20.821	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	83.280%	
21) 2-Butanone-d5	7.094	46		49116	65.525	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	131.060%	
24) Chloroform-d	7.648	84		219751	26.939	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	107.760%	
26) 1,2-Dichloroethane-d4	8.307	65		128938	32.122	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	128.480%	
32) Benzene-d6	8.270	84		351464	21.805	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	87.200%	
36) 1,2-Dichloropropane-d6	9.270	67		132862	28.140	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	112.560%	
41) Toluene-d8	10.319	98		309359	21.267	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	85.080%	
43) trans-1,3-Dichloroprop...	10.575	79		49590	26.088	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	104.360%	
47) 2-Hexanone-d5	10.922	63		33285	60.172	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	120.340%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		105251	33.031	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	132.120%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		103286	27.068	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	108.280%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
Data File : VW031211.D
Acq On : 11 Dec 2024 14:05
Operator : SY/MD
Sample : P5153-16
Misc : 8.66g/10mL/MSVOA_W/SOIL/B
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Q3

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:03:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 12 03:01:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 12/12/2024
Supervised By :Mahesh Dadoda 12/13/2024

