




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
Data File : VW031214.D
Acq On : 11 Dec 2024 15:16
Operator : SY/MD
Sample : P5155-10
Misc : 4.60g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28T5

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:04:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 12 03:01:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 12/12/2024
Supervised By :Mahesh Dadoda 12/13/2024

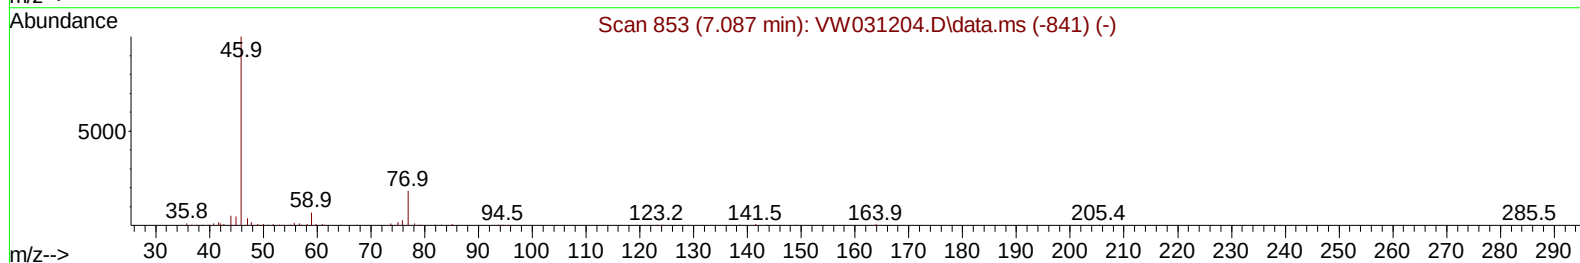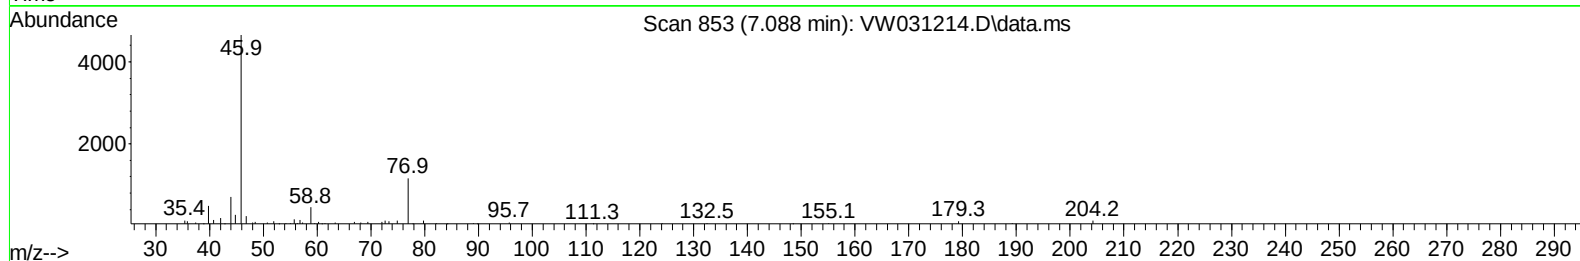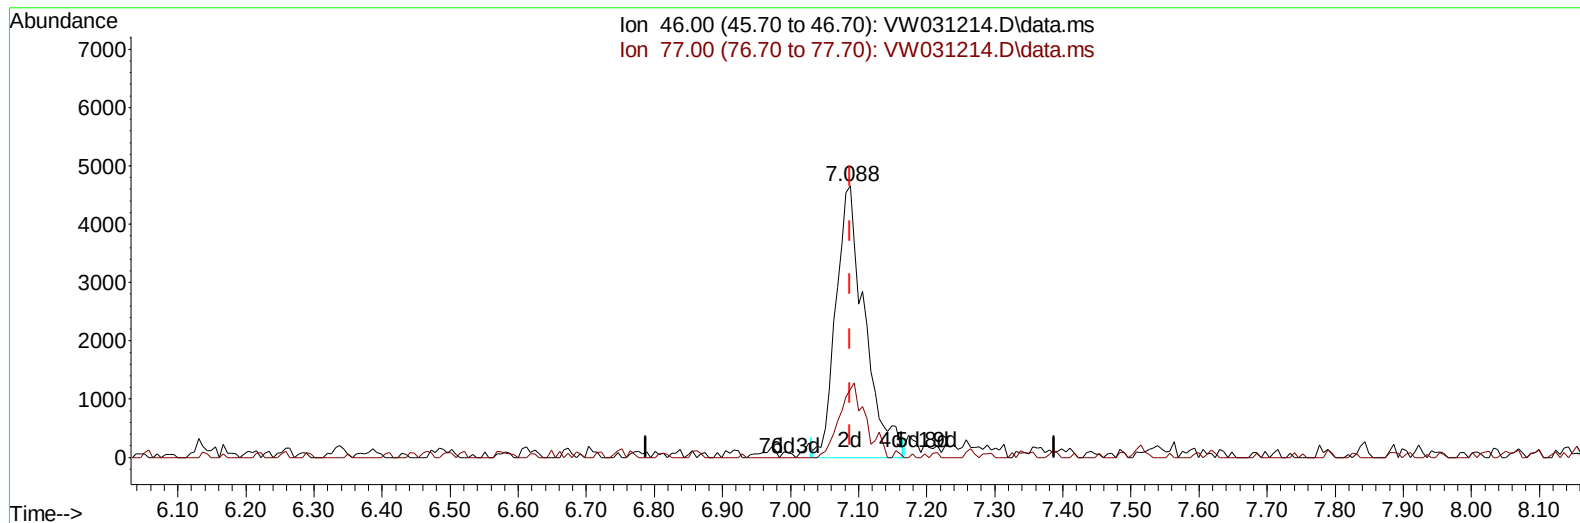

TIC: VW031214.D\data.ms

(21) 2-Butanone-d5 (S)

7.088min (+ 0.000) 34.09 ug/L m

response 13644

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	27.80	0.17#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121124\
 Data File : VW031214.D
 Acq On : 11 Dec 2024 15:16
 Operator : SY/MD
 Sample : P5155-10
 Misc : 4.60g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28T5

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:04:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 12 03:01:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/12/2024
 Supervised By :Mahesh Dadoda 12/13/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		148722	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117		111914	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		22607	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		41098	17.957	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	71.840%		
7) Chloroethane-d5	2.893	69		35264	19.860	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.440%		
11) 1,1-Dichloroethene-d2	4.015	65		16083	15.402	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	61.600%		
21) 2-Butanone-d5	7.088	46		13644m	34.088	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	68.180%		
24) Chloroform-d	7.648	84		79654	18.287	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	73.160%		
26) 1,2-Dichloroethane-d4	8.307	65		45262	21.117	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	84.480%		
32) Benzene-d6	8.276	84		118284	17.196	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	68.800%		
36) 1,2-Dichloropropane-d6	9.270	67		46003	22.832	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	91.320%		
41) Toluene-d8	10.319	98		83670	13.479	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	53.920%		
43) trans-1,3-Dichloroprop...	10.575	79		11531	14.215	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	56.880%		
47) 2-Hexanone-d5	10.922	63		6589	27.912	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	55.820%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		32212	23.689	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	94.760%		
66) 1,2-Dichlorobenzene-d4	13.849	152		14269	17.770	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	71.080%#		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
Data File : VW031214.D
Acq On : 11 Dec 2024 15:16
Operator : SY/MD
Sample : P5155-10
Misc : 4.60g/10mL/MSVOA_W/SoIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28T5

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 12/12/2024
Supervised By :Mahesh Dadoda 12/13/2024

Quant Time: Dec 12 03:04:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 12 03:01:22 2024
Response via : Initial Calibration

