




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
 Data File : VW031217.D
 Acq On : 11 Dec 2024 16:28
 Operator : SY/MD
 Sample : P5153-13RE
 Misc : 8.29g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28Q0RE

Manual IntegrationsAPPROVED

Quant Time: Dec 12 07:25:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 12 03:01:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/12/2024
 Supervised By :Mahesh Dadoda 12/13/2024

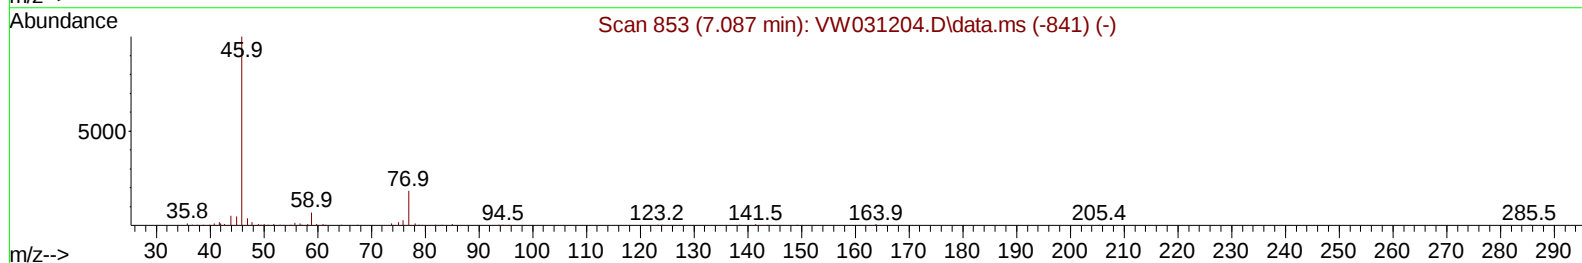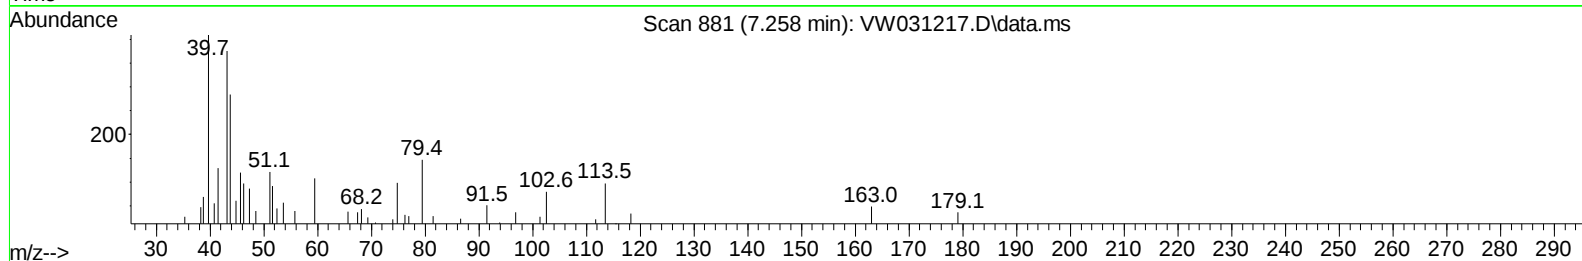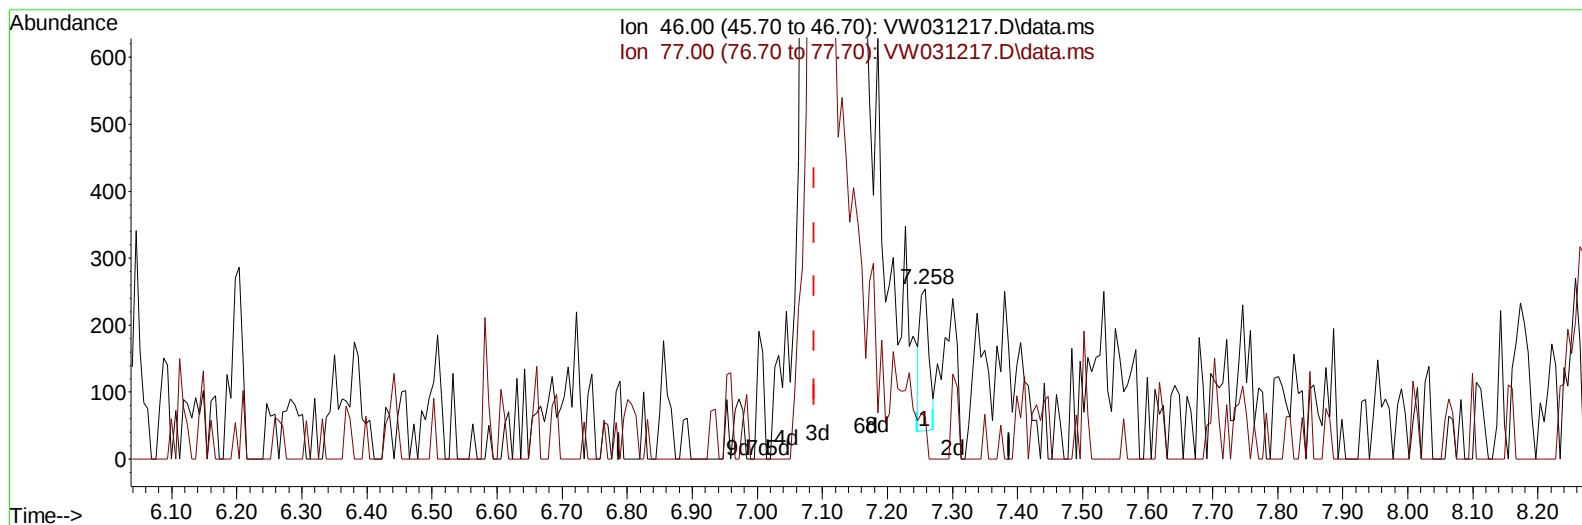

TIC: VW031217.D\data.ms

(21) 2-Butanone-d5 (S)

7.258min (+ 0.171) 0.28 ug/L

response 208

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	27.80	23.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
Data File : VW031217.D
Acq On : 11 Dec 2024 16:28
Operator : SY/MD
Sample : P5153-13RE
Misc : 8.29g/10mL/MSVOA_W/SOIL/B
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Q0RE

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:05:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 12 03:01:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 12/12/2024
Supervised By :Mahesh Dadoda 12/13/2024

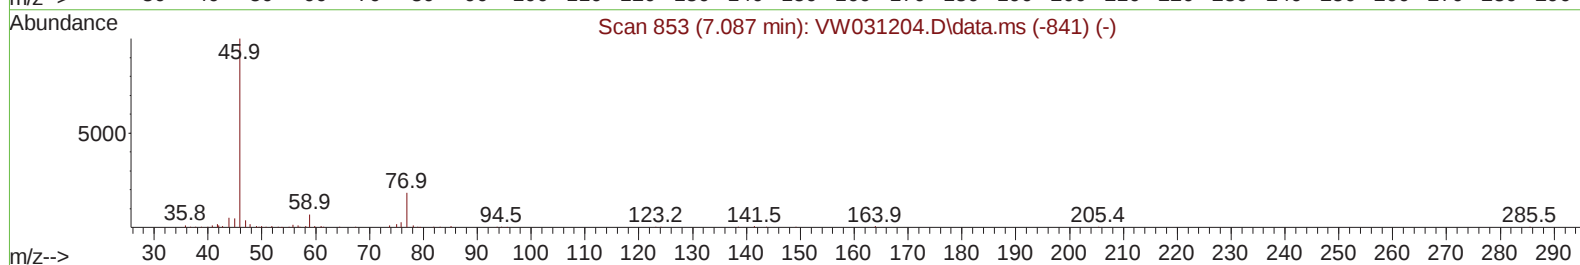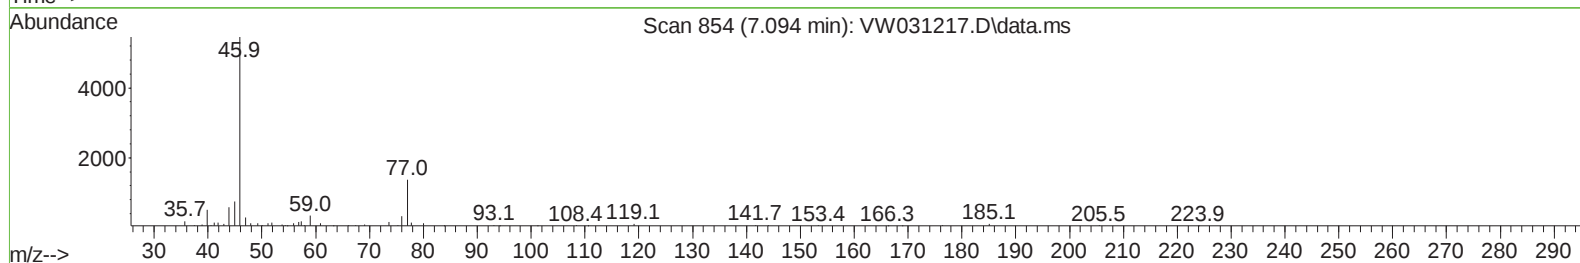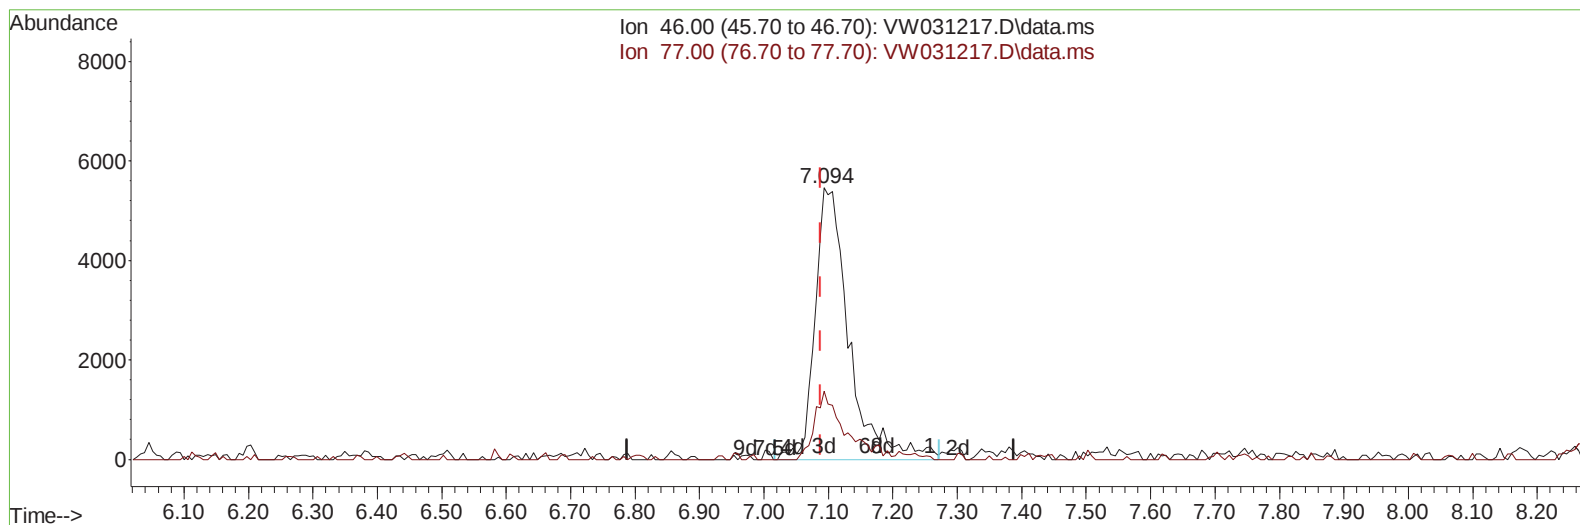

TIC: VW031217.D\data.ms

(21) 2-Butanone-d5 (S)

7.094min (+ 0.006) 26.54 ug/L m

response 20019

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	27.80	0.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
 Data File : VW031217.D
 Acq On : 11 Dec 2024 16:28
 Operator : SY/MD
 Sample : P5153-13RE
 Misc : 8.29g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28Q0RE

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:05:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 12 03:01:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/12/2024
 Supervised By :Mahesh Dadoda 12/13/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	280253	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.623	117	164562	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	28193	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	82409	19.108	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	76.440%	
7) Chloroethane-d5	2.893	69	71206	21.281	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	85.120%	
11) 1,1-Dichloroethene-d2	4.015	65	34072	17.316	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	69.280%	
21) 2-Butanone-d5	7.094	46	20019m	26.541	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	53.080%	
24) Chloroform-d	7.648	84	176691	21.526	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	86.120%	
26) 1,2-Dichloroethane-d4	8.301	65	94534	23.405	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	93.640%	
32) Benzene-d6	8.270	84	258322	25.540	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	102.160%	
36) 1,2-Dichloropropane-d6	9.270	67	101419	34.232	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	136.920%#	
41) Toluene-d8	10.319	98	165337	18.114	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	72.440%	
43) trans-1,3-Dichloroprop...	10.581	79	20595	17.266	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	69.080%	
47) 2-Hexanone-d5	10.922	63	9439	27.193	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	54.380%	
56) 1,1,2,2-Tetrachloroeth...	12.684	84	50802	25.408	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	101.640%	
66) 1,2-Dichlorobenzene-d4	13.848	152	17804	17.779	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	71.120%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121124\
Data File : VW031217.D
Acq On : 11 Dec 2024 16:28
Operator : SY/MD
Sample : P5153-13RE
Misc : 8.29g/10mL/MSVOA_W/SOIL/B
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Q0RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 12/12/2024
Supervised By :Mahesh Dadoda 12/13/2024

Quant Time: Dec 12 03:05:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 12 03:01:22 2024
Response via : Initial Calibration

