
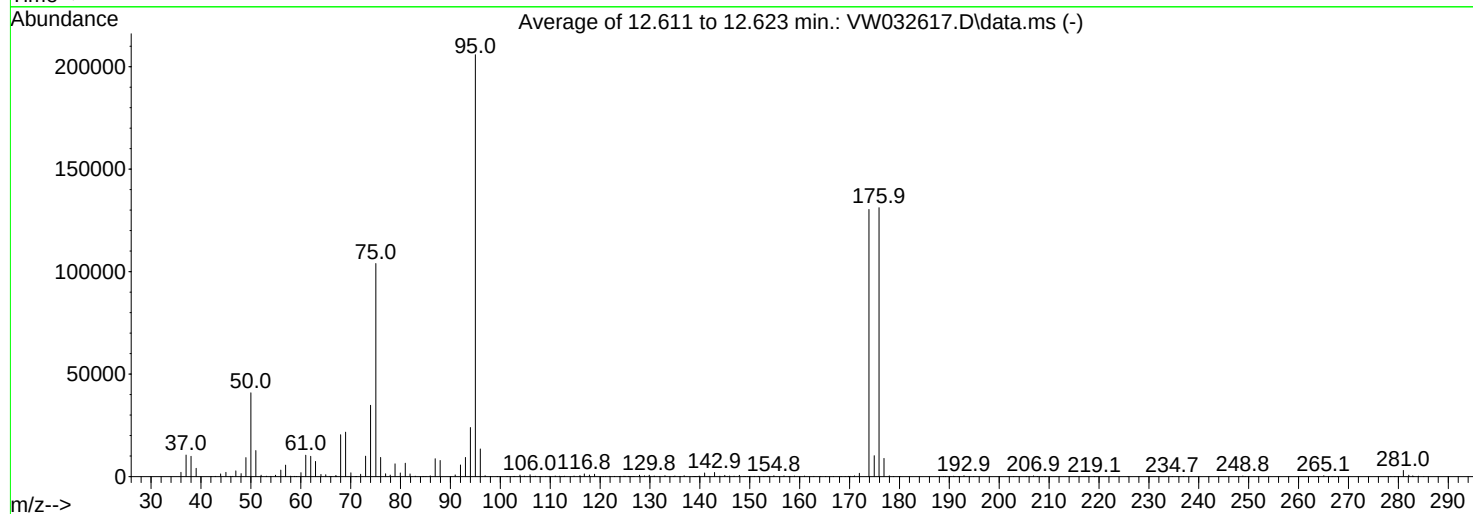


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW121125\  
Data File : VW032617.D  
Acq On : 11 Dec 2025 07:29  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\82W121025S.M  
Title : SW846 8260  
Last Update : Thu Dec 11 01:56:28 2025

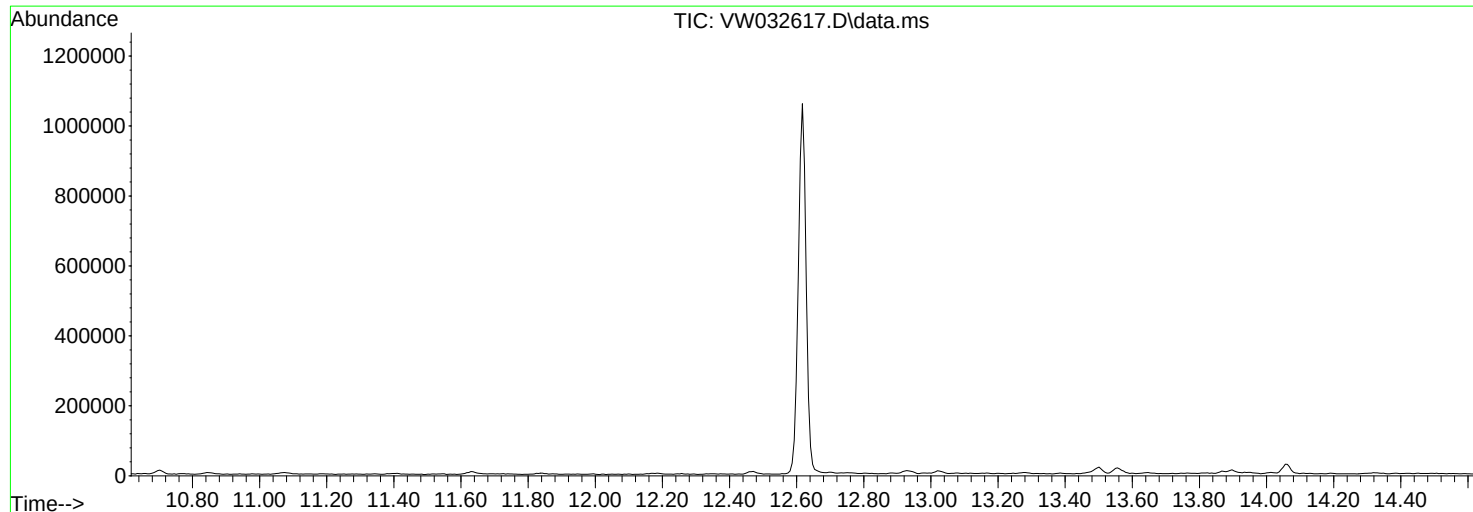

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1747

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.9  | 40880  | PASS      |
| 75     | 95      | 30     | 60     | 50.5  | 103944 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 205803 | PASS      |
| 96     | 95      | 5      | 9      | 6.5   | 13454  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.0   | 0      | PASS      |
| 174    | 95      | 50     | 100    | 63.3  | 130336 | PASS      |
| 175    | 174     | 5      | 9      | 7.8   | 10219  | PASS      |
| 176    | 174     | 95     | 101    | 100.7 | 131213 | PASS      |
| 177    | 176     | 5      | 9      | 6.8   | 8893   | PASS      |