

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
 Data File : VW014324.D
 Acq On : 12 Dec 2019 14:20
 Operator : SY/VA
 Sample : K6238-04RE
 Misc : 3.98G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFPZ7RE

Manual Integrations
 APPROVED

apatel
 12/16/2019 1:01:41 PM

Quant Time: Dec 13 06:10:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:08:10 2019
 Response via : Initial Calibration

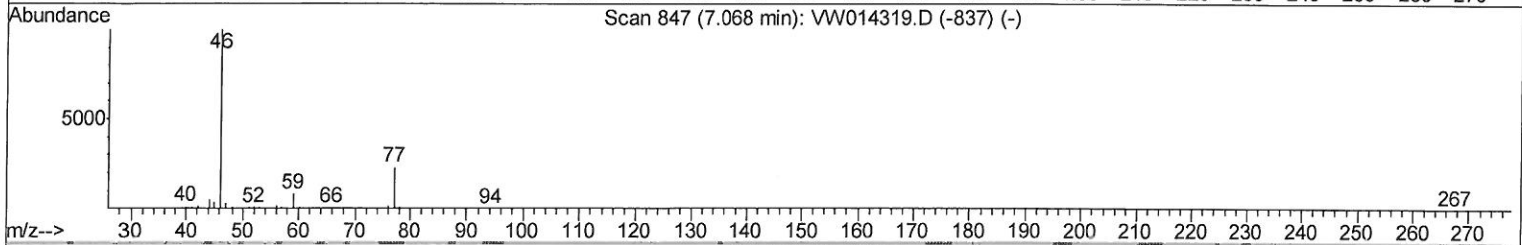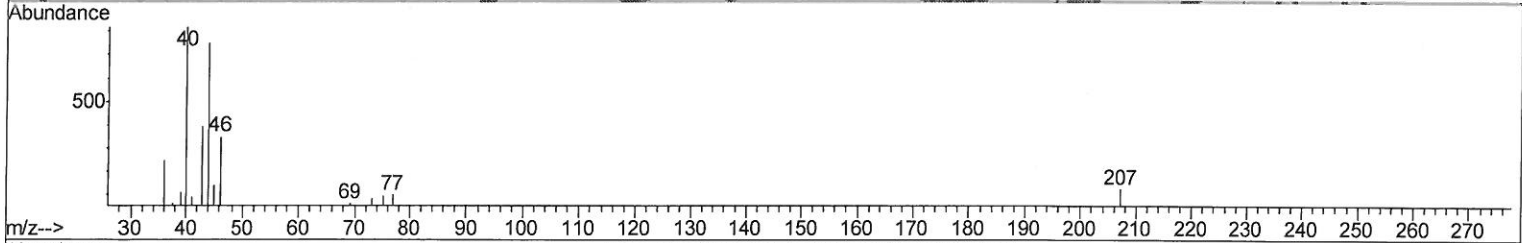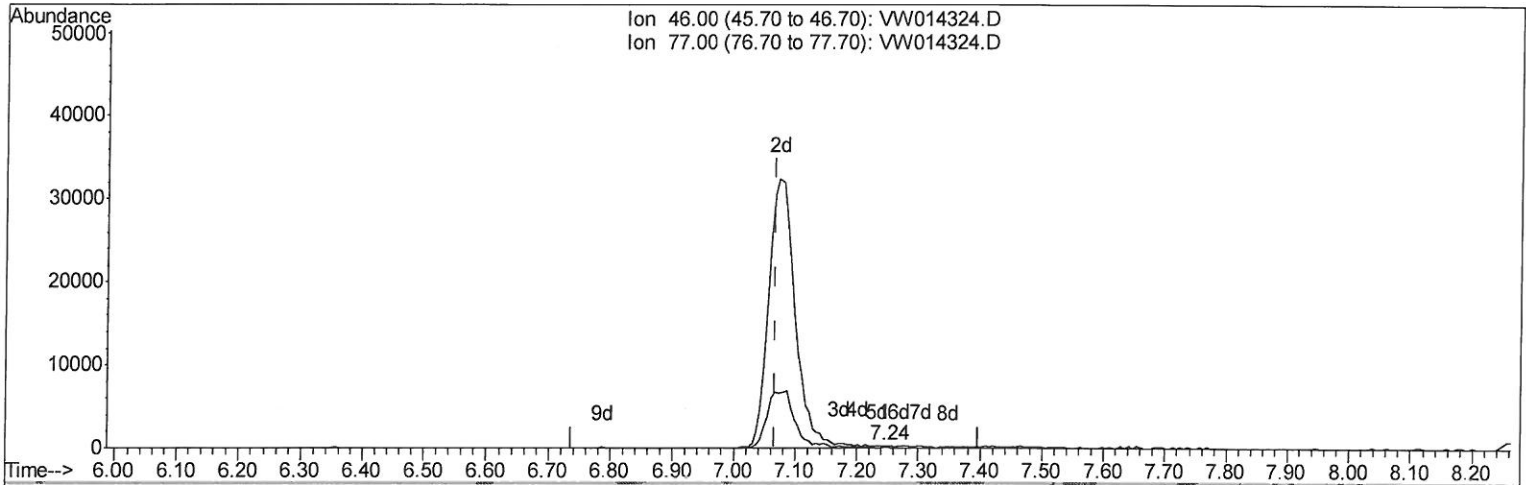

TIC: VW014324.D

(20) 2-Butanone-d5 (S)
 7.244min (+0.177) 0.08ug/L
 response 302

Ion	Exp%	Act%
46.00	100	100
77.00	26.00	23.84
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
 Data File : VW014324.D
 Acq On : 12 Dec 2019 14:20
 Operator : SY/VA
 Sample : K6238-04RE
 Misc : 3.98G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFPZ7RE

Manual Integrations
 APPROVED

apatel
 12/16/2019 1:01:41 PM

Quant Time: Dec 13 06:10:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:08:10 2019
 Response via : Initial Calibration

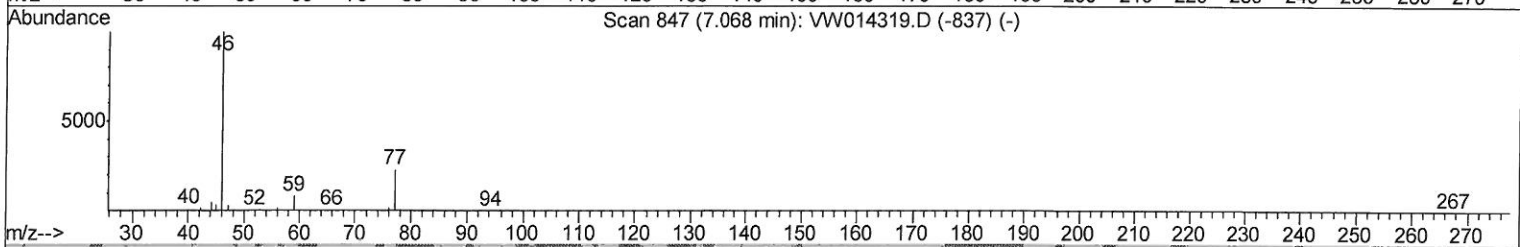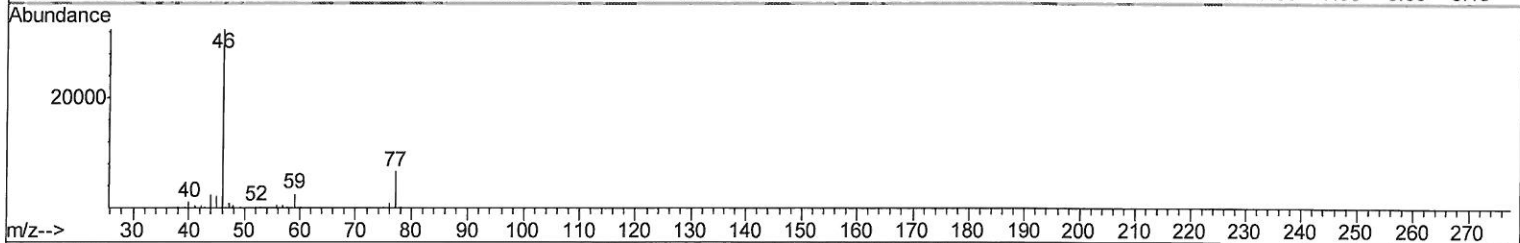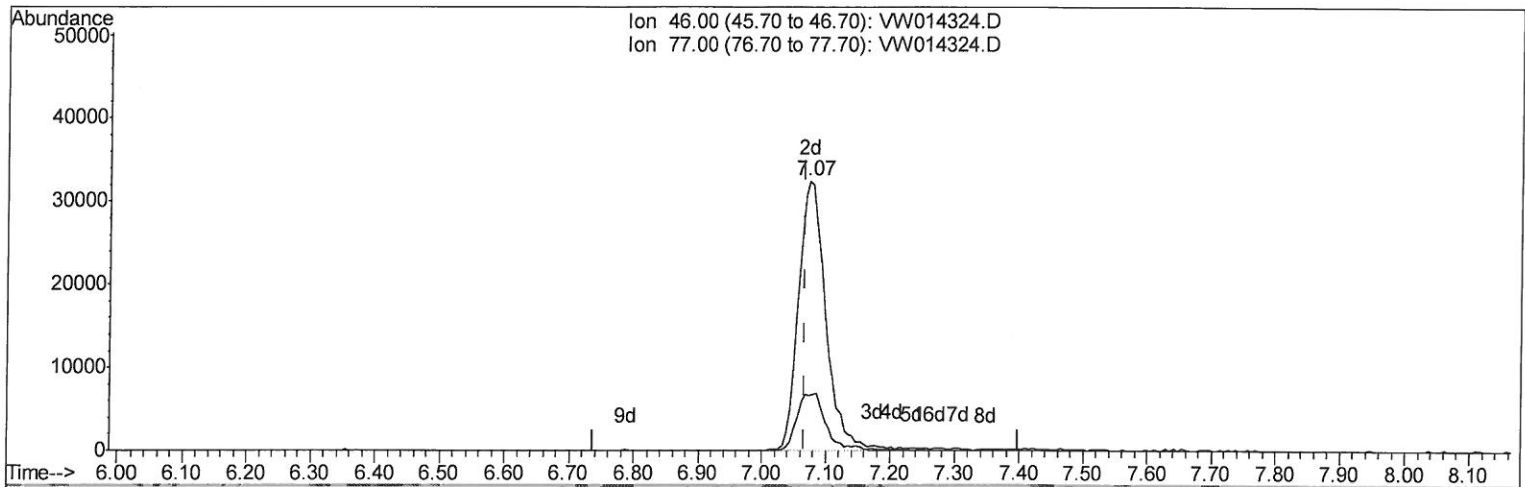

(20) 2-Butanone-d5 (S)

7.074min (+0.006) 23.77ug/L m

> 12/13/19 SY

response 95321

Ion	Exp%	Act%
46.00	100	100
77.00	26.00	0.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
 Data File : VW014324.D
 Acq On : 12 Dec 2019 14:20
 Operator : SY/VA
 Sample : K6238-04RE
 Misc : 3.98G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFPZ7RE

Manual Integrations
 APPROVED

apatel
 12/16/2019 1:01:41 PM

Quant Time: Dec 13 06:45:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:08:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1016154	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	705072	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	167304	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	368632	23.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.84%
7) Chloroethane-d5	2.89	69	306355	26.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.12%
10) 1,1-Dichloroethene-d2	4.01	63	522108	19.21	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.84%
20) 2-Butanone-d5	7.07	46	95321m	23.77	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	47.54%
24) Chloroform-d	7.65	84	656830	25.39	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.56%
26) 1,2-Dichloroethane-d4	8.30	65	330534	24.37	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.48%
29) Benzene-d6	8.27	84	1348619	32.64	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	130.56%
33) 1,2-Dichloropropane-d6	9.27	67	405654	31.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	127.64%#
37) Toluene-d8	10.32	98	1054502	28.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	112.88%
38) trans-1,3-Dichloropropene-	10.57	79	121239	22.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.92%
39) 2-Hexanone-d5	10.92	63	81726	32.33	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.66%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	190326	18.37	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.48%
61) 1,2-Dichlorobenzene-d4	13.85	152	145407	22.74	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.96%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.12	43	32345	8.366	ug/L	94
16) Methylene chloride	4.92	84	41704	2.677	ug/L	96
44) Toluene	10.38	91	30240	0.646	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
Data File : VW014324.D
Acq On : 12 Dec 2019 14:20
Operator : SY/VA
Sample : K6238-04RE
Misc : 3.98G/10ML/MSVOA W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFPZ7RE

Manual Integrations
APPROVED

apatel
12/16/2019 1:01:41 PM

Quant Time: Dec 13 06:45:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 13 06:08:10 2019
Response via : Initial Calibration

