

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
 Data File : VW014327.D
 Acq On : 12 Dec 2019 15:43
 Operator : SY/VA
 Sample : K6236-15
 Misc : 5.84G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFEX1

Manual Integrations
 APPROVED

apatel
 12/16/2019 1:01:46 PM

Quant Time: Dec 13 06:11:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:08:10 2019
 Response via : Initial Calibration

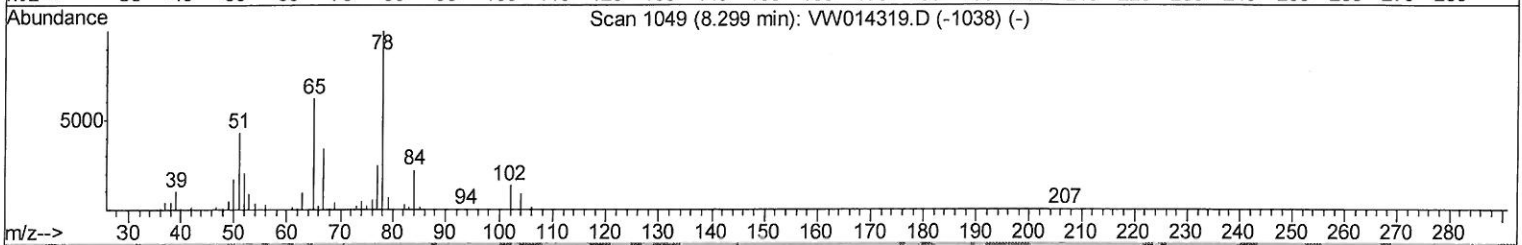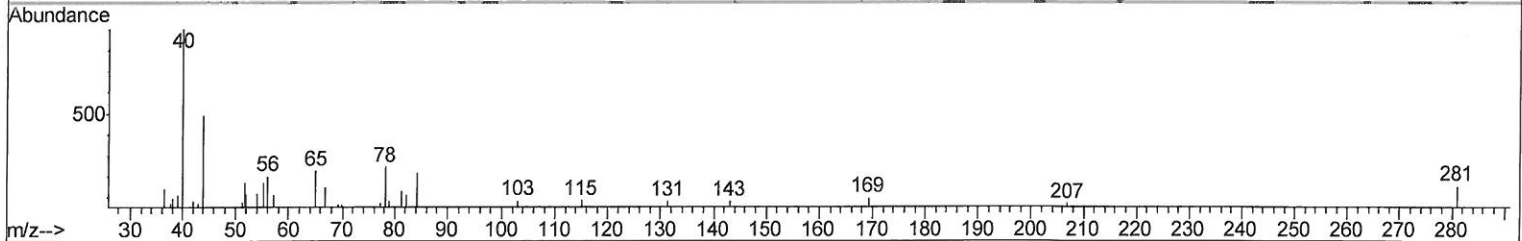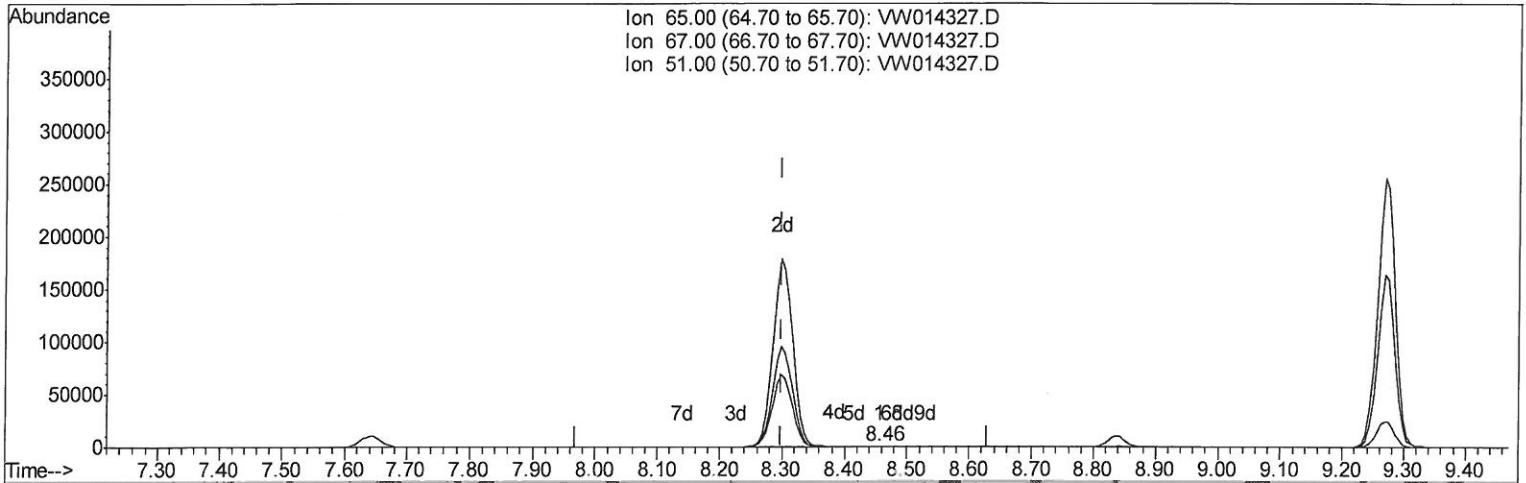

TIC: VW014327.D

(26) 1,2-Dichloroethane-d4 (S)

8.457min (+0.158) 0.01ug/L

response 208

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	68.75
51.00	107.20	118.75
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
 Data File : VW014327.D
 Acq On : 12 Dec 2019 15:43
 Operator : SY/VA
 Sample : K6236-15
 Misc : 5.84G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFEX1

Manual Integrations
 APPROVED

apatel
 12/16/2019 1:01:46 PM

Quant Time: Dec 13 06:11:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:08:10 2019
 Response via : Initial Calibration

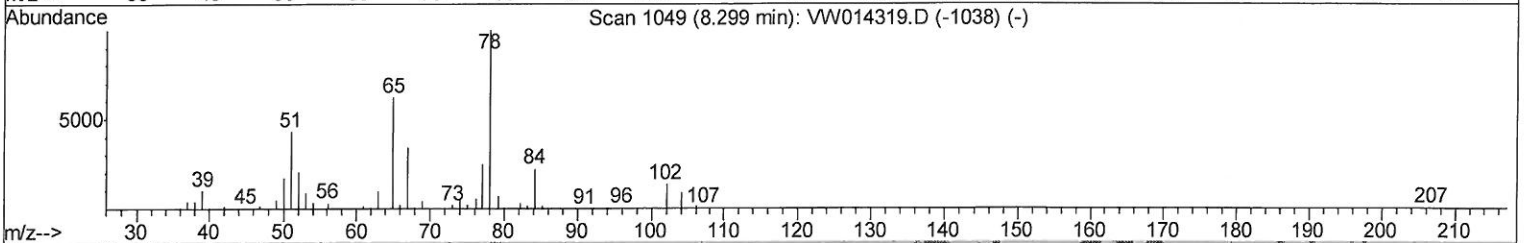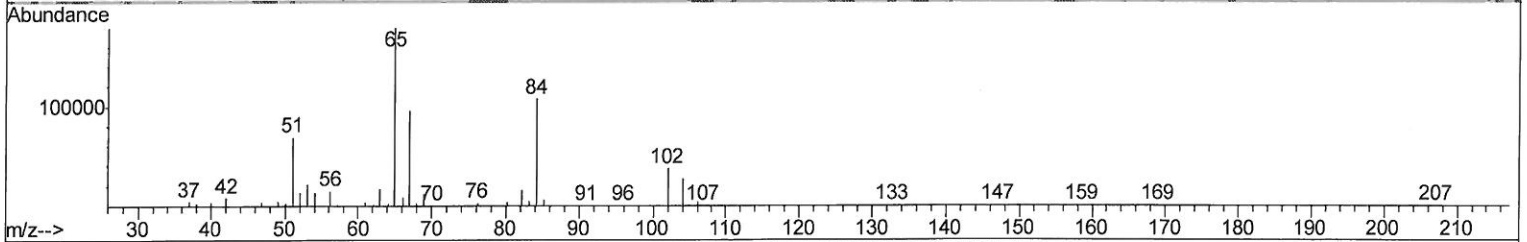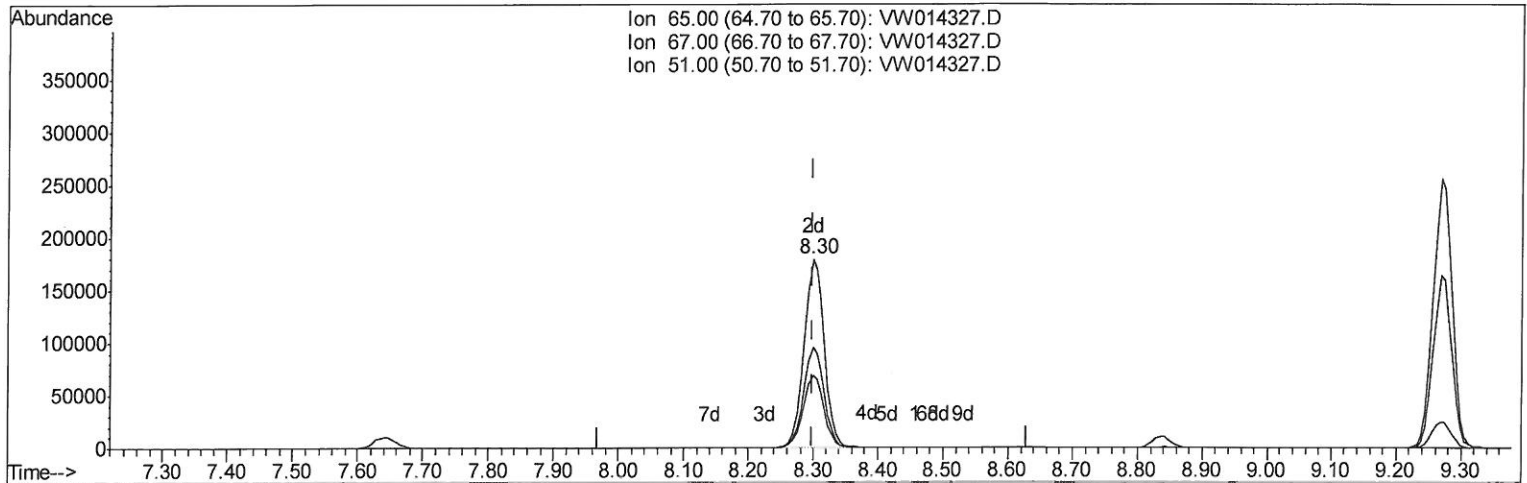

TIC: VW014327.D

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.000) 23.18ug/L m

response 390320

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	0.04#
51.00	107.20	0.06#
0.00	0.00	0.00

12/13/19 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
 Data File : VW014327.D
 Acq On : 12 Dec 2019 15:43
 Operator : SY/VA
 Sample : K6236-15
 Misc : 5.84G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFEX1

Manual Integrations
 APPROVED

apatel
 12/16/2019 1:01:46 PM

Quant Time: Dec 13 07:22:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:08:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	1261452	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1021980	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	357700	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	443148	23.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.80%
7) Chloroethane-d5	2.89	69	356351	25.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.36%
10) 1,1-Dichloroethene-d2	4.01	63	614580	18.22	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.88%
20) 2-Butanone-d5	7.07	46	196120	39.40	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.80%
24) Chloroform-d	7.64	84	773867	24.09	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.36%
26) 1,2-Dichloroethane-d4	8.30	65	390320m	23.18	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.72%
29) Benzene-d6	8.27	84	1674951	27.96	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.84%
33) 1,2-Dichloropropane-d6	9.27	67	512421	27.81	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.24%
37) Toluene-d8	10.32	98	1414112	26.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.44%
38) trans-1,3-Dichloropropene-	10.57	79	181704	23.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.00%
39) 2-Hexanone-d5	10.92	63	157367	42.95	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.90%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	305538	20.35	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.40%
61) 1,2-Dichlorobenzene-d4	13.85	152	335827	24.57	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.28%

Target Compounds				Ovalue
13) Acetone	4.12	43	64619	13.464 ug/L 98
16) Methylene chloride	4.91	84	80293	4.152 ug/L 92
56) Styrene	12.18	104	14385	0.313 ug/L 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
Data File : VW014327.D
Acq On : 12 Dec 2019 15:43
Operator : SY/VA
Sample : K6236-15
Misc : 5.84G/10ML/MSVOA W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFEX1

Manual Integrations
APPROVED

apatel
12/16/2019 1:01:46 PM

Quant Time: Dec 13 07:22:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 13 06:08:10 2019
Response via : Initial Calibration

