

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
 Data File : VW014338.D
 Acq On : 12 Dec 2019 20:33
 Operator : SY/VA
 Sample : K6322-05
 Misc : 3.83G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 C0C35

Quant Time: Dec 13 06:12:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:08:10 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 12/16/2019 1:08:11 PM

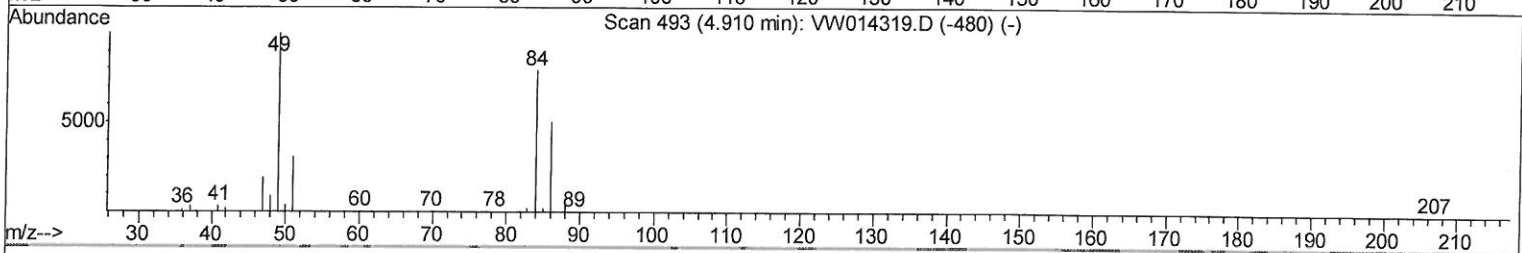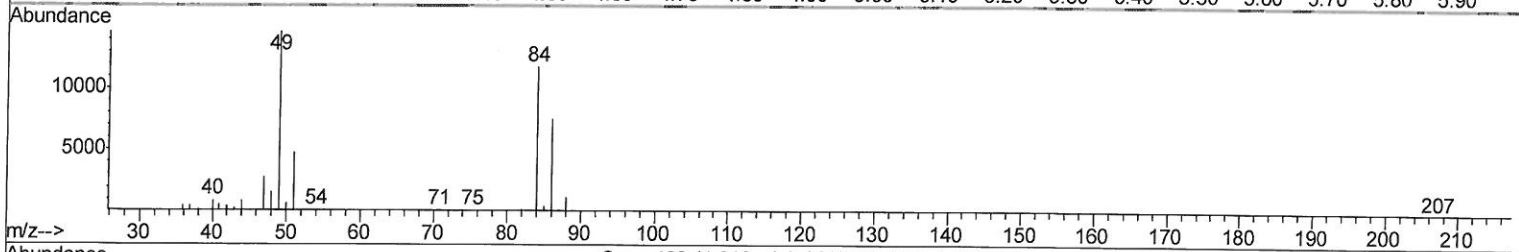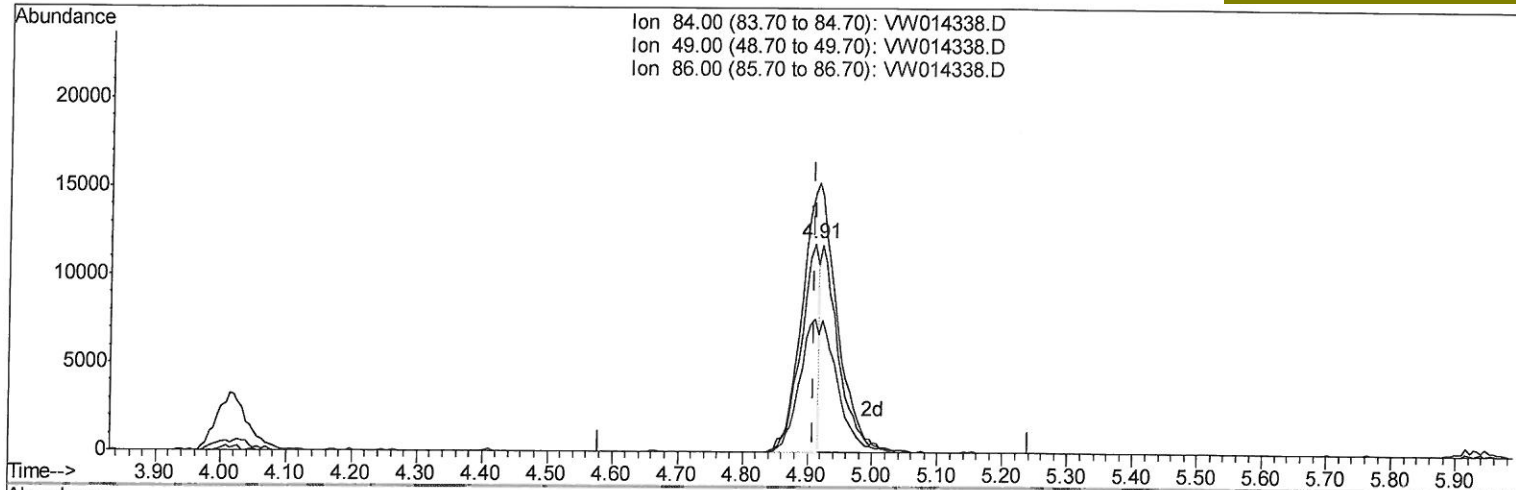

TIC: VW014338.D

(16) Methylene chloride (T)

4.909min (-0.000) 1.41ug/L

response 23103

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	123.86
86.00	62.40	63.80
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
 Data File : VW014338.D
 Acq On : 12 Dec 2019 20:33
 Operator : SY/VA
 Sample : K6322-05
 Misc : 3.83G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 C0C35

Quant Time: Dec 13 06:12:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:08:10 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 12/16/2019 1:08:11 PM

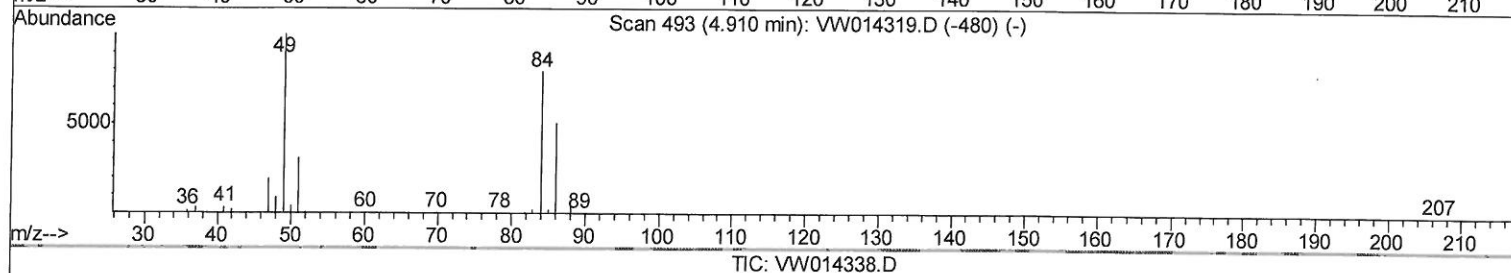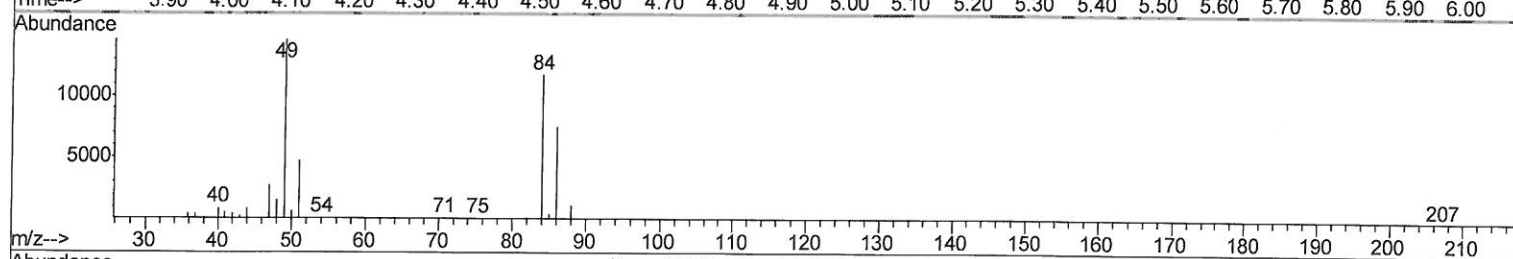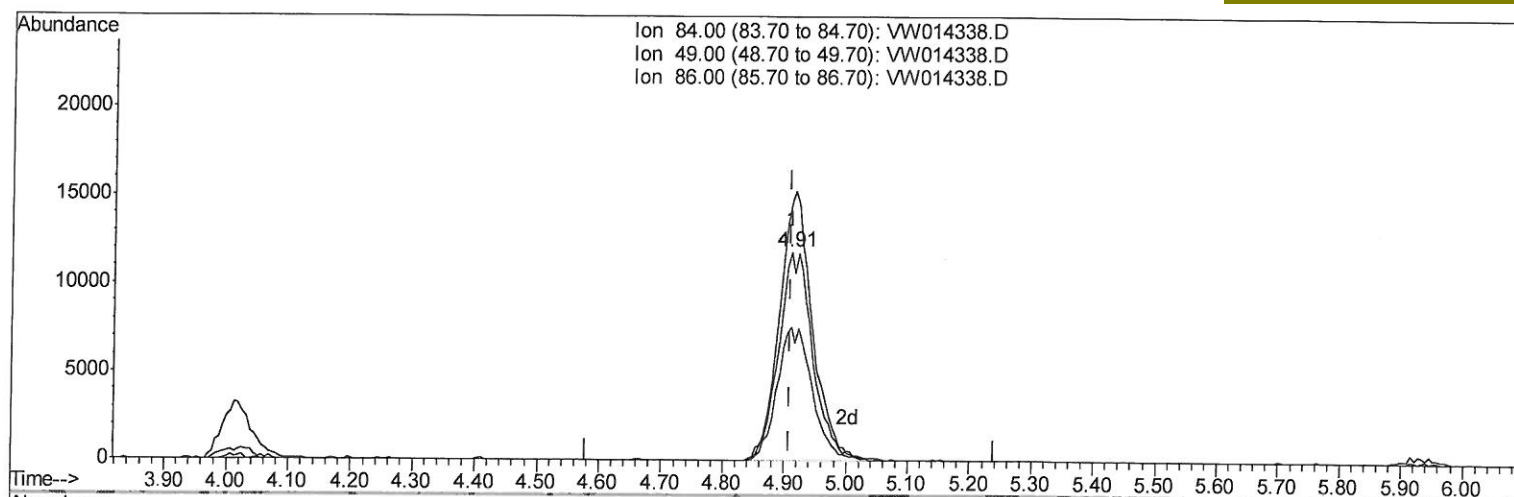

(16) Methylene chloride (T)

4.909min (-0.000) 2.79ug/L m

response 45772

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	123.86
86.00	62.40	63.80
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
 Data File : VW014338.D
 Acq On : 12 Dec 2019 20:33
 Operator : SY/VA
 Sample : K6322-05
 Misc : 3.83G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 C0C35

Quant Time: Dec 13 08:00:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:08:10 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 12/16/2019 1:08:11 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1071663	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	826046	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	244119	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	335150	20.65	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.60%		
7) Chloroethane-d5	2.89	69	272307	22.57	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.28%		
10) 1,1-Dichloroethene-d2	4.01	63	449059	15.67	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	62.68%		
20) 2-Butanone-d5	7.07	46	158112	37.39	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	74.78%		
24) Chloroform-d	7.64	84	622036	22.80	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.20%		
26) 1,2-Dichloroethane-d4	8.30	65	328415	22.96	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.84%		
29) Benzene-d6	8.27	84	1278318	26.40	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	105.60%		
33) 1,2-Dichloropropane-d6	9.27	67	420183	28.21	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	112.84%		
37) Toluene-d8	10.32	98	1022999	23.37	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.48%		
38) trans-1,3-Dichloropropene-	10.57	79	125919	20.15	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.60%		
39) 2-Hexanone-d5	10.92	63	116237	39.25	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	78.50%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	282093	23.24	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	92.96%		
61) 1,2-Dichlorobenzene-d4	13.85	152	228389	24.48	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	97.92%		

Target Compounds

13) Acetone	4.12	43	14027	3.440	ug/L	Ovalue 89
16) Methylene chloride	4.91	84	45772m	2.786	ug/L	12/11/18/19 > y

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121219\
Data File : VW014338.D
Acq On : 12 Dec 2019 20:33
Operator : SY/VA
Sample : K6322-05
Misc : 3.83G/10ML/MSVOA W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0C35

Quant Time: Dec 13 08:00:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 13 06:08:10 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

apatel
12/16/2019 1:08:11 PM

