
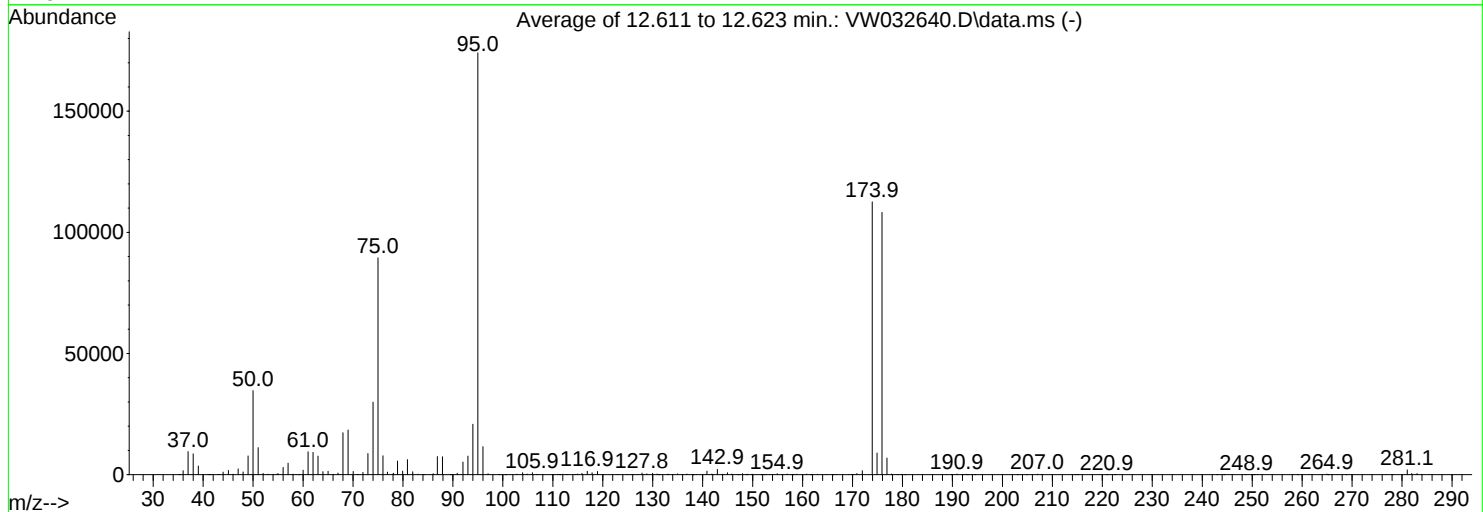


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121225\
Data File : VW032640.D
Acq On : 12 Dec 2025 07:43
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W121025S.M
Title : SW846 8260
Last Update : Thu Dec 11 01:56:28 2025

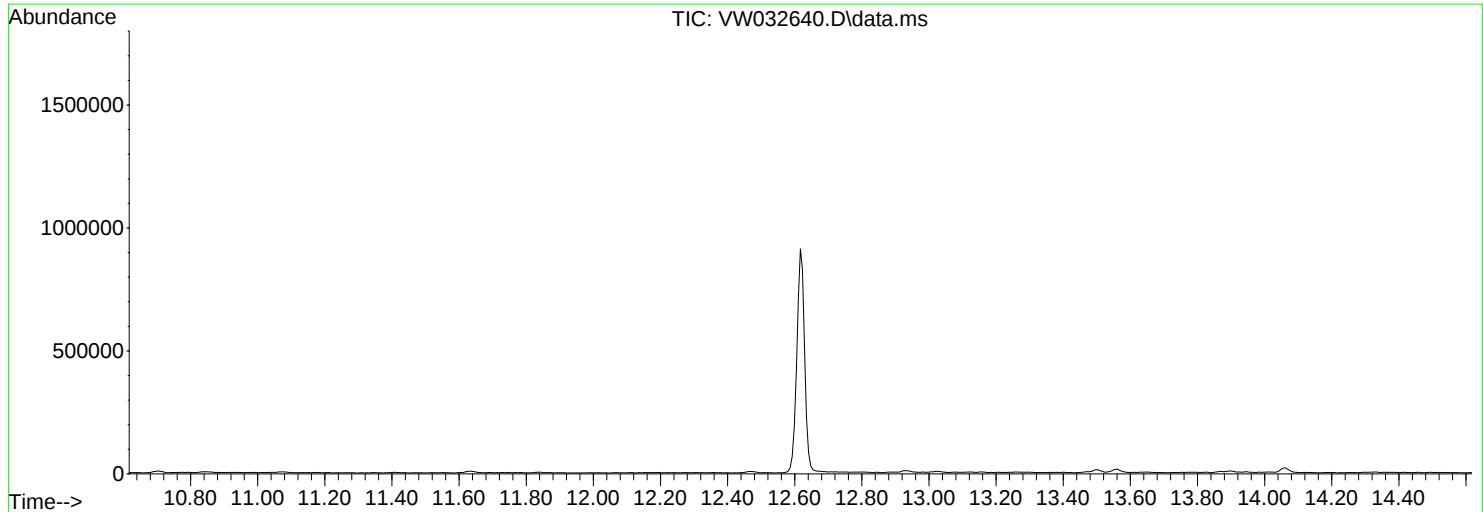

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	34642	PASS
75	95	30	60	51.4	89459	PASS
95	95	100	100	100.0	174080	PASS
96	95	5	9	6.6	11535	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	64.7	112584	PASS
175	174	5	9	7.9	8929	PASS
176	174	95	101	96.1	108208	PASS
177	176	5	9	6.3	6843	PASS