

Data File : VW014354.D
Acq On : 13 Dec 2019 17:15
Operator : SY/VA
Sample : K6270-05
Misc : 5.18G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETK83

Quant Time: Dec 14 04:32:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 14 04:28:18 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1322588	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1190826	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	536684	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	353504	17.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.60%
7) Chloroethane-d5	2.89	69	282859	18.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.96%
10) 1,1-Dichloroethene-d2	4.01	63	501040	14.16	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.64%
20) 2-Butanone-d5	7.07	46	259269	49.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.36%
24) Chloroform-d	7.64	84	694901	20.64	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.56%
26) 1,2-Dichloroethane-d4	8.30	65	399620	22.63	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.52%
29) Benzene-d6	8.27	84	1447525	20.74	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.96%
33) 1,2-Dichloropropane-d6	9.27	67	460633	21.45	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.80%
37) Toluene-d8	10.32	98	1256237	19.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.64%
38) trans-1,3-Dichloropropene-	10.57	79	184774	20.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.04%
39) 2-Hexanone-d5	10.92	63	223056	52.24	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.48%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	406749	23.25	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.00%
61) 1,2-Dichlorobenzene-d4	13.85	152	425249	20.74	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.96%

Target Compounds


					Qvalue
30) Cyclohexane	7.95	56	16151	0.543 ug/L #	26
34) Benzene	8.32	78	76295	1.012 ug/L	100
44) Toluene	10.38	91	201368	2.547 ug/L	100
49) 2-Hexanone	10.93	43	31001	3.409 ug/L #	60
53) Ethylbenzene	11.73	91	68839	0.803 ug/L	91
54) m,p-Xylene	11.83	106	39209	1.188 ug/L	96
55) o-xylene	12.16	106	16021	0.512 ug/L	93
59) 1,2,3-Trichloropropane	13.55	75	63108	4.714 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014354.D
Acq On : 13 Dec 2019 17:15
Operator : SY/VA
Sample : K6270-05
Misc : 5.18G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETK83

Quant Time: Dec 14 04:32:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 14 04:28:18 2019
Response via : Initial Calibration




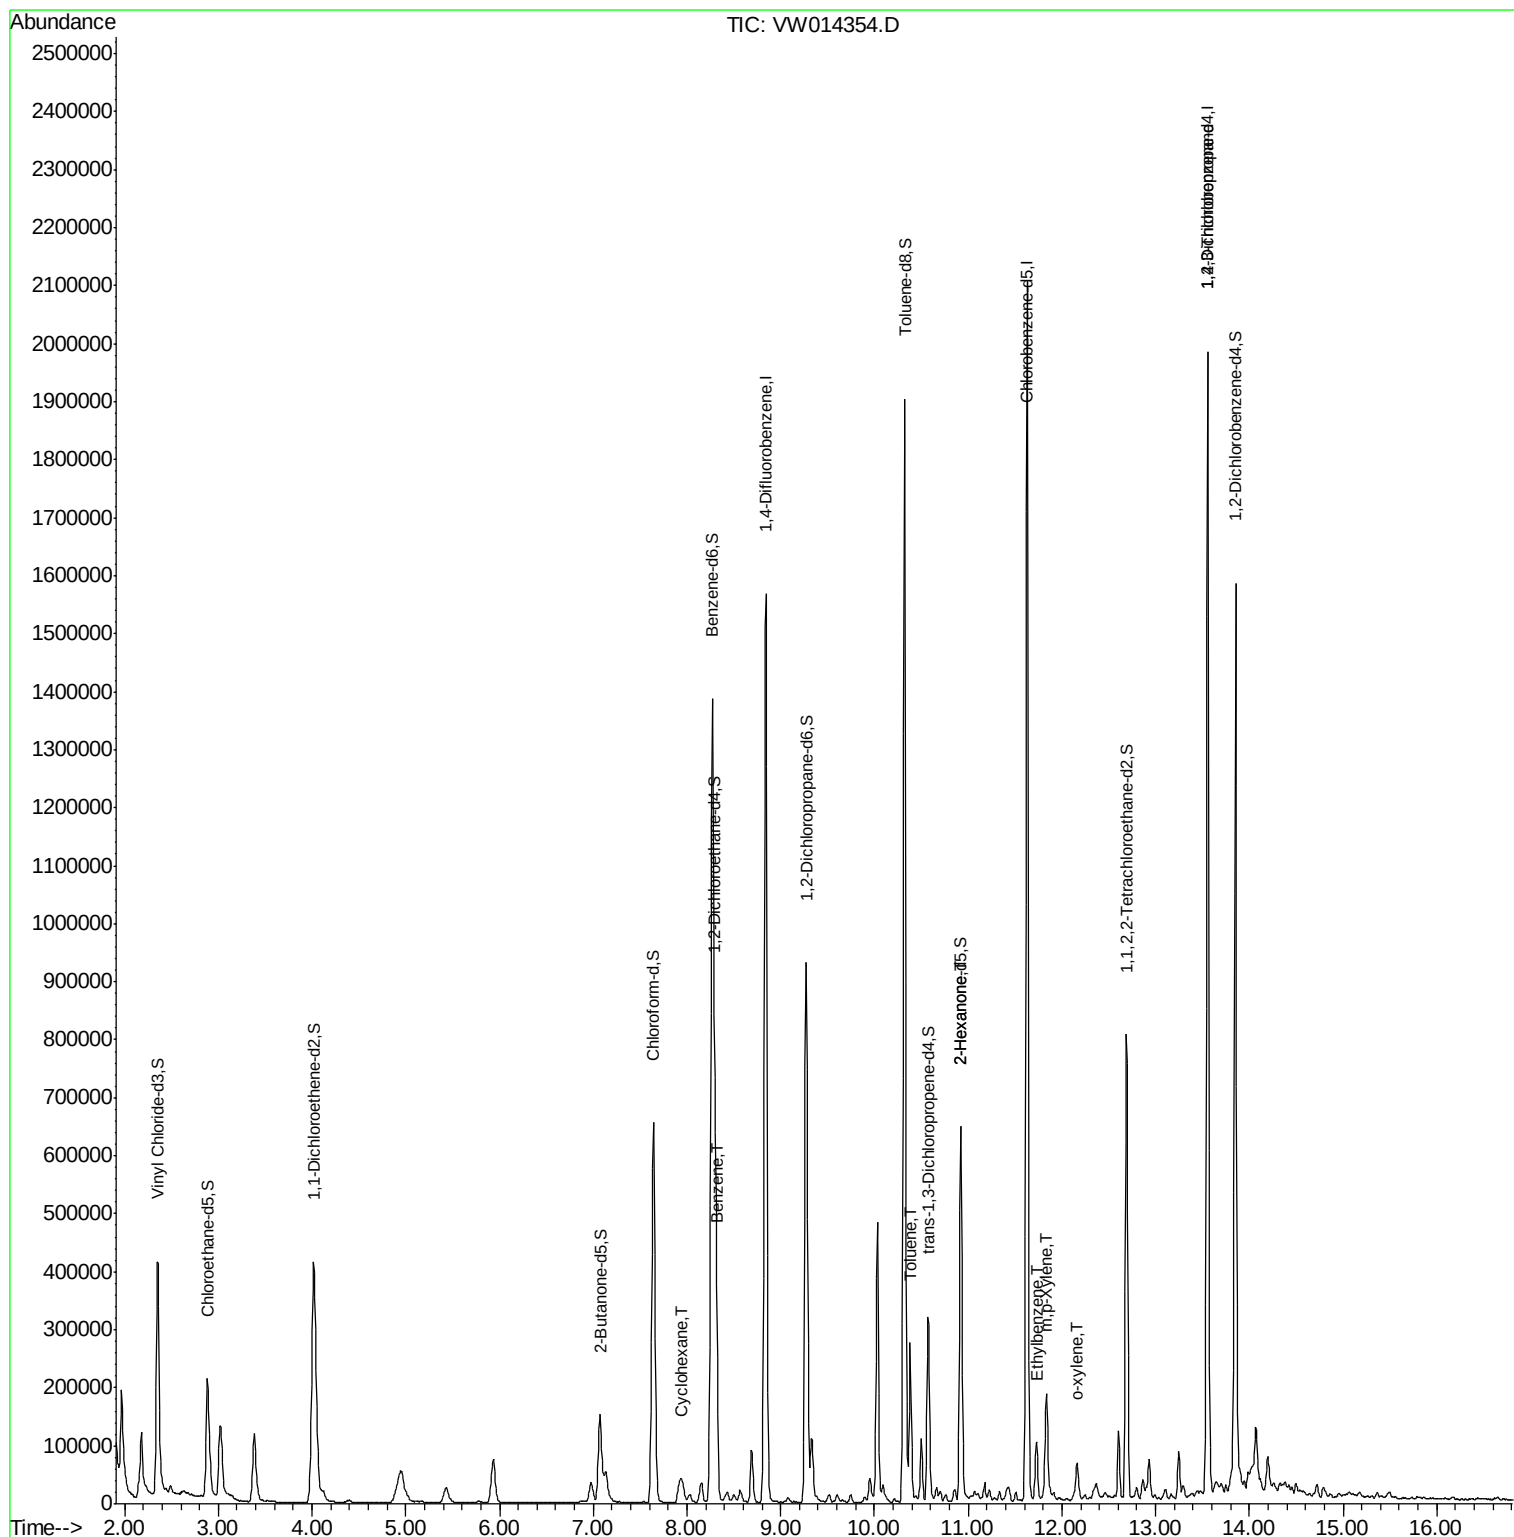


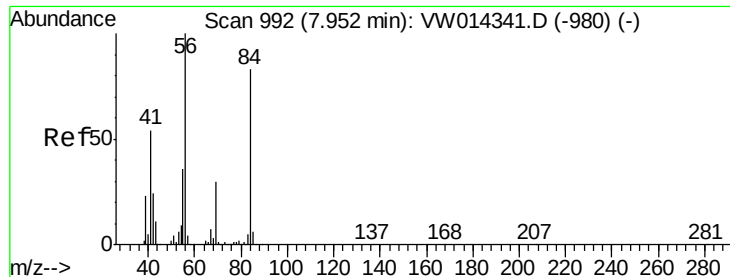

#30
Cyclohexane
Concen: 0.543 ug/L
RT: 7.95 min Scan# 991
Delta R.T. -0.01 min
Lab File: VW014354.D
Acq: 13 Dec 2019 17:15




Instrument :
MSVOA_W
ClientSampled :
ETK83


Tgt Ion: 56 Resp: 16151
Ion Ratio Lower Upper
56 100
69 40.6 24.6 37.0#
84 1.3 70.2 105.2#

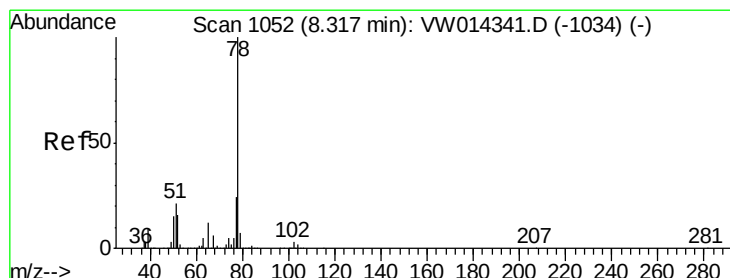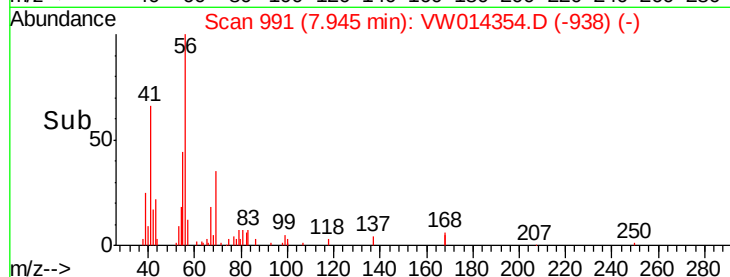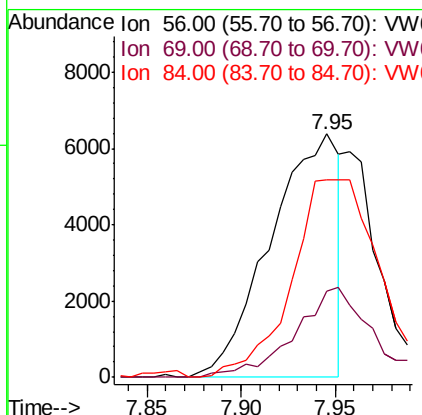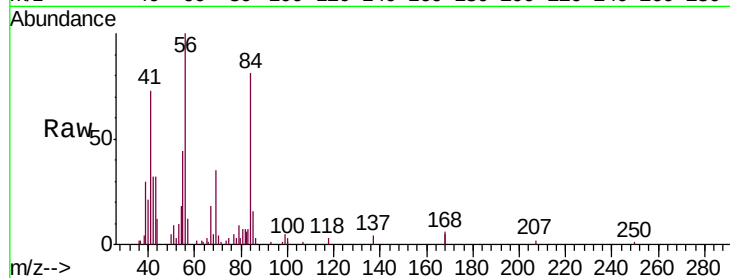

#34
Benzene
Concen: 1.012 ug/L
RT: 8.32 min Scan# 1053
Delta R.T. 0.01 min
Lab File: VW014354.D
Acq: 13 Dec 2019 17:15

Tgt Ion: 78 Resp: 76295

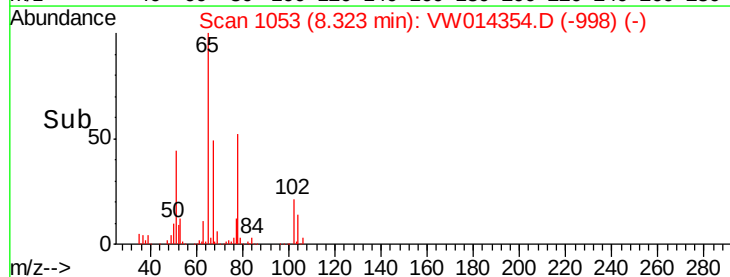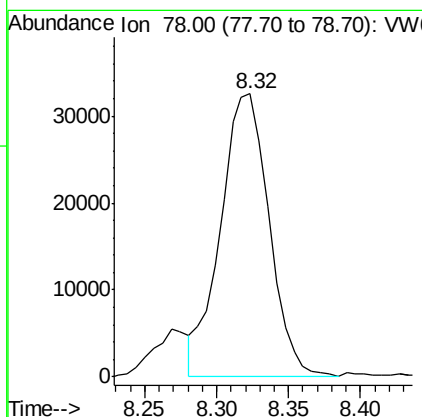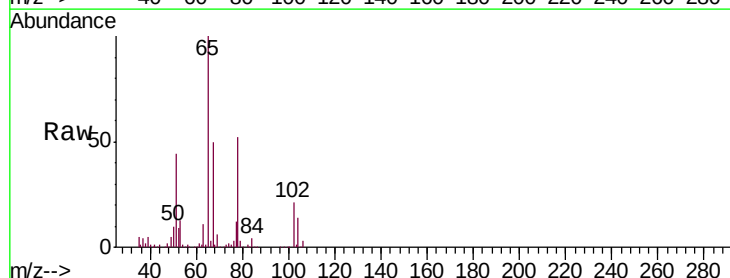

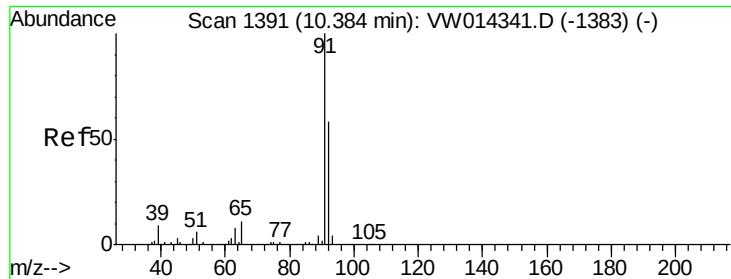

#44

Toluene

Concen: 2.547 ug/L

RT: 10.38 min Scan# 1391

Delta R.T. -0.00 min

Lab File: VW014354.D

Acq: 13 Dec 2019 17:15

Instrument :

MSVOA_W

ClientSampleId :





ETK83

Tgt Ion: 91 Resp: 201368

Ion Ratio Lower Upper

91 100

92 57.9 40.7 75.7

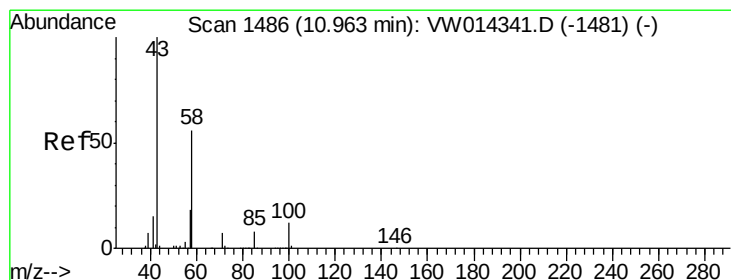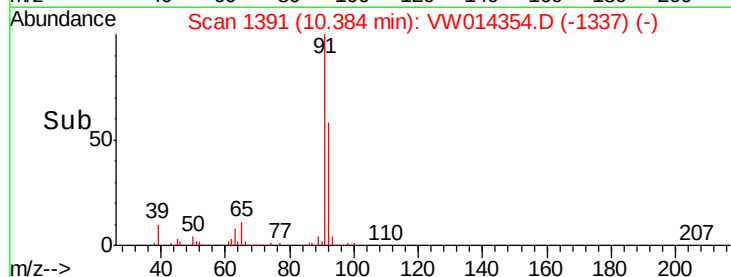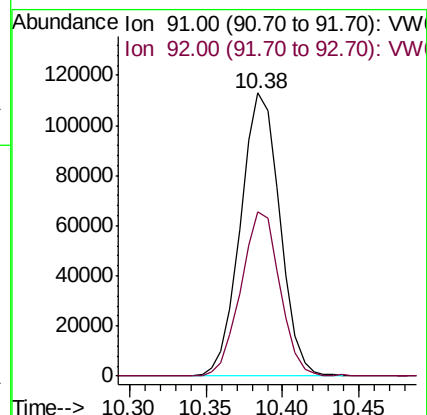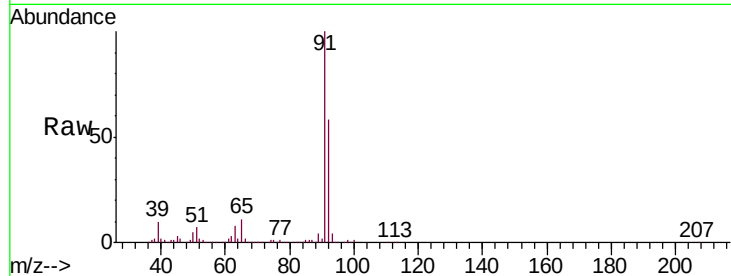

#49

2-Hexanone

Concen: 3.409 ug/L

RT: 10.93 min Scan# 1480

Delta R.T. -0.04 min

Lab File: VW014354.D

Acq: 13 Dec 2019 17:15

Tgt Ion: 43 Resp: 31001




Ion Ratio Lower Upper


43 100

58 23.4 44.4 66.6#

57 37.1 16.5 24.7#

100 1.5 11.1 16.7#

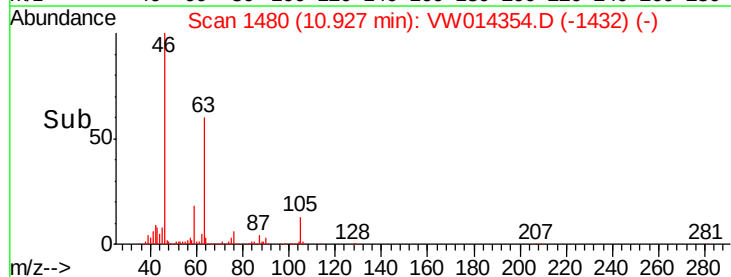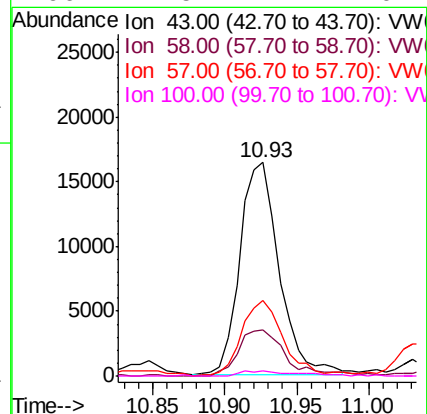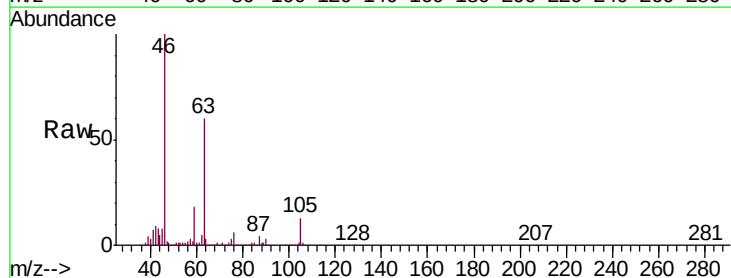

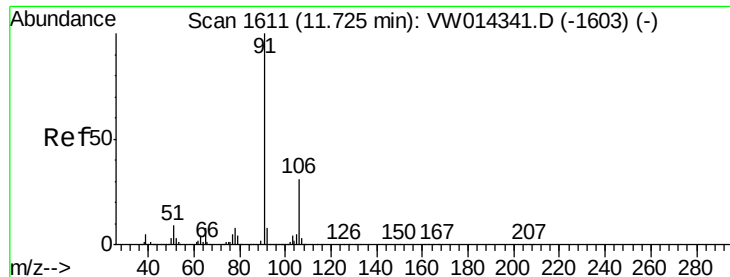

#53

Ethylbenzene

Concen: 0.803 ug/L

RT: 11.73 min Scan# 1611

Delta R.T. -0.00 min

Lab File: VW014354.D

Acq: 13 Dec 2019 17:15

Instrument :

MSVOA_W

ClientSampleId :





ETK83

Tgt Ion: 91 Resp: 68839

Ion Ratio Lower Upper

91 100

106 26.7 22.3 41.5

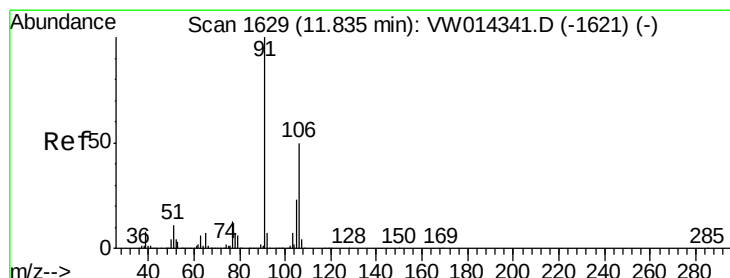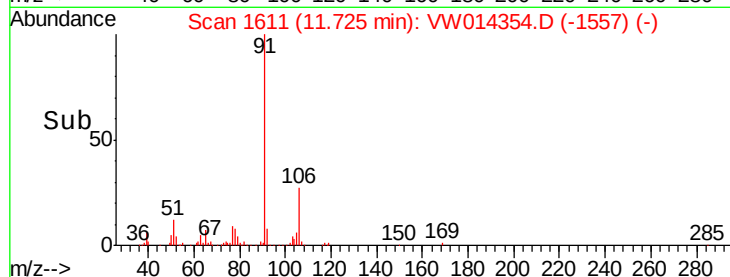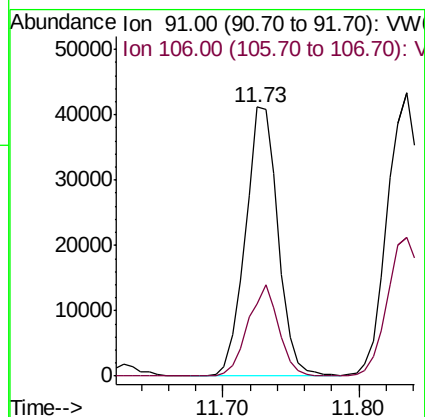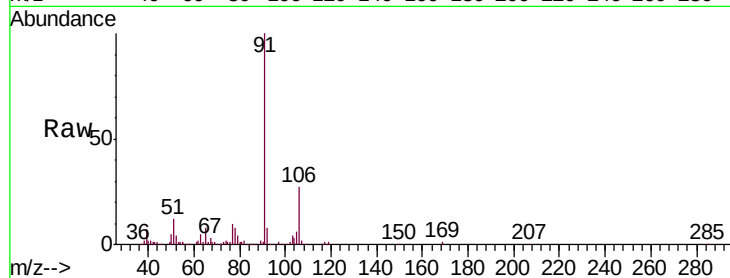

#54

m,p-Xylene

Concen: 1.188 ug/L

RT: 11.83 min Scan# 1629

Delta R.T. -0.00 min

Lab File: VW014354.D




Acq: 13 Dec 2019 17:15


Tgt Ion: 106 Resp: 39209

Ion Ratio Lower Upper

106 100

91 204.8 138.7 257.5


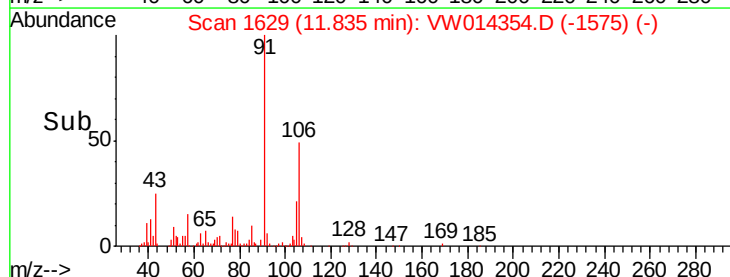
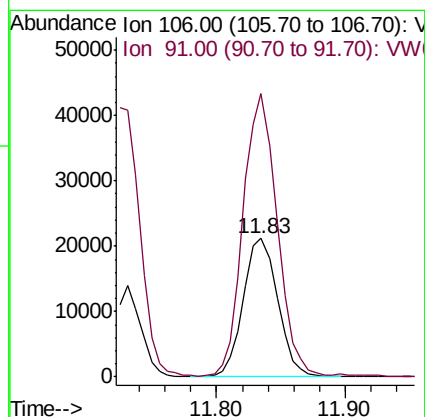
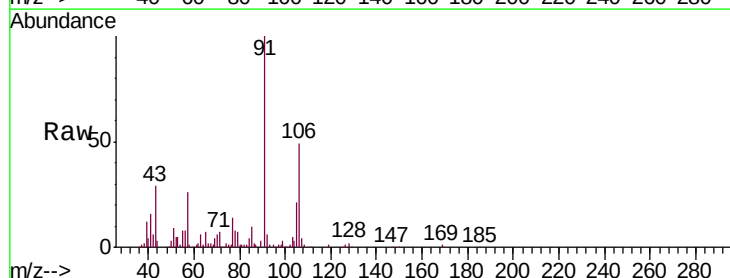


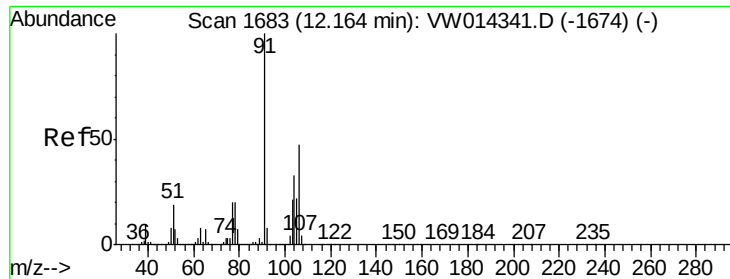

#55
o-xylene
Concen: 0.512 ug/L
RT: 12.16 min Scan# 1683
Delta R.T. -0.00 min
Lab File: VW014354.D
Acq: 13 Dec 2019 17:15

Instrument :
MSVOA_W
ClientSampled :
ETK83

Tgt Ion:106 Resp: 16021
Ion Ratio Lower Upper
106 100
91 200.5 148.3 275.5

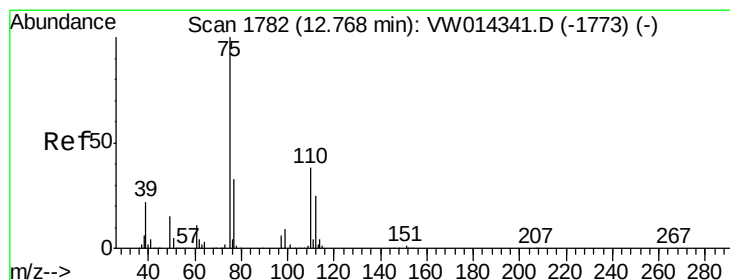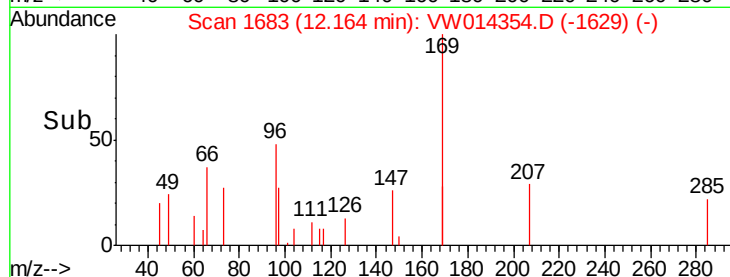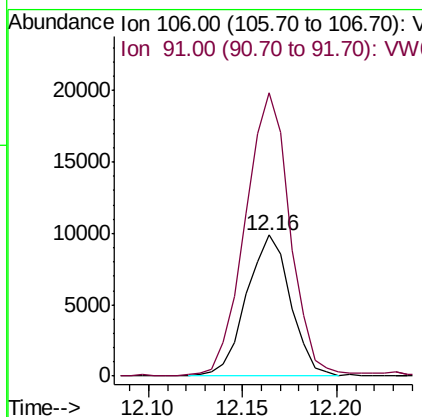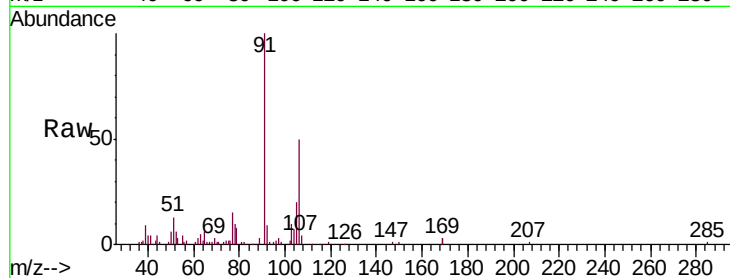

#59
1,2,3-Trichloropropane
Concen: 4.714 ug/L
RT: 13.55 min Scan# 1911
Delta R.T. 0.79 min
Lab File: VW014354.D
Acq: 13 Dec 2019 17:15

Tgt Ion: 75 Resp: 63108
Ion Ratio Lower Upper
75 100
77 38.2 25.9 38.9

