

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121319\
 Data File : VW014344.D
 Acq On : 13 Dec 2019 12:51
 Operator : SY/VA
 Sample : K6322-02RE
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0C30RE

Quant Time: Dec 14 05:19:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 14 04:28:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	893762	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	674924	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	196080	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	296925	21.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.76%
7) Chloroethane-d5	2.89	69	261161	25.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.80%
10) 1,1-Dichloroethene-d2	4.02	63	417973	17.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.92%
20) 2-Butanone-d5	7.07	46	155119	43.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.96%
24) Chloroform-d	7.65	84	627770	27.59	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	110.36%
26) 1,2-Dichloroethane-d4	8.30	65	319756	26.80	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.20%
29) Benzene-d6	8.27	84	1282793	32.43	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	129.72%
33) 1,2-Dichloropropane-d6	9.27	67	420703	34.57	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	138.28%#
37) Toluene-d8	10.32	98	1007910	28.18	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	112.72%
38) trans-1,3-Dichloropropene-	10.57	79	114197	22.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.48%
39) 2-Hexanone-d5	10.92	63	119331	49.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.62%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	274091	27.64	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	110.56%
61) 1,2-Dichlorobenzene-d4	13.85	152	226910	30.28	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	121.12%#


Target Compounds					Ovalue
13) Acetone	4.12	43	13770	4.050 ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW121319\
Data File : VW014344.D
Acq On : 13 Dec 2019 12:51
Operator : SY/VA
Sample : K6322-02RE
Misc : 5.02G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0C30RE

Quant Time: Dec 14 05:19:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 14 04:28:18 2019
Response via : Initial Calibration

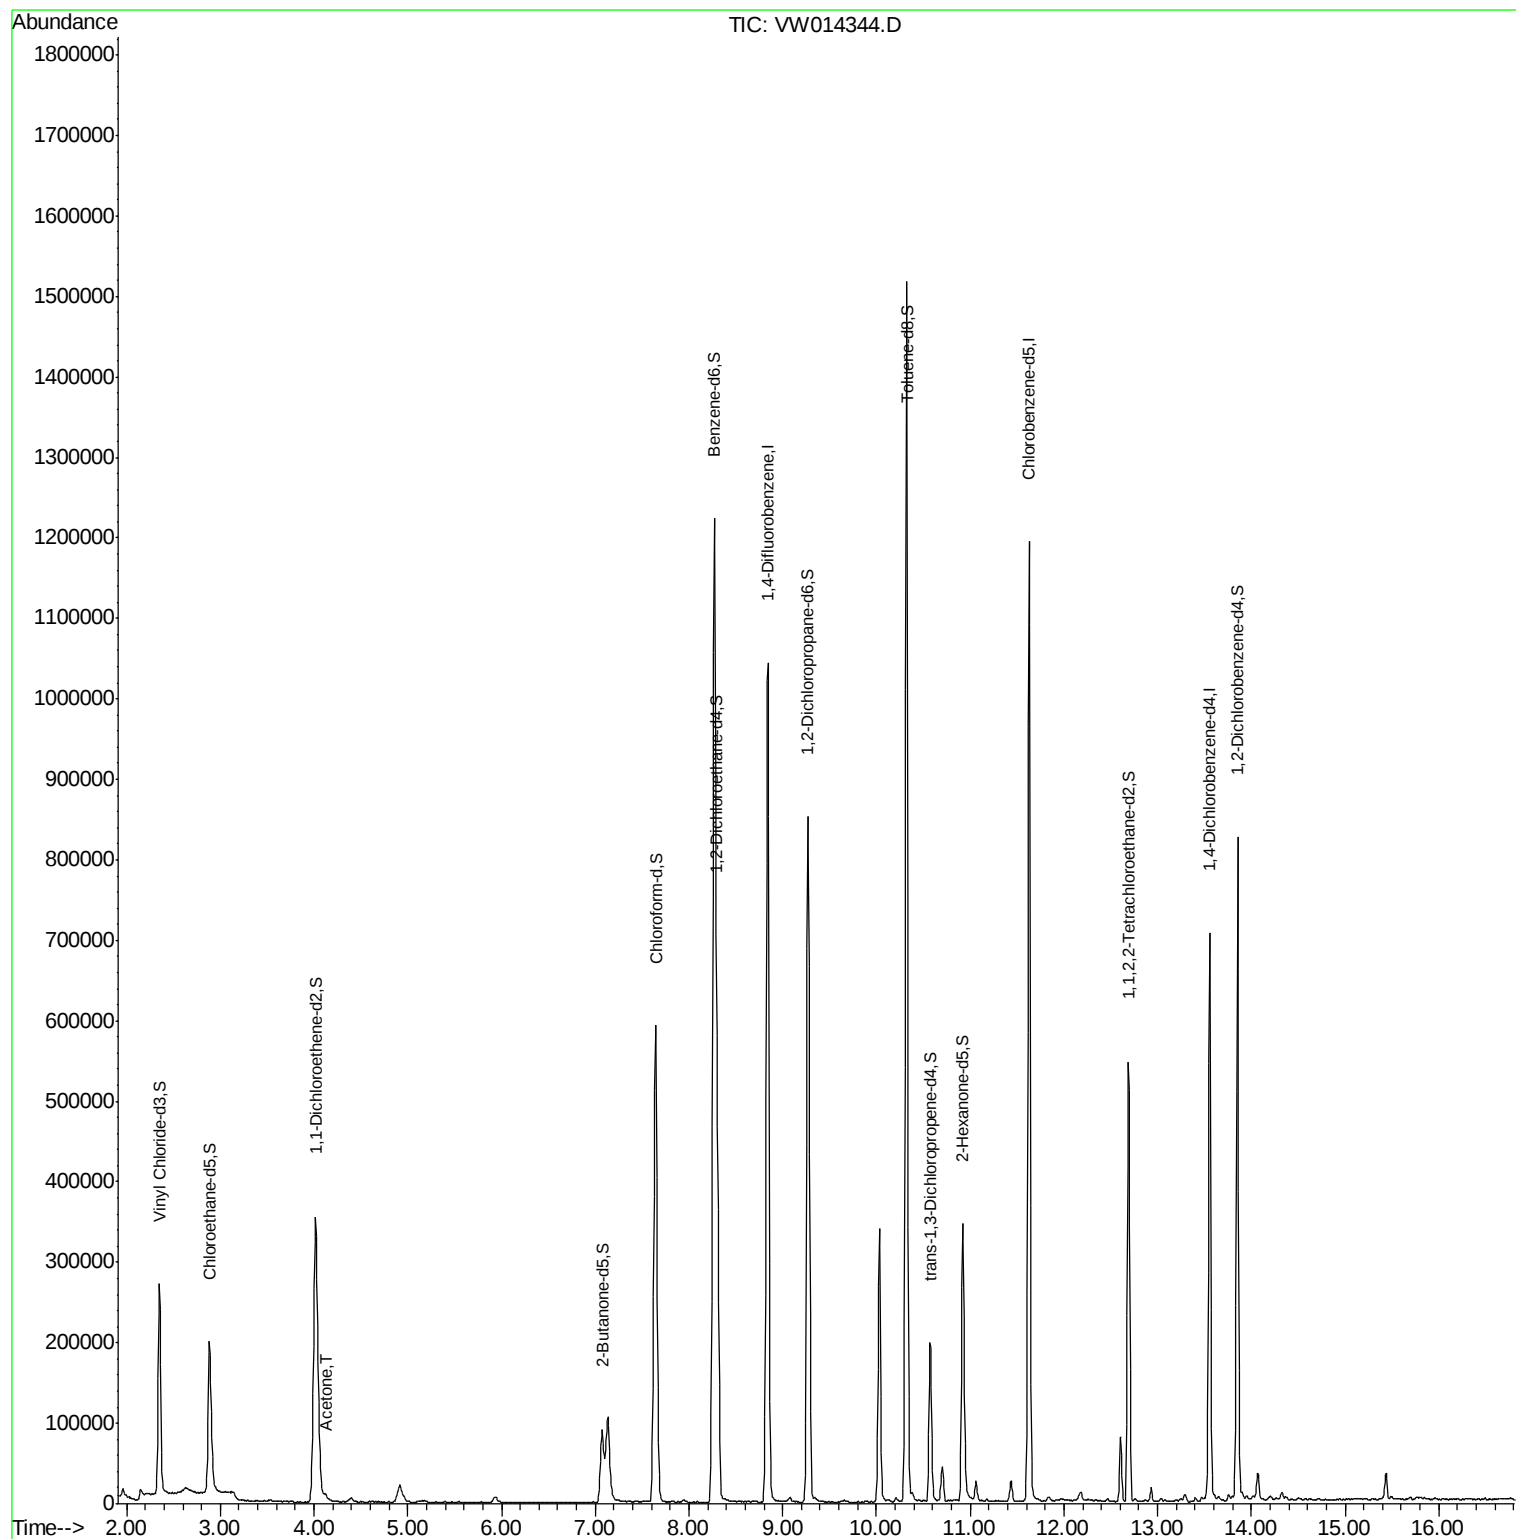

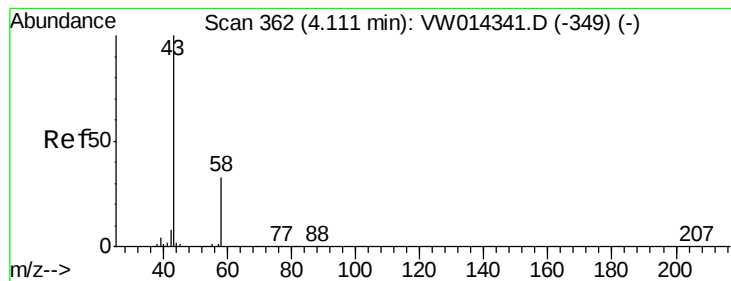

#13

Acetone

Concen: 4.050 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW014344.D

Acq: 13 Dec 2019 12:51

Instrument :

MSVOA_W

ClientSampleId :

C0C30RE

Tot Ion: 43 Resp: 13770

Ion Ratio Lower Upper

43 100

58 18.2 0.0 65.4

