


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW121418\
 Data File : VW007433.D
 Acq On : 12 Dec 2018 10:21
 Operator : SY/AP
 Sample : BFB86
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB86

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
 Title : VOC Analysis
 Last Update : Thu Dec 13 00:38:14 2018

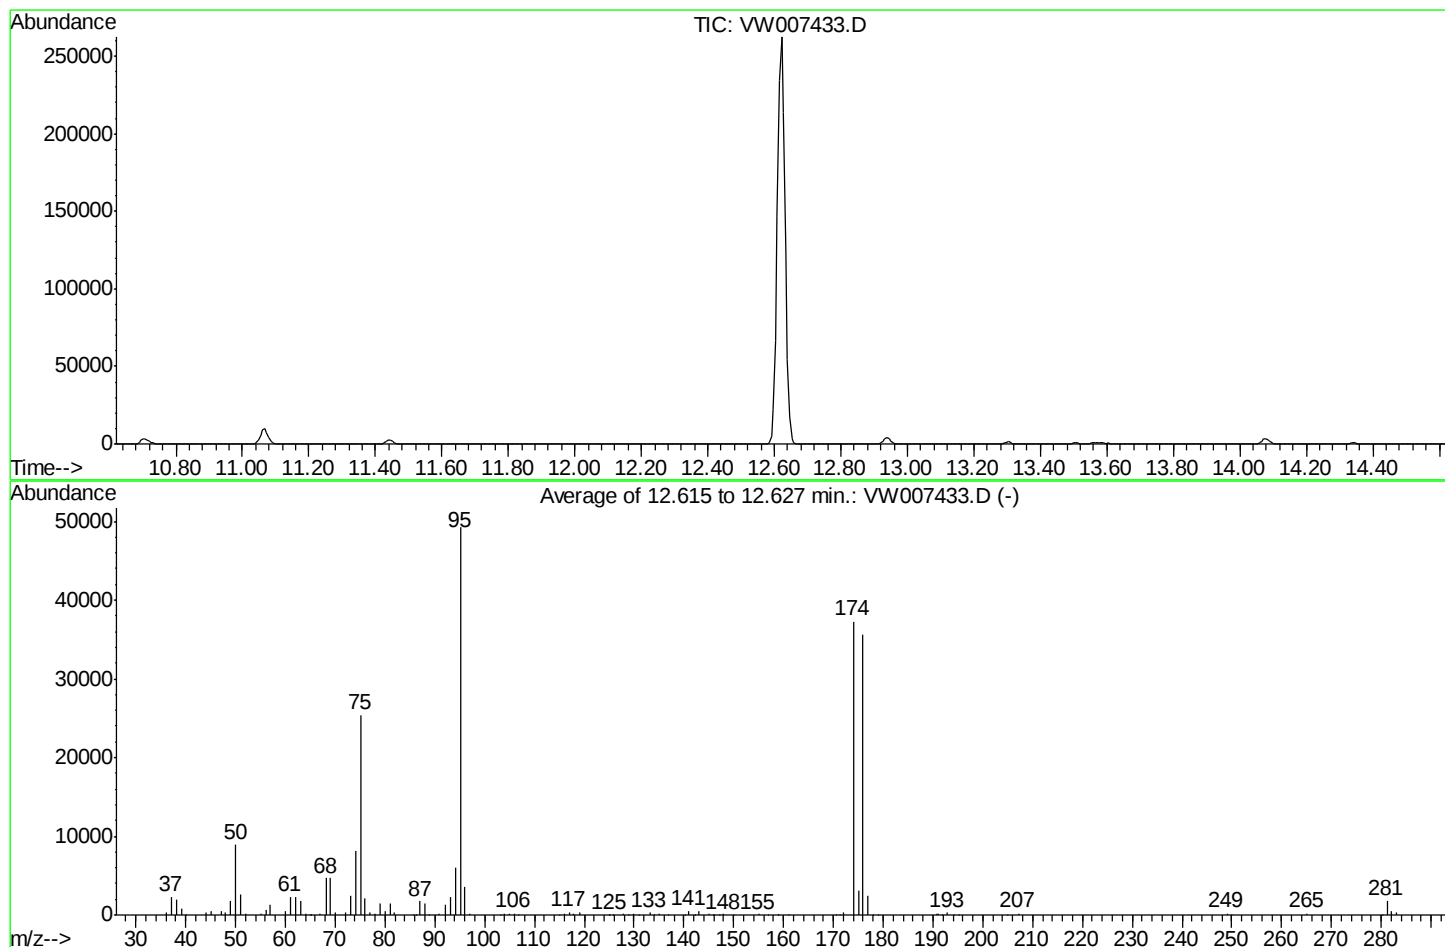

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	8890	PASS
75	95	30	80	51.5	25384	PASS
95	95	100	100	100.0	49258	PASS
96	95	5	9	7.3	3587	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.7	37293	PASS
175	174	5	9	8.4	3151	PASS
176	174	95	101	95.6	35648	PASS
177	176	5	9	6.6	2364	PASS

m/z	Abundance
36.00	269.0
37.10	2004.0
38.10	1933.0
39.00	551.0
40.10	76.0
44.00	239.0
45.10	307.0
47.10	429.0
48.10	316.0
49.00	1399.0
50.10	6961.0
51.10	2166.0
52.00	133.0
54.90	73.0
56.00	584.0
57.00	1217.0
60.00	422.0
61.00	2045.0
62.00	1938.0
63.10	1541.0
64.00	168.0
67.10	107.0
68.10	3823.0
69.10	4004.0
70.00	372.0
71.90	256.0
73.10	1885.0
74.00	7007.0
75.10	22280.0
76.10	1916.0
77.00	277.0
78.00	147.0
78.90	1316.0
80.00	420.0
80.90	1437.0
81.90	253.0
86.20	51.0
87.00	1577.0
88.10	1371.0
91.00	154.0
92.00	1215.0
93.00	1972.0
94.10	5310.0
95.10	44160.0
96.10	3142.0
97.00	103.0
103.90	225.0
104.90	51.0
105.90	230.0
114.90	52.0
116.00	176.0
116.90	409.0
117.90	236.0
118.90	226.0
125.10	79.0
127.90	169.0
128.80	63.0
129.80	120.0
130.80	92.0
133.10	208.0
135.00	96.0
137.00	80.0
140.00	98.0
141.00	534.0
142.10	75.0
143.00	572.0
144.90	72.0
145.70	61.0
147.90	128.0
150.10	50.0
155.00	146.0
156.80	68.0
158.90	71.0
170.50	55.0
172.10	290.0
174.00	36160.0
175.00	3197.0
176.00	35376.0
177.00	2309.0
190.90	92.0
191.20	101.0
192.90	136.0
194.10	53.0
207.20	119.0
249.10	112.0
265.10	147.0
281.10	1197.0
282.00	460.0
283.00	184.0

Instrument :
MSVOA_W
ClientSampleId :
BFB86

m/z	Abundance
44.20	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB86

m/z	Abundance
36.10	437.0
37.00	2467.0
38.10	2022.0
39.10	934.0
40.00	61.0
44.10	364.0
45.10	479.0
47.00	634.0
48.00	406.0
49.00	2110.0
50.10	9521.0
51.00	2494.0
52.20	140.0
55.10	139.0
56.10	749.0
57.00	1398.0
60.10	404.0
61.00	2311.0
62.10	2465.0
63.00	1884.0
64.10	204.0
64.90	72.0
65.20	80.0
67.00	203.0
68.10	4954.0
69.10	4862.0
70.10	389.0
72.20	247.0
73.10	2591.0
74.10	8168.0
75.10	25848.0
76.00	2098.0
76.90	289.0
77.90	283.0
79.00	1622.0
79.90	449.0
81.00	1473.0
81.90	330.0
85.80	66.0
87.00	2010.0
88.00	1545.0
91.00	168.0
92.00	1414.0
93.00	2437.0
94.10	6215.0
95.10	48928.0
96.10	3632.0
97.10	92.0
103.20	62.0
103.90	188.0
104.90	153.0
106.00	222.0
106.80	66.0
115.10	121.0
116.00	171.0
117.00	372.0
118.00	204.0
119.00	437.0
124.90	141.0
125.80	56.0
127.90	165.0
128.80	69.0
129.90	251.0
133.20	441.0
134.00	140.0
135.00	83.0
136.90	59.0
140.90	605.0
143.00	556.0
144.90	80.0
145.80	119.0
148.00	179.0
150.00	53.0
154.90	155.0
158.80	97.0
161.00	87.0
171.90	335.0
174.00	34368.0
175.10	2764.0
176.00	31656.0
177.00	2221.0
177.90	117.0
178.80	75.0
190.90	258.0
192.90	423.0
194.10	94.0
195.00	55.0
204.90	63.0
207.10	295.0
249.00	220.0
250.00	55.0
265.20	288.0

Instrument :
MSVOA_W
ClientSampleId :
BFB86

281.10	2322.0
282.10	700.0
283.10	520.0

Instrument :
MSVOA_W
ClientSampleId :
BFB86

m/z	Abundance
36.10	462.0
37.00	2363.0
38.10	2096.0
39.10	823.0
44.10	381.0
45.10	521.0
47.10	587.0
48.10	216.0
49.10	2076.0
50.10	10189.0
51.00	2991.0
52.00	116.0
55.00	161.0
56.10	701.0
57.10	1367.0
60.00	524.0
61.00	2670.0
62.10	2573.0
63.00	2033.0
64.00	130.0
65.10	107.0
67.10	216.0
68.10	5216.0
69.10	5513.0
70.00	346.0
72.00	371.0
73.00	2932.0
74.00	9076.0
75.10	28024.0
76.10	2494.0
77.00	296.0
77.90	241.0
79.00	1617.0
79.90	377.0
80.90	1671.0
81.90	379.0
85.70	54.0
87.00	1737.0
88.00	1574.0
88.80	64.0
90.80	229.0
92.00	1518.0
93.10	2461.0
94.10	6439.0
95.10	54688.0
96.10	3989.0
97.00	136.0
104.00	251.0
104.90	66.0
106.00	239.0
114.90	80.0
115.90	239.0
116.90	369.0
117.80	249.0
119.00	385.0
125.10	122.0
125.80	60.0
128.00	214.0
128.80	126.0
130.00	160.0
130.80	74.0
133.10	241.0
133.90	113.0
134.90	163.0
136.90	109.0
140.10	86.0
140.90	570.0
143.00	510.0
145.00	156.0
146.00	102.0
147.10	95.0
147.80	112.0
150.10	70.0
154.90	147.0
156.80	67.0
159.00	110.0
160.90	66.0
171.20	129.0
172.00	334.0
174.00	41352.0
175.10	3494.0
176.00	39912.0
177.00	2563.0
177.90	93.0
178.90	84.0
191.10	216.0
191.90	51.0
193.00	319.0
194.10	77.0
195.10	55.0
204.90	62.0
207.10	148.0

Instrument :
MSVOA_W
ClientSampleId :
BFB86

249.00	219.0
265.00	186.0
280.20	96.0
281.10	2097.0
282.10	471.0
283.00	306.0

Instrument :
MSVOA_W
ClientSampleId :
BFB86