


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121521\
 Data File : VW021380.D
 Acq On : 15 Dec 2021 09:47
 Operator : SY/VA
 Sample : BFB481
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB481

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Title : SFAM01.0
 Last Update : Sat Dec 18 00:55:20 2021

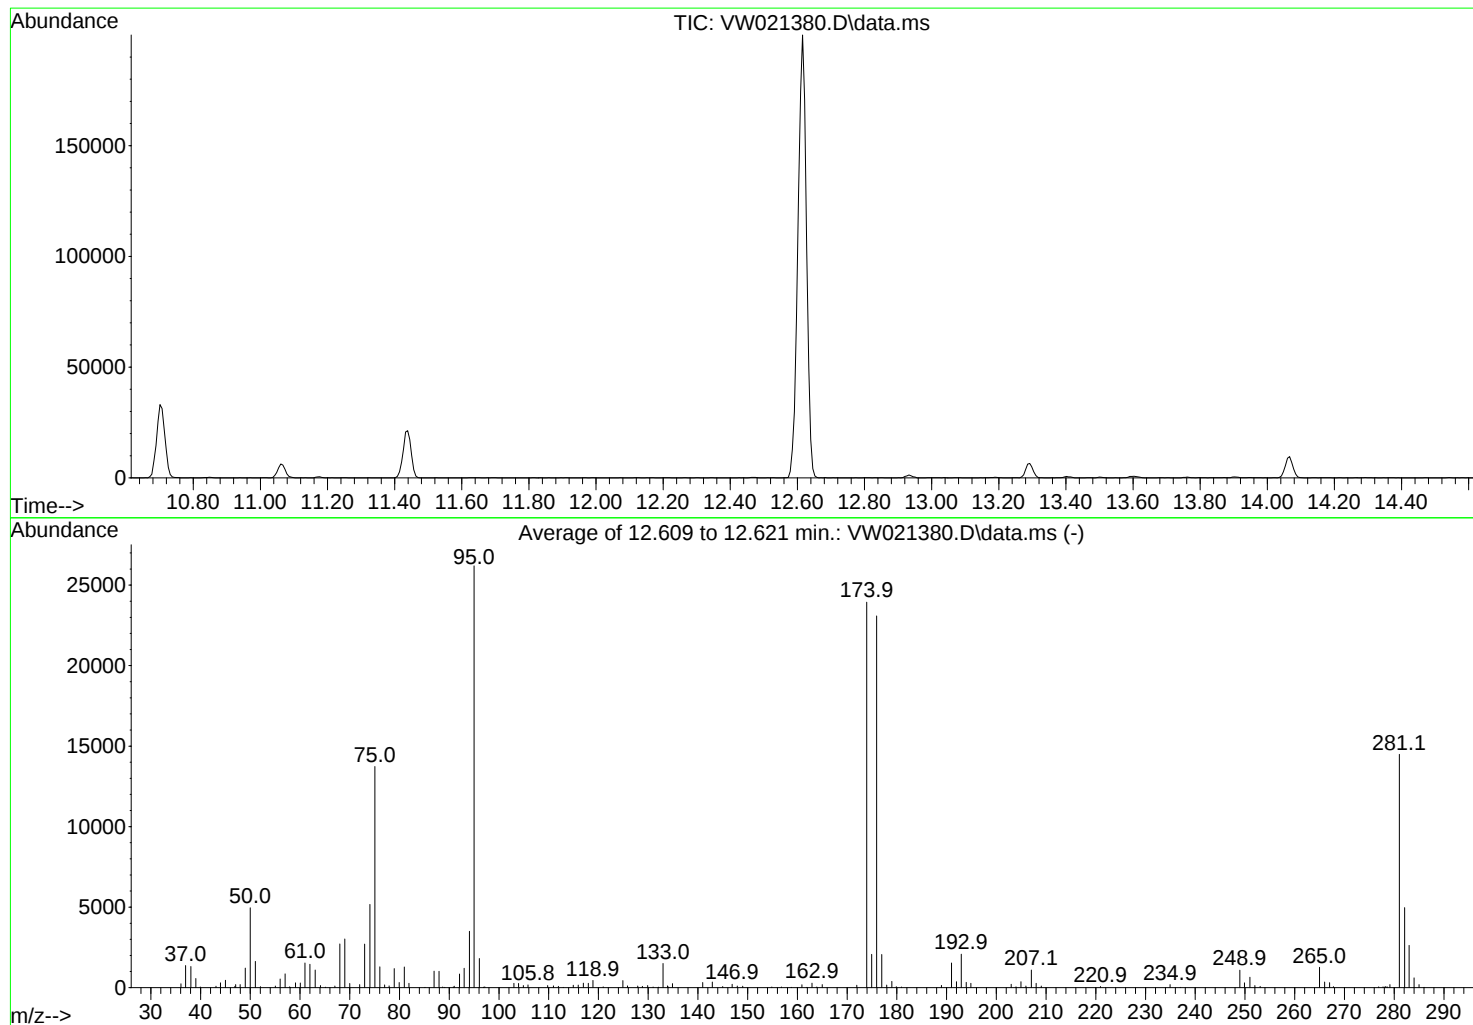

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	4960	PASS
75	95	30	80	52.4	13730	PASS
95	95	100	100	100.0	26197	PASS
96	95	5	9	6.9	1805	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.4	23939	PASS
175	174	5	9	8.6	2068	PASS
176	174	95	105	96.4	23085	PASS
177	176	5	10	8.9	2054	PASS

m/z	Abundance
73.00	64.0
281.10	187.0

Instrument :
MSVOA_W
ClientSampleId :
BFB481

m/z	Abundance
36.10	242.0
37.00	1095.0
38.00	1081.0
39.00	569.0
43.10	140.0
44.00	276.0
45.00	622.0
46.90	237.0
48.00	173.0
49.00	1098.0
50.00	4321.0
51.00	1503.0
52.00	103.0
55.00	90.0
55.90	470.0
57.00	804.0
57.90	70.0
59.10	454.0
60.10	287.0
61.00	1455.0
62.00	1212.0
63.10	1034.0
64.10	140.0
65.10	88.0
67.00	121.0
68.00	2273.0
69.00	2749.0
70.00	255.0
72.00	173.0
73.00	3643.0
74.00	4855.0
75.00	12233.0
76.10	1088.0
77.00	154.0
78.00	128.0
78.90	953.0
80.00	293.0
80.90	1202.0
81.90	216.0
85.10	69.0
86.90	967.0
87.90	766.0
88.70	111.0
90.80	113.0
92.00	679.0
93.00	1084.0
94.00	3095.0
95.00	22768.0
96.00	1653.0
97.10	87.0
103.00	486.0
104.00	229.0
104.90	140.0
105.80	157.0
109.80	148.0
110.90	149.0
112.10	83.0
115.00	213.0
116.00	148.0
116.90	284.0
117.90	309.0
118.90	465.0
121.00	91.0
125.00	700.0
125.90	247.0
127.90	74.0
128.90	62.0
129.80	121.0
131.00	111.0
132.10	80.0
133.00	2260.0
134.90	254.0
140.90	245.0
142.90	341.0
145.00	57.0
146.90	354.0
147.90	115.0
149.00	127.0
158.80	70.0
160.90	235.0
161.90	72.0
162.90	397.0
163.90	109.0
165.00	283.0
172.10	133.0
174.00	17368.0
175.00	1669.0
176.00	17864.0
177.00	2114.0
178.00	192.0
179.00	541.0
180.00	91.0

Instrument :
MSVOA_W
ClientSampleId :
BFB481

181.00	64.0
189.00	197.0
191.00	2301.0
192.00	524.0
192.90	3082.0
193.90	467.0
194.90	425.0
203.00	329.0
203.90	90.0
205.00	505.0
205.90	149.0
207.00	1613.0
208.00	427.0
209.10	137.0
220.90	147.0
234.90	229.0
237.00	54.0
249.00	1343.0
249.90	466.0
251.00	909.0
252.00	203.0
253.10	70.0
265.00	1567.0
266.00	524.0
267.00	390.0
267.80	78.0
276.90	70.0
277.80	83.0
278.10	134.0
278.60	150.0
279.10	250.0
281.00	17736.0
282.10	6236.0
283.00	3776.0
284.00	1011.0
285.00	255.0
286.00	60.0

Instrument :
MSVOA_W
ClientSampleId :
BFB481

m/z	Abundance
36.00	270.0
37.00	1618.0
38.00	1475.0
39.00	598.0
39.90	62.0
43.10	83.0
44.00	352.0
45.00	444.0
47.10	322.0
47.90	173.0
49.00	1262.0
50.00	5755.0
51.00	1822.0
52.10	72.0
55.00	83.0
56.00	618.0
57.00	938.0
57.90	67.0
59.10	283.0
60.00	318.0
61.00	1729.0
62.00	1613.0
63.10	1256.0
64.10	124.0
67.10	114.0
68.00	2972.0
69.00	3381.0
70.00	257.0
72.00	211.0
73.00	2818.0
74.00	5708.0
75.00	15288.0
76.00	1509.0
77.00	163.0
77.90	91.0
79.00	1404.0
79.90	336.0
81.00	1391.0
81.90	315.0
87.00	962.0
87.90	1129.0
89.10	54.0
91.00	141.0
92.00	1028.0
93.00	1335.0
94.10	3783.0
95.00	29376.0
96.10	2155.0
97.20	54.0
103.00	226.0
103.90	306.0
104.90	130.0
105.80	176.0
109.80	159.0
111.00	120.0
111.90	82.0
112.90	56.0
114.90	120.0
115.90	140.0
117.00	276.0
117.90	272.0
118.90	538.0
120.90	54.0
124.90	339.0
127.90	133.0
128.80	89.0
129.90	141.0
133.00	1424.0
133.90	319.0
134.90	297.0
141.00	346.0
142.90	361.0
144.90	79.0
146.90	192.0
147.90	111.0
149.00	133.0
154.90	59.0
156.80	59.0
160.90	154.0
163.00	286.0
165.00	198.0
171.90	200.0
173.90	27784.0
174.90	2176.0
175.90	25320.0
177.00	2113.0
177.90	180.0
179.00	434.0
179.80	86.0
180.90	68.0
188.90	151.0
191.00	1488.0

Instrument :
MSVOA_W
ClientSampleId :
BFB481

192.00	384.0
193.00	2127.0
194.00	366.0
194.90	268.0
203.00	173.0
204.00	51.0
204.90	410.0
206.00	155.0
207.10	1091.0
208.00	253.0
209.00	162.0
221.00	60.0
235.00	209.0
248.90	1325.0
249.90	290.0
251.00	718.0
252.10	109.0
253.00	89.0
265.00	1406.0
266.00	426.0
267.00	375.0
267.80	97.0
276.90	87.0
277.70	69.0
278.30	149.0
279.20	213.0
281.10	14720.0
282.10	6005.0
283.00	2759.0
284.00	524.0
285.00	196.0

Instrument :
MSVOA_W
ClientSampleId :
BFB481

m/z	Abundance
36.00	201.0
37.00	1390.0
38.10	1374.0
39.10	533.0
40.00	51.0
43.00	58.0
44.00	280.0
45.00	301.0
47.00	260.0
47.90	219.0
49.00	1263.0
50.00	4803.0
51.00	1578.0
55.10	130.0
56.10	528.0
57.00	811.0
58.10	65.0
59.10	150.0
60.00	275.0
61.00	1404.0
62.00	1530.0
63.00	995.0
64.10	121.0
66.90	60.0
68.00	2898.0
69.00	2928.0
70.00	264.0
72.00	192.0
73.10	1831.0
74.10	4936.0
75.10	13669.0
76.00	1293.0
77.00	177.0
77.80	97.0
78.90	1189.0
79.90	339.0
80.90	1256.0
81.90	288.0
86.90	1154.0
88.00	1158.0
91.00	142.0
92.10	818.0
93.00	1200.0
94.00	3627.0
95.00	26448.0
96.00	1608.0
96.90	81.0
102.80	91.0
103.90	249.0
104.90	106.0
105.90	163.0
109.90	89.0
110.90	56.0
111.90	71.0
114.90	130.0
115.90	176.0
116.90	277.0
118.00	226.0
118.90	337.0
124.80	260.0
125.70	69.0
127.90	83.0
128.90	88.0
130.00	133.0
132.90	822.0
134.10	134.0
134.90	184.0
140.90	365.0
142.90	332.0
145.10	67.0
146.90	85.0
147.90	87.0
154.80	73.0
156.80	73.0
160.90	140.0
162.90	167.0
164.90	82.0
171.90	130.0
173.90	26664.0
175.00	2359.0
175.90	26072.0
176.90	1936.0
177.90	110.0
179.00	178.0
189.10	66.0
191.00	809.0
192.00	204.0
193.00	1019.0
194.00	139.0
194.90	119.0
202.90	125.0
204.90	195.0

Instrument :
MSVOA_W
ClientSampleId :
BFB481

207.00	578.0
207.90	129.0
234.90	126.0
248.90	592.0
250.00	135.0
250.90	298.0
251.90	81.0
253.00	75.0
265.00	808.0
266.00	89.0
267.00	161.0
278.30	65.0
279.20	114.0
281.10	11565.0
282.00	2682.0
283.00	1328.0
284.10	294.0
285.00	111.0

Instrument :
MSVOA_W
ClientSampleId :
BFB481