

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121523\
 Data File : VW027678.D
 Acq On : 16 Dec 2023 09:21
 Operator : SY/MD
 Sample : 05806-09
 Misc : 4.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 52 Sample Multiplier: 1

Quant Time: Dec 16 22:56:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 16 04:21:48 2023
 Response via : Initial Calibration


Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	287659	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	167949	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	34584	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.363	65	128490	31.540	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 126.160%		
7) Chloroethane-d5		2.899	69	104944	33.085	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 132.320%		
11) 1,1-Dichloroethene-d2		4.021	65	42680	26.158	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 104.640%		
21) 2-Butanone-d5		7.081	46	43901	63.283	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 126.560%		
24) Chloroform-d		7.648	84	187997	27.465	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 109.880%		
26) 1,2-Dichloroethane-d4		8.307	65	88800	27.630	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 110.520%		
32) Benzene-d6		8.276	84	382604	38.980	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 155.920%#		
36) 1,2-Dichloropropane-d6		9.270	67	112241	40.363	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 161.440%#		
41) Toluene-d8		10.319	98	267444	29.367	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 117.480%		
43) trans-1,3-Dichloroprop...		10.575	79	25802	23.965	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 95.880%		
47) 2-Hexanone-d5		10.922	63	29151	71.935	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 143.860%#		
56) 1,1,2,2-Tetrachloroeth...		12.690	84	70114	33.341	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 133.360%#		
66) 1,2-Dichlorobenzene-d4		13.848	152	39168	31.639	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 126.560%#		
Target Compounds							Qvalue
14) Carbon disulfide		4.387	76	6960	0.588	ug/L	97
16) Methylene chloride		4.923	84	18865	4.183	ug/L	90
39) cis-1,3-Dichloropropene		10.032	75	2195	0.613	ug/L #	72
46) Tetrachloroethene		10.861	164	3671	1.732	ug/L	86
49) Dibromochloromethane		10.855	129	3492	1.919	ug/L #	10

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121523\
Data File : VW027678.D
Acq On : 16 Dec 2023 09:21
Operator : SY/MD
Sample : 05806-09
Misc : 4.12g/10mL/MSVOA_W/SOIL
ALS Vial : 52 Sample Multiplier: 1





Quant Time: Dec 16 22:56:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 16 04:21:48 2023
Response via : Initial Calibration

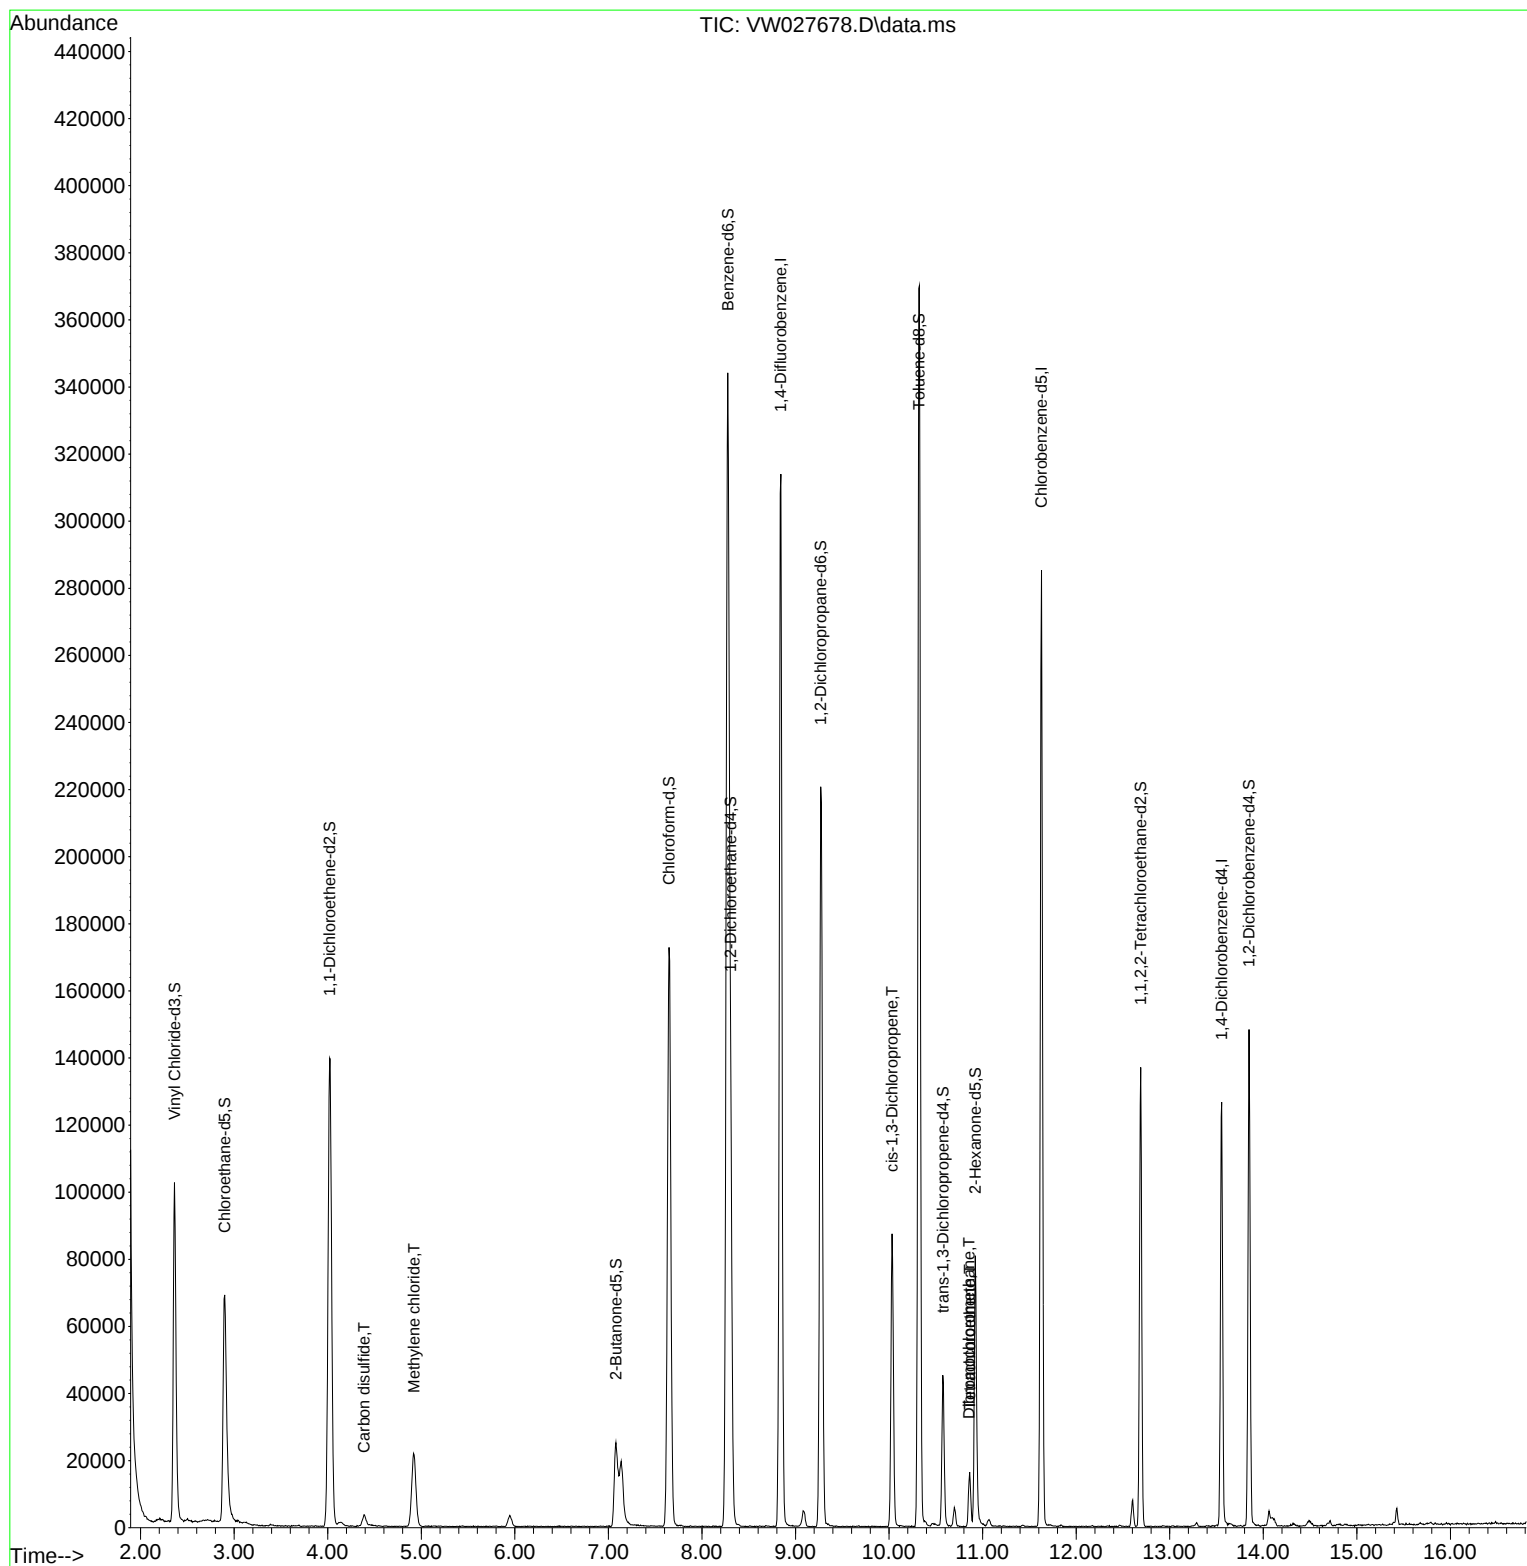

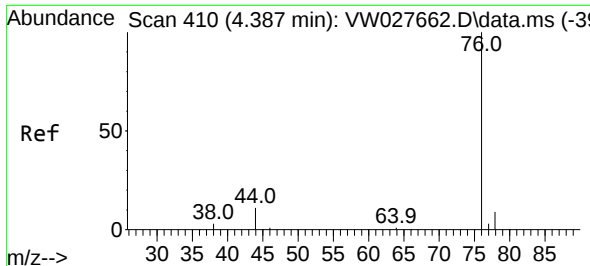




#14
Carbon disulfide
Concen: 0.588 ug/L
RT: 4.387 min Scan# 410
Delta R.T. -0.000 min
Lab File: VW027678.D
Acq: 16 Dec 2023 09:21


Tgt Ion: 76 Resp: 6960
Ion Ratio Lower Upper
76 100
78 7.8 7.0 10.6

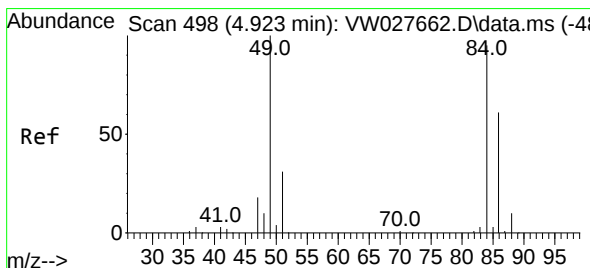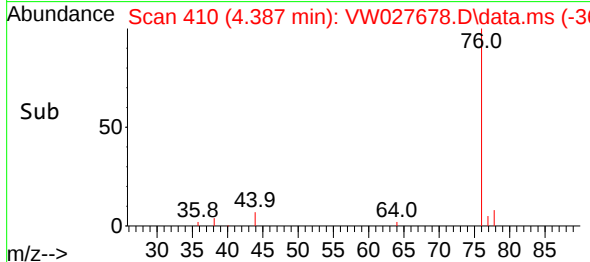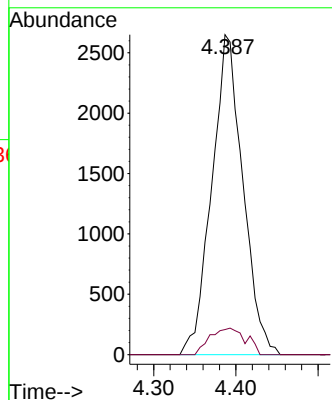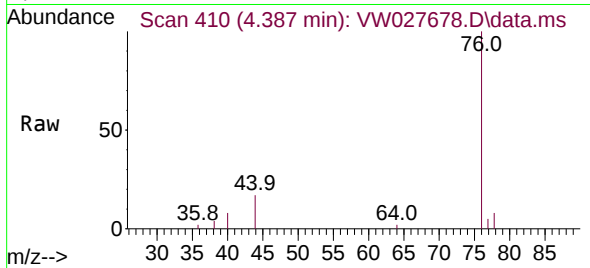

#16
Methylene chloride
Concen: 4.183 ug/L
RT: 4.923 min Scan# 498
Delta R.T. -0.000 min
Lab File: VW027678.D
Acq: 16 Dec 2023 09:21





Tgt Ion: 84 Resp: 18865
Ion Ratio Lower Upper
84 100
86 57.1 45.8 85.2
49 99.0 76.2 141.6

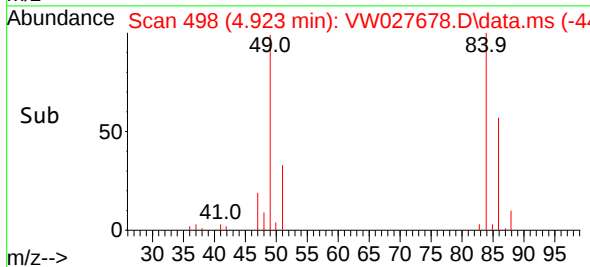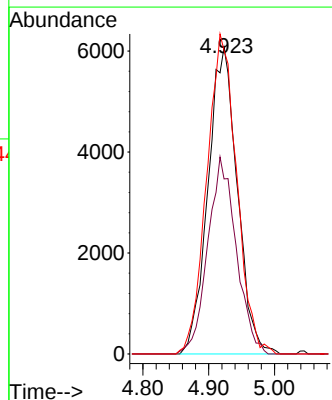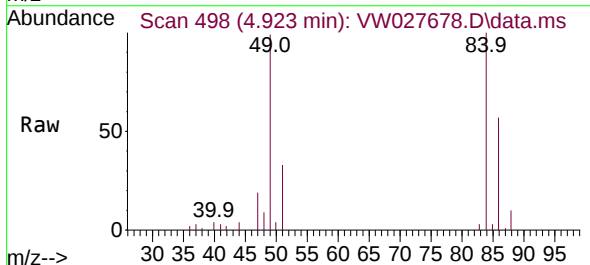

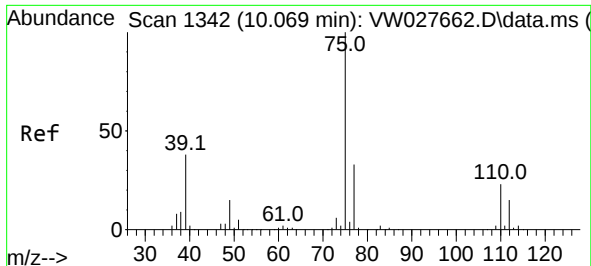




#39
cis-1,3-Dichloropropene
Concen: 0.613 ug/L
RT: 10.032 min Scan# 1336
Delta R.T. -0.037 min
Lab File: VW027678.D
Acq: 16 Dec 2023 09:21


Tgt Ion: 75 Resp: 2195
Ion Ratio Lower Upper
75 100
77 46.9 21.8 40.6#

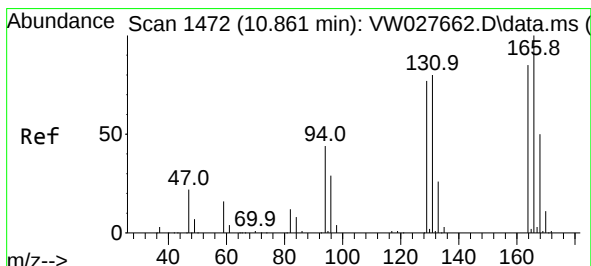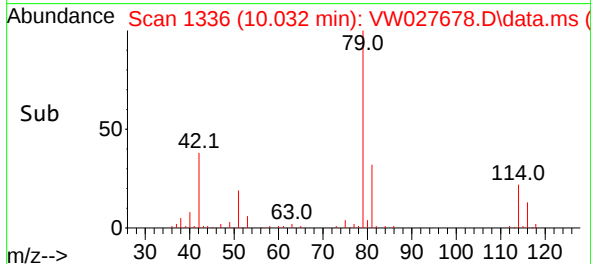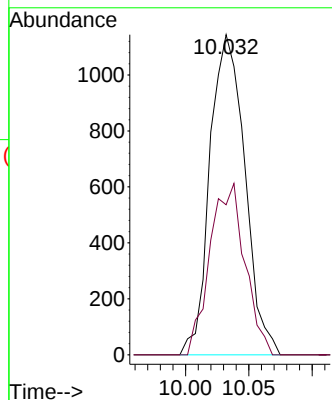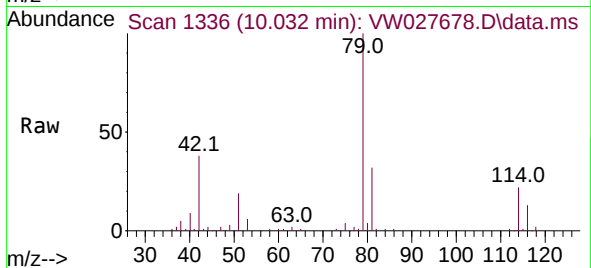

#46
Tetrachloroethene
Concen: 1.732 ug/L
RT: 10.861 min Scan# 1472
Delta R.T. -0.000 min
Lab File: VW027678.D
Acq: 16 Dec 2023 09:21

Tgt Ion:164 Resp: 3671
Ion Ratio Lower Upper
164 100
129 81.5 70.5 130.9
131 93.5 64.8 120.3
166 111.7 94.8 176.0

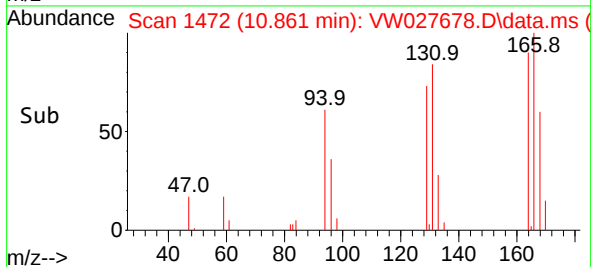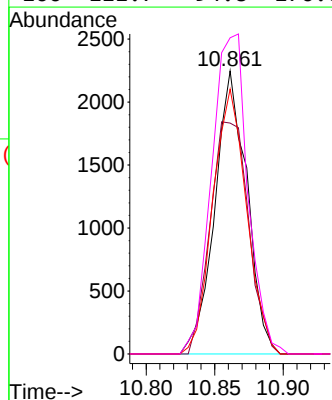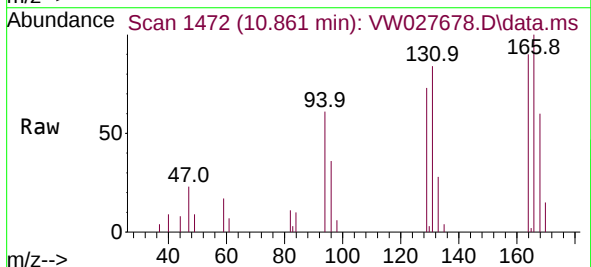

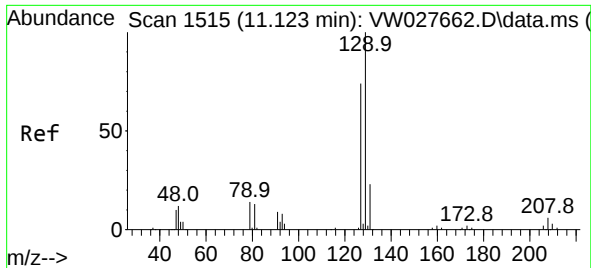

#49
Dibromochloromethane
Concen: 1.919 ug/L
RT: 10.855 min Scan# 1471
Delta R.T. -0.268 min
Lab File: VW027678.D
Acq: 16 Dec 2023 09:21

Tgt Ion:129 Resp: 3492
Ion Ratio Lower Upper
129 100
127 0.0 55.4 102.8#

