

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121523\
 Data File : VW027707.D
 Acq On : 16 Dec 2023 22:52
 Operator : SY/MD
 Sample : 05836-09
 Misc : 4.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Dec 17 03:41:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	593622	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	519097	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	249550	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	188638	22.438	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.760%
7) Chloroethane-d5	2.899	69	149645	22.861	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.440%
11) 1,1-Dichloroethene-d2	4.021	65	73085	21.706	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.840%
21) 2-Butanone-d5	7.093	46	59652	41.669	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.340%
24) Chloroform-d	7.654	84	321391	22.753	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.000%
26) 1,2-Dichloroethane-d4	8.307	65	150022	22.620	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.480%
32) Benzene-d6	8.276	84	709666	23.392	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.560%
36) 1,2-Dichloropropane-d6	9.270	67	198375	23.080	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.320%
41) Toluene-d8	10.325	98	648672	23.046	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	10.575	79	70628	21.224	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.880%
47) 2-Hexanone-d5	10.922	63	57542	45.941	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.880%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	140605	21.632	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.520%
66) 1,2-Dichlorobenzene-d4	13.848	152	201498	22.557	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.240%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	4809	0.434	ug/L	# 63

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121523\
Data File : VW027707.D
Acq On : 16 Dec 2023 22:52
Operator : SY/MD
Sample : 05836-09
Misc : 4.93g/10mL/MSVOA_W/SOIL
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Dec 17 03:41:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

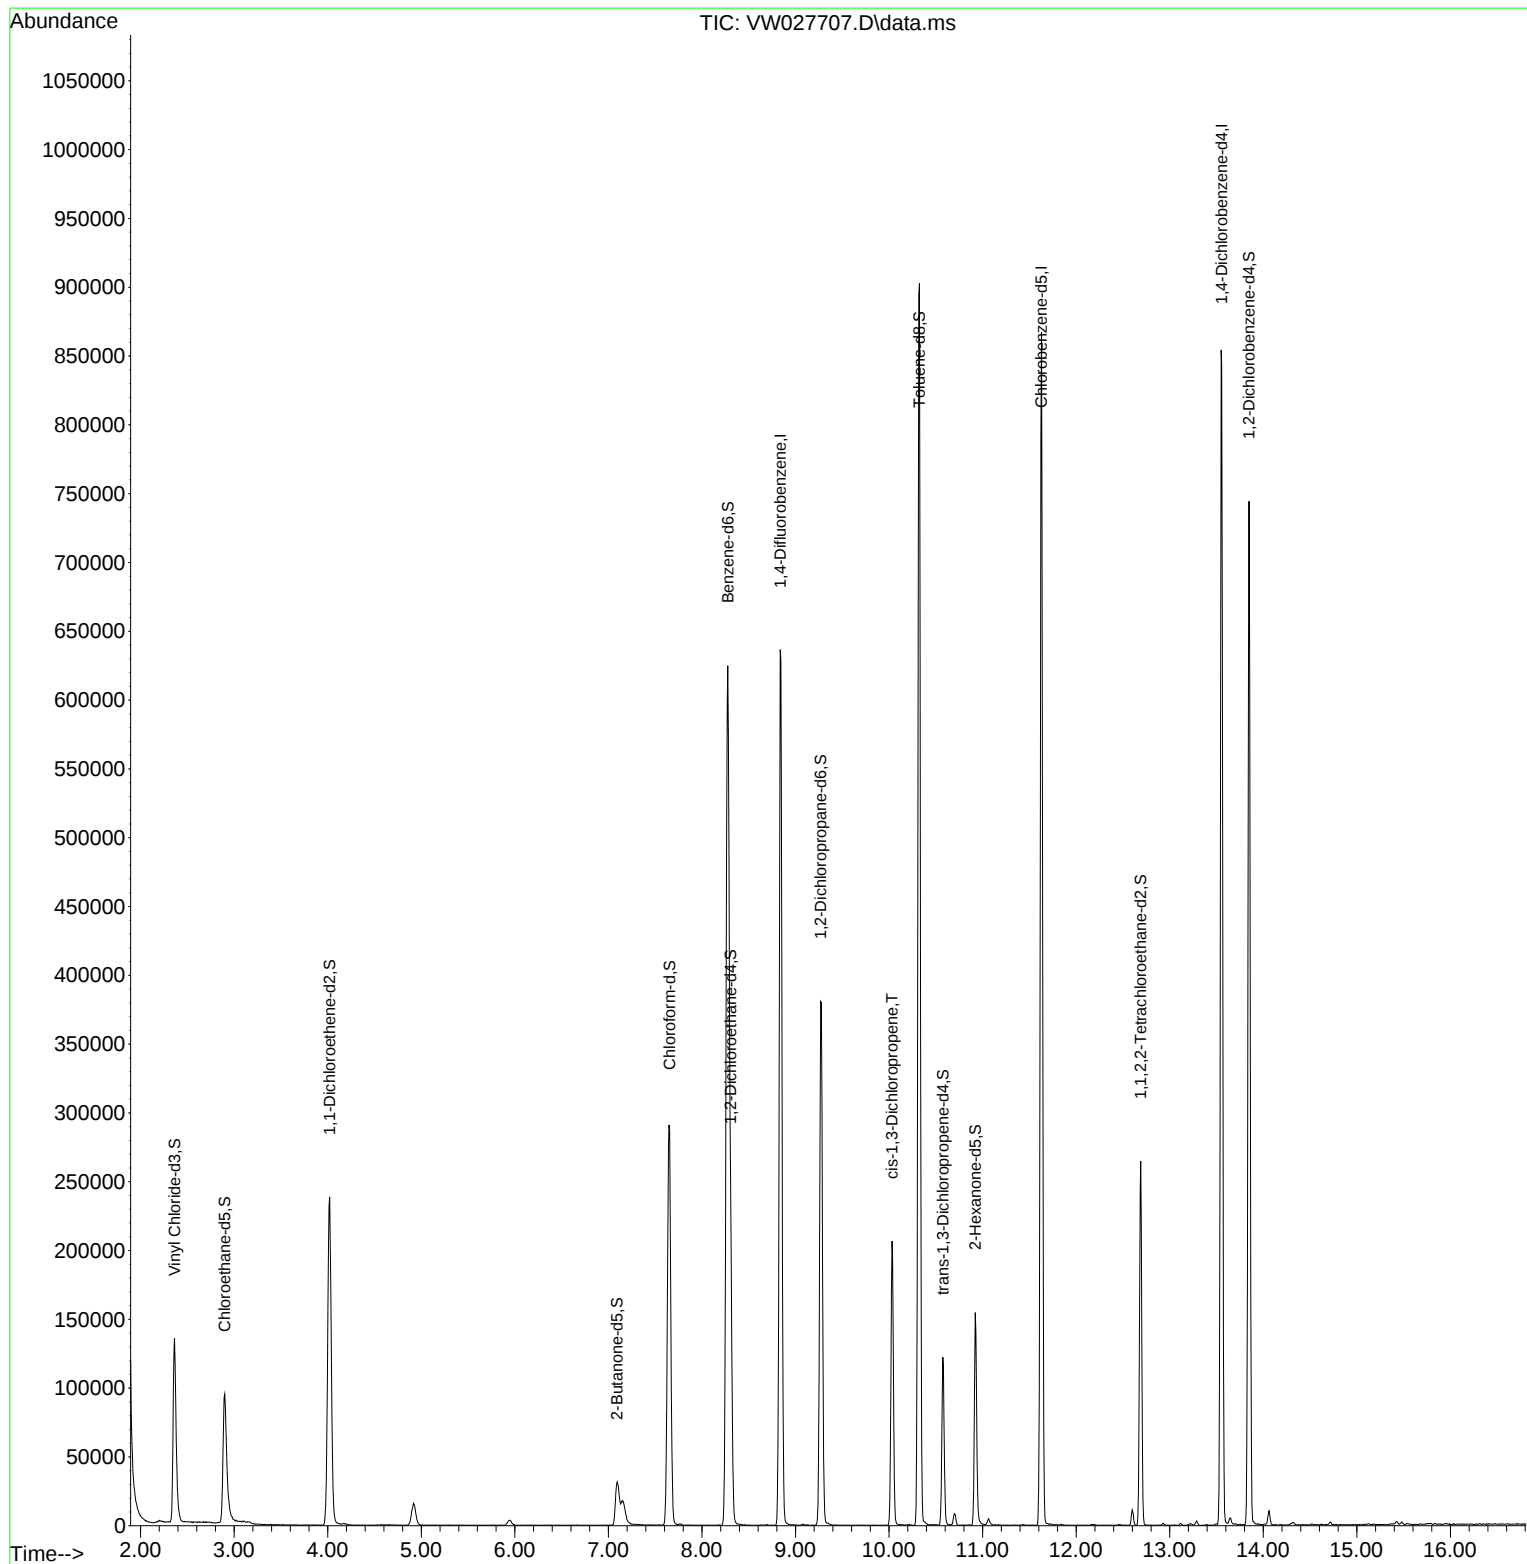

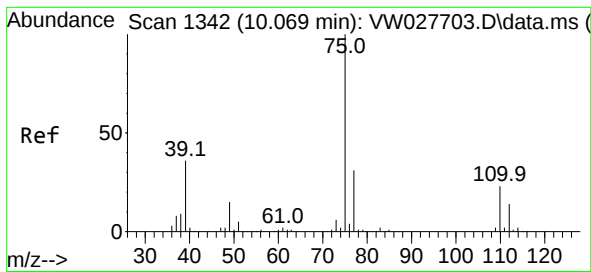

#39
 cis-1,3-Dichloropropene
 Concen: 0.434 ug/L
 RT: 10.032 min Scan# 1336
 Delta R.T. -0.037 min
 Lab File: VW027707.D
 Acq: 16 Dec 2023 22:52

Tgt Ion: 75 Resp: 4809
 Ion Ratio Lower Upper
 75 100
 77 51.4 21.8 40.6#

