




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121523\
Data File : VW027656.D
Acq On : 15 Dec 2023 23:54
Operator : SY/MD
Sample : 05834-13
Misc : 5.87g/10mL/MSVOA_W/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGR26

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/17/2023
Supervised By :Semsettin Yesilyurt 12/17/2023

Quant Time: Dec 16 01:42:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 16 00:05:51 2023
Response via : Initial Calibration

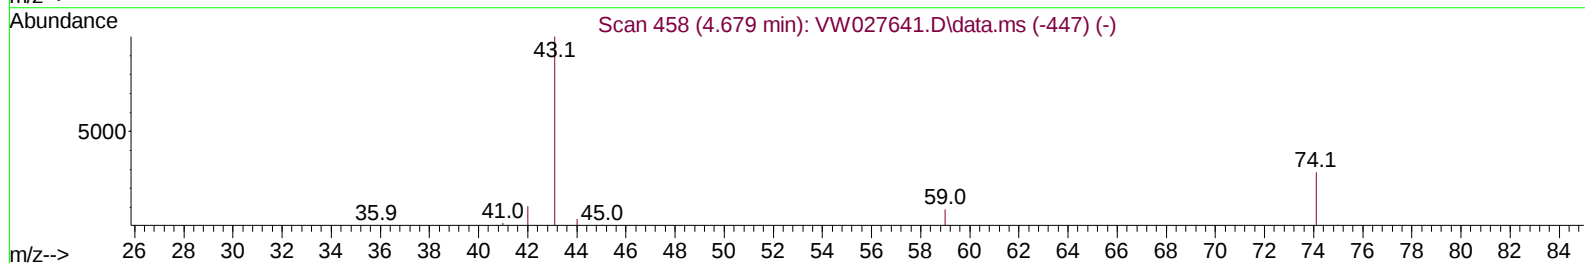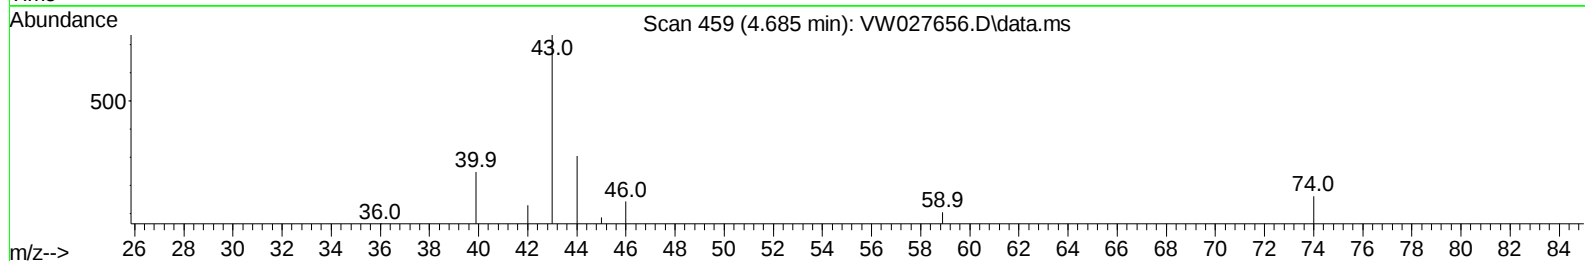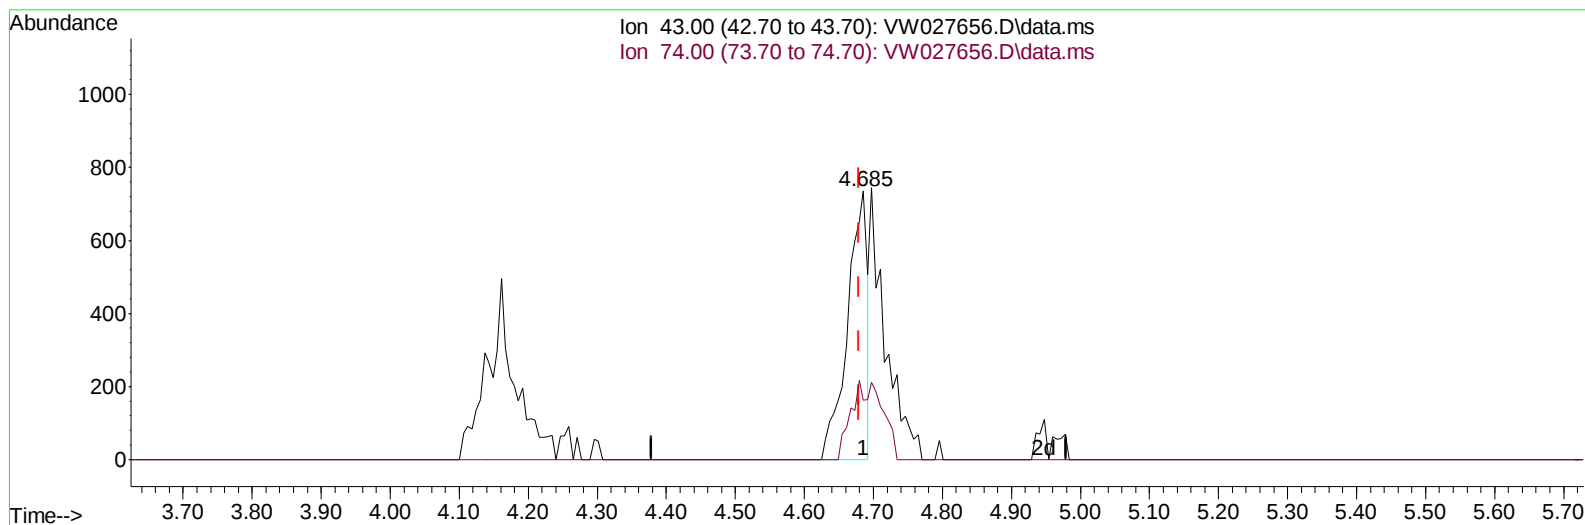

TIC: VW027656.D\data.ms

(15) Methyl Acetate (T)

4.685min (+ 0.006) 0.64 ug/L

response 1461

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.60	20.33#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121523\
Data File : VW027656.D
Acq On : 15 Dec 2023 23:54
Operator : SY/MD
Sample : 05834-13
Misc : 5.87g/10mL/MSVOA_W/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGR26

Manual IntegrationsAPPROVED

Quant Time: Dec 16 01:42:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 16 00:05:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/17/2023
Supervised By :Semsettin Yesilyurt 12/17/2023

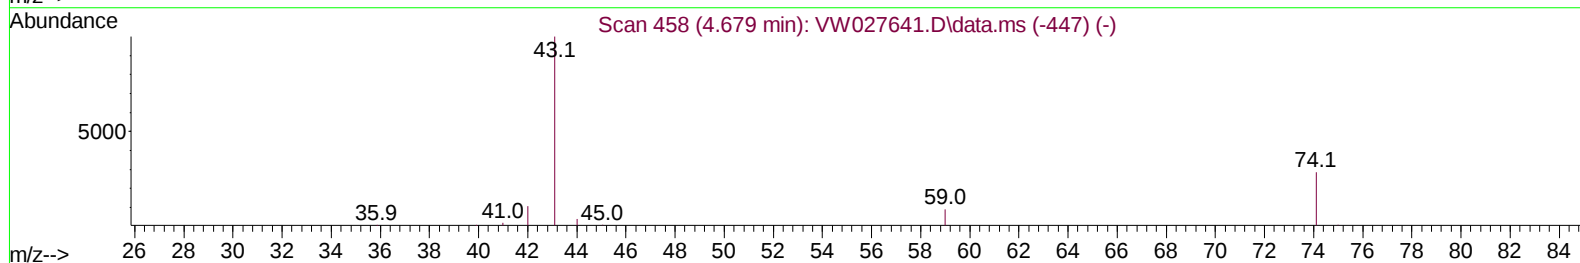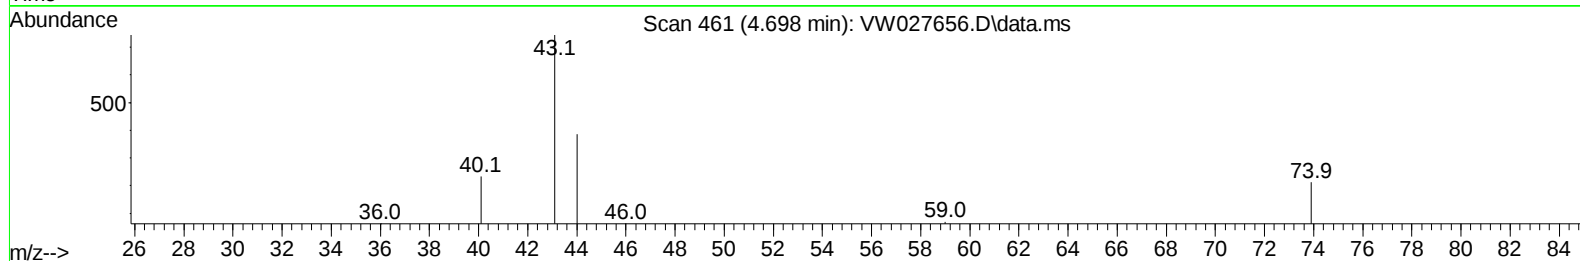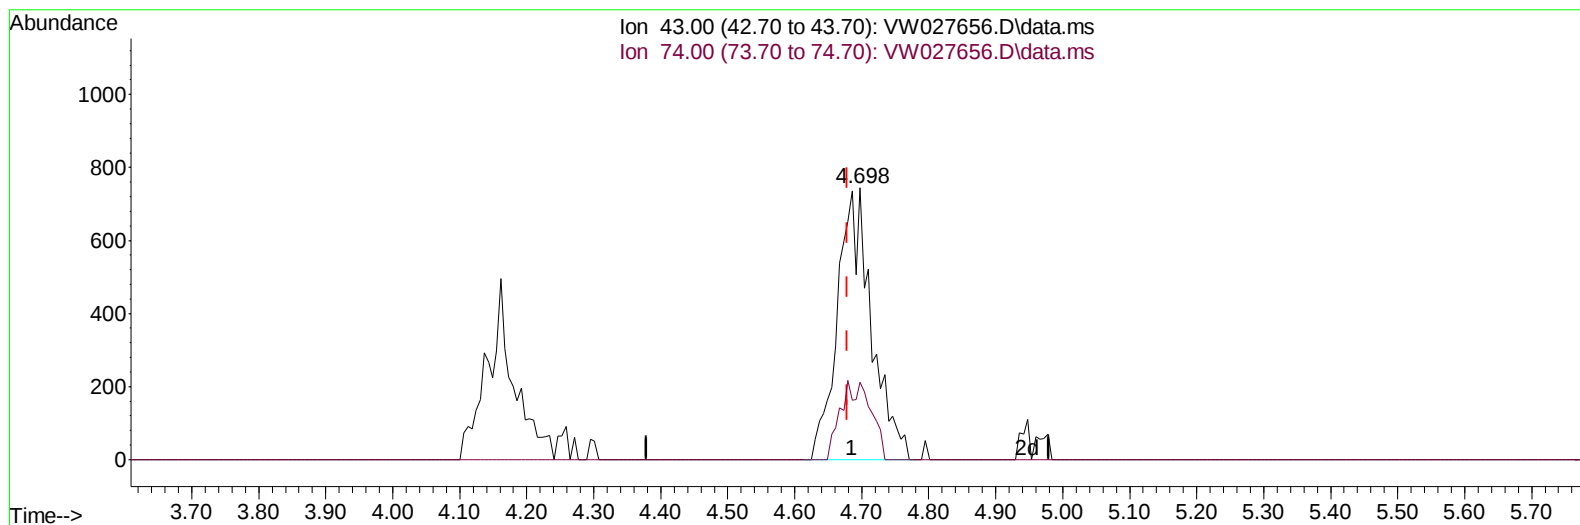

TIC: VW027656.D\data.ms

(15) Methyl Acetate (T)

4.698min (+ 0.018) 1.14 ug/L m

response 2612

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.60	11.37#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121523\
 Data File : VW027656.D
 Acq On : 15 Dec 2023 23:54
 Operator : SY/MD
 Sample : 05834-13
 Misc : 5.87g/10mL/MSVOA_W/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGR26

Manual IntegrationsAPPROVED

Quant Time: Dec 16 01:42:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 16 00:05:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/17/2023
 Supervised By :Semsettin Yesilyurt 12/17/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		577329	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		467816	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		173019	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		206526	25.259	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	101.040%	
7) Chloroethane-d5	2.899	69		169857	26.682	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	106.720%	
11) 1,1-Dichloroethene-d2	4.021	65		79161	24.174	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	96.680%	
21) 2-Butanone-d5	7.087	46		40939	29.404	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	58.800%	
24) Chloroform-d	7.648	84		351872	25.614	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	102.440%	
26) 1,2-Dichloroethane-d4	8.307	65		169395	26.262	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	105.040%	
32) Benzene-d6	8.276	84		786090	28.752	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	115.000%	
36) 1,2-Dichloropropane-d6	9.276	67		226724	29.270	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	117.080%	
41) Toluene-d8	10.319	98		629994	24.835	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	99.360%	
43) trans-1,3-Dichloroprop...	10.575	79		72604	24.210	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	96.840%	
47) 2-Hexanone-d5	10.922	63		39021	34.569	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	69.140%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		137371	23.451	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	93.800%	
66) 1,2-Dichlorobenzene-d4	13.848	152		142952	23.082	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	92.320%	
Target Compounds							
15) Methyl Acetate	4.698	43		2612m	1.144	ug/L	
25) Chloroform	7.673	83		4238	0.338	ug/L	82
46) Tetrachloroethene	10.861	164		351025	59.468	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121523\
Data File : VW027656.D
Acq On : 15 Dec 2023 23:54
Operator : SY/MD
Sample : 05834-13
Misc : 5.87g/10mL/MSVOA_W/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGR26

Manual IntegrationsAPPROVED

Quant Time: Dec 16 01:42:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 16 00:05:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/17/2023
Supervised By :Semsettin Yesilyurt 12/17/2023

