


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121621\
 Data File : VW021403.D
 Acq On : 16 Dec 2021 08:18
 Operator : SY/VA
 Sample : BFB482
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB482

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Title : SFAM01.0
 Last Update : Fri Dec 24 01:43:02 2021

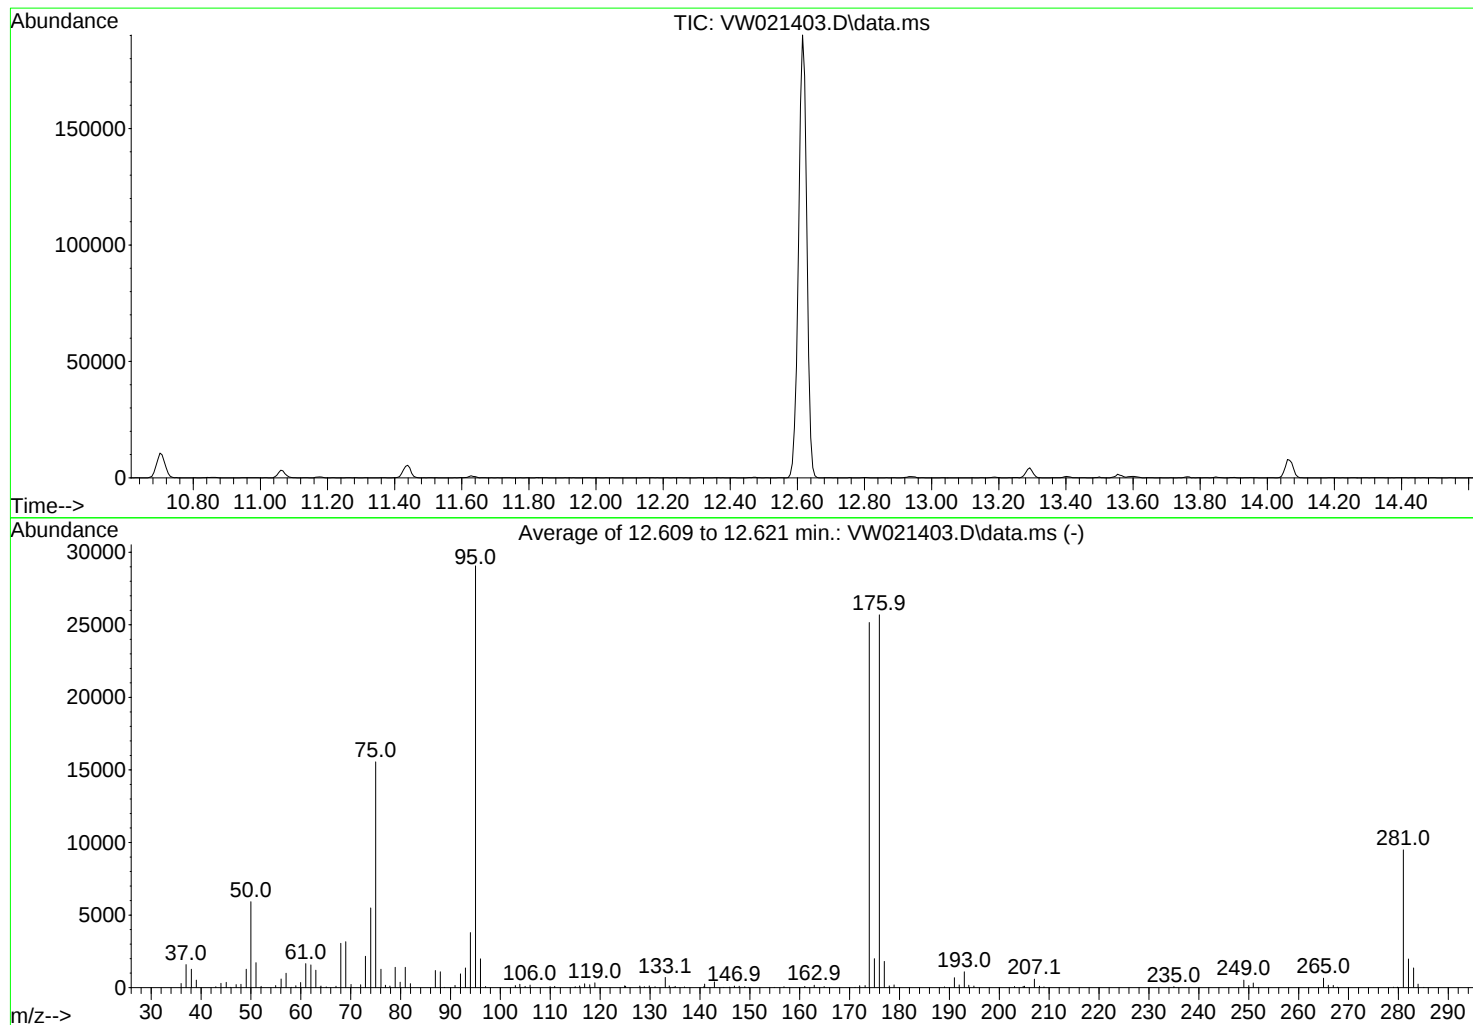

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	5919	PASS
75	95	30	80	53.5	15554	PASS
95	95	100	100	100.0	29064	PASS
96	95	5	9	6.8	1983	PASS
173	174	0.00	2	0.6	141	PASS
174	95	50	120	86.6	25157	PASS
175	174	5	9	7.9	1995	PASS
176	174	95	105	102.1	25693	PASS
177	176	5	10	7.1	1812	PASS

m/z	Abundance
40.10	54.0
72.90	52.0
281.00	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

m/z	Abundance
36.00	314.0
37.00	1421.0
38.00	1198.0
39.10	531.0
43.00	101.0
44.00	277.0
45.10	350.0
47.00	215.0
48.00	170.0
49.00	1164.0
50.00	5350.0
51.00	1527.0
52.00	99.0
55.00	120.0
56.00	571.0
57.00	849.0
59.00	189.0
59.90	319.0
61.00	1530.0
62.00	1299.0
63.00	944.0
63.90	128.0
65.10	63.0
67.20	89.0
68.00	2737.0
69.00	2741.0
70.10	188.0
72.00	194.0
73.00	2633.0
74.00	4479.0
75.00	13247.0
76.00	1264.0
77.00	163.0
77.90	163.0
78.90	1148.0
79.90	357.0
80.90	1204.0
81.90	253.0
87.00	953.0
88.00	854.0
88.80	76.0
90.90	143.0
92.00	796.0
93.00	1119.0
94.00	3162.0
95.00	25088.0
96.00	1905.0
97.00	75.0
103.00	240.0
103.90	199.0
104.90	107.0
106.00	137.0
109.90	106.0
110.90	90.0
114.90	97.0
115.90	92.0
116.90	267.0
118.00	222.0
118.90	365.0
124.90	309.0
128.00	118.0
128.80	55.0
129.80	108.0
131.00	80.0
133.10	1021.0
133.90	223.0
135.00	183.0
140.80	233.0
142.90	267.0
144.80	60.0
145.90	56.0
146.90	146.0
147.80	88.0
149.00	100.0
156.80	59.0
161.00	120.0
162.90	276.0
164.90	134.0
172.00	171.0
173.10	423.0
173.90	20560.0
174.90	1643.0
176.00	19688.0
176.90	1728.0
178.00	118.0
179.00	263.0
189.00	87.0
191.00	956.0
192.00	283.0
193.00	1611.0
193.90	234.0
194.90	197.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

203.00	150.0
204.80	262.0
207.00	855.0
208.10	167.0
209.00	110.0
235.00	147.0
249.00	826.0
249.90	208.0
250.90	460.0
251.90	55.0
265.00	869.0
266.00	219.0
267.00	212.0
267.90	54.0
281.00	13060.0
282.00	2425.0
283.00	2177.0
284.00	328.0
285.10	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

m/z	Abundance
36.00	273.0
37.00	1773.0
38.10	1467.0
39.00	568.0
42.80	56.0
44.00	315.0
45.00	485.0
47.10	273.0
48.00	288.0
49.10	1482.0
50.00	6556.0
51.00	1987.0
52.00	81.0
54.90	157.0
56.10	733.0
57.00	1122.0
58.10	53.0
59.00	113.0
60.00	427.0
61.00	1667.0
62.00	1708.0
63.00	1359.0
64.10	189.0
65.10	88.0
67.00	136.0
68.00	3410.0
69.00	3456.0
69.90	274.0
71.90	191.0
73.00	2151.0
74.00	6211.0
75.00	17736.0
76.00	1299.0
77.00	175.0
77.80	83.0
78.90	1629.0
79.90	359.0
80.90	1501.0
81.90	275.0
86.90	1194.0
88.00	1263.0
90.90	161.0
92.00	998.0
93.00	1493.0
94.00	4075.0
95.00	31312.0
96.00	2113.0
97.00	87.0
103.00	131.0
103.90	260.0
104.90	100.0
105.90	239.0
110.00	76.0
110.90	96.0
115.10	111.0
115.90	164.0
116.90	254.0
117.90	193.0
118.90	359.0
125.10	287.0
127.90	100.0
128.90	75.0
129.90	116.0
131.00	69.0
133.00	753.0
133.80	157.0
134.60	75.0
135.10	78.0
136.90	69.0
141.00	303.0
142.90	477.0
145.90	59.0
146.90	110.0
147.90	104.0
149.00	87.0
149.80	56.0
156.90	72.0
161.00	163.0
162.90	148.0
164.90	101.0
172.00	229.0
173.90	29344.0
174.90	2103.0
175.90	25984.0
177.00	1889.0
177.90	126.0
178.80	170.0
189.00	84.0
191.00	742.0
191.90	213.0
193.00	1198.0
194.00	165.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

194.90	123.0
203.10	75.0
205.00	176.0
207.10	570.0
208.10	81.0
208.90	63.0
235.00	81.0
249.00	401.0
250.00	128.0
250.90	338.0
265.00	770.0
265.90	207.0
266.90	177.0
267.80	61.0
279.00	90.0
281.00	10409.0
282.00	2239.0
283.10	1426.0
283.90	276.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

m/z	Abundance
36.00	278.0
37.00	1558.0
38.00	1133.0
39.10	450.0
42.90	60.0
44.00	310.0
45.00	268.0
45.90	55.0
47.00	158.0
48.00	241.0
49.00	1154.0
50.00	5851.0
51.00	1652.0
52.10	81.0
55.00	148.0
56.10	496.0
57.10	992.0
59.00	99.0
60.00	315.0
61.00	1770.0
62.00	1690.0
63.00	1298.0
64.00	145.0
66.90	89.0
68.00	3024.0
69.00	3313.0
70.10	214.0
72.10	220.0
73.00	1855.0
74.00	5795.0
75.00	15679.0
76.10	1225.0
76.90	163.0
77.90	85.0
78.90	1429.0
79.90	422.0
81.00	1513.0
82.00	286.0
86.90	1379.0
87.90	1163.0
90.90	168.0
92.00	1056.0
93.00	1456.0
94.00	4143.0
95.00	30792.0
96.00	1930.0
97.10	63.0
103.00	64.0
103.90	235.0
105.00	70.0
105.90	168.0
110.90	73.0
115.00	53.0
115.90	117.0
116.90	263.0
117.80	196.0
119.00	279.0
124.90	69.0
127.90	125.0
128.90	66.0
129.90	133.0
131.00	68.0
133.10	333.0
134.80	93.0
136.90	103.0
140.90	439.0
142.90	431.0
146.90	62.0
147.90	111.0
154.90	72.0
156.90	81.0
162.80	79.0
171.10	65.0
174.00	25568.0
175.00	2238.0
175.90	31408.0
176.90	1819.0
178.00	106.0
179.00	138.0
191.00	341.0
192.10	81.0
193.00	470.0
193.80	86.0
205.10	112.0
207.00	334.0
207.90	62.0
249.10	326.0
250.10	106.0
250.90	158.0
265.00	327.0
265.90	79.0
266.90	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

279.80	83.0
281.00	5226.0
282.00	1263.0
283.10	478.0
283.80	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482