

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121624\
 Data File : VW031268.D
 Acq On : 16 Dec 2024 13:47
 Operator : SY/MD
 Sample : P5226-15
 Misc : 4.92g/10mL/MSVOA_W/SOILB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 17 00:36:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Dec 17 00:33:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	851777	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	617670	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	198049	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	246887	19.264	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.040%
7) Chloroethane-d5	2.893	69	179161	18.898	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.600%
11) 1,1-Dichloroethene-d2	4.015	65	113543	18.677	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.720%
21) 2-Butanone-d5	7.087	46	101448	42.032	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.060%
24) Chloroform-d	7.648	84	424986	18.210	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	72.840%
26) 1,2-Dichloroethane-d4	8.301	65	235064	20.056	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.240%
32) Benzene-d6	8.270	84	859399	21.708	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.840%
36) 1,2-Dichloropropane-d6	9.270	67	253697	21.988	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.960%
41) Toluene-d8	10.319	98	715864	19.437	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.760%
43) trans-1,3-Dichloroprop...	10.575	79	110109	20.697	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.800%
47) 2-Hexanone-d5	10.922	63	80367	51.794	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.580%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	164365	22.689	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	137876	18.753	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.000%
Target Compounds					Qvalue	
25) Chloroform	7.673	83	14151	0.682	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121624\
Data File : VW031268.D
Acq On : 16 Dec 2024 13:47
Operator : SY/MD
Sample : P5226-15
Misc : 4.92g/10mL/MSVOA_W/SOILB
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 17 00:36:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Dec 17 00:33:32 2024
Response via : Initial Calibration

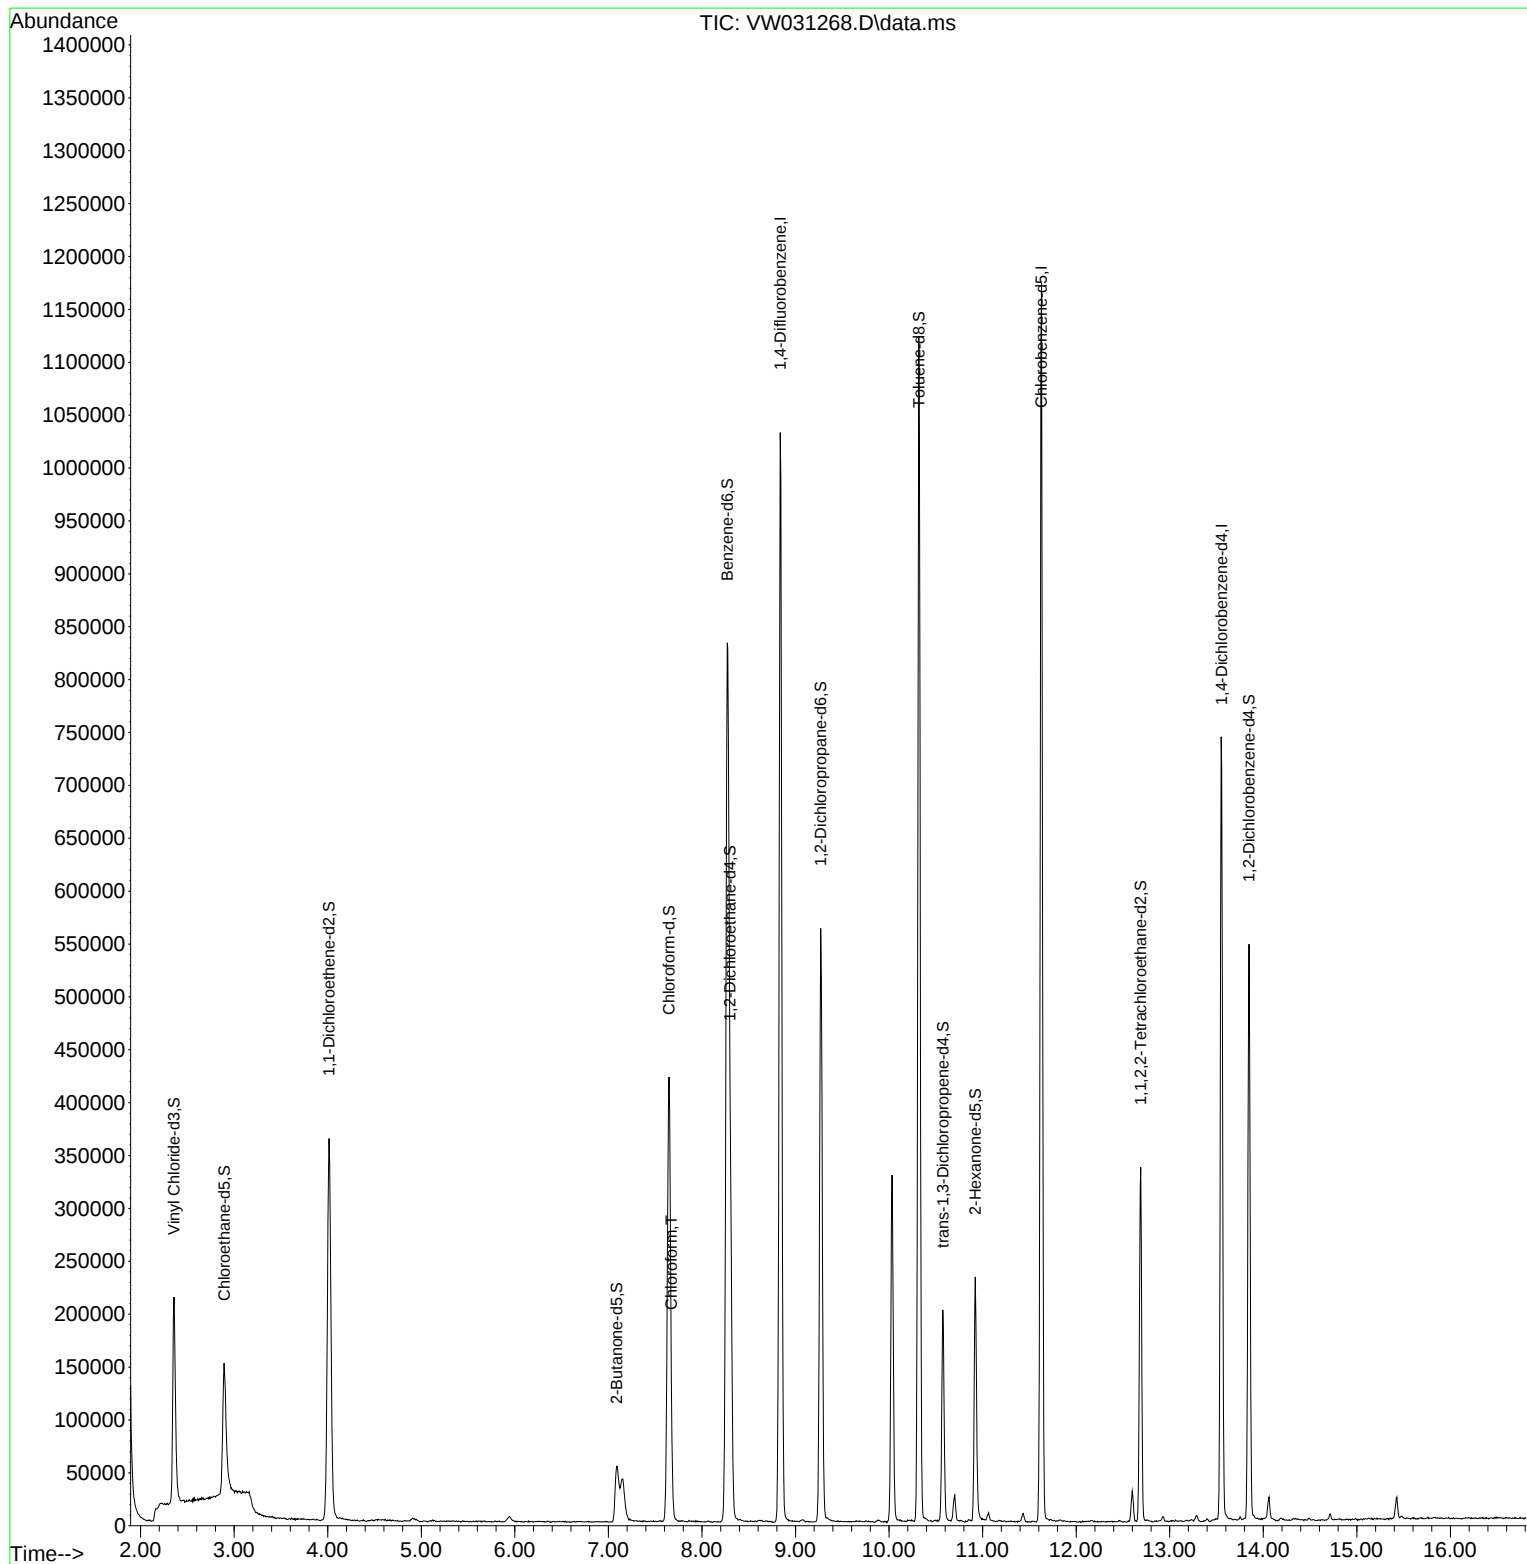

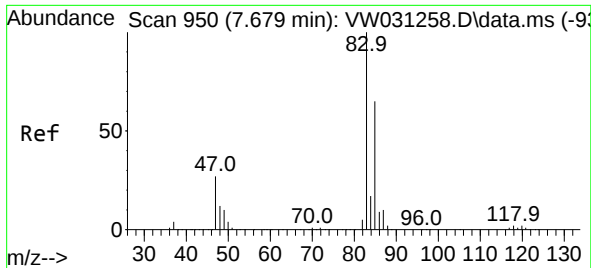

#25
 Chloroform
 Concen: 0.682 ug/L
 RT: 7.673 min Scan# 94
 Delta R.T. -0.006 min
 Lab File: VW031268.D
 Acq: 16 Dec 2024 13:47

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 83 Resp: 14151
 Ion Ratio Lower Upper
 83 100
 85 66.7 46.1 85.5

