

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121624\
 Data File : VW031273.D
 Acq On : 16 Dec 2024 15:47
 Operator : SY/MD
 Sample : P5232-19
 Misc : 3.57g/10mL/MSVOA_W/SOILB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 17 00:37:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Dec 17 00:33:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	1070374	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	610020	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	132010	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	322158	20.004	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.000%
7) Chloroethane-d5	2.893	69	253301	21.262	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.040%
11) 1,1-Dichloroethene-d2	4.015	65	142287	18.625	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.520%
21) 2-Butanone-d5	7.100	46	60748	20.029	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	40.060%
24) Chloroform-d	7.648	84	585861	19.977	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.920%
26) 1,2-Dichloroethane-d4	8.532	65	99	0.007	ug/L	0.23
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.270	84	1074005	27.469	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.880%
36) 1,2-Dichloropropane-d6	9.270	67	337846	29.648	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	118.600%
41) Toluene-d8	10.319	98	796582	21.900	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.600%
43) trans-1,3-Dichloroprop...	10.575	79	86828	16.525	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.120%
47) 2-Hexanone-d5	10.922	63	39820	25.985	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	51.960%
56) 1,1,2,2-Tetrachloroeth...	12.684	84	155290	21.705	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.800%
66) 1,2-Dichlorobenzene-d4	13.848	152	84458	17.234	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	68.920%#
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	6568	0.413	ug/L	Qvalue # 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121624\
Data File : VW031273.D
Acq On : 16 Dec 2024 15:47
Operator : SY/MD
Sample : P5232-19
Misc : 3.57g/10mL/MSVOA_W/SOILB
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 17 00:37:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Dec 17 00:33:32 2024
Response via : Initial Calibration

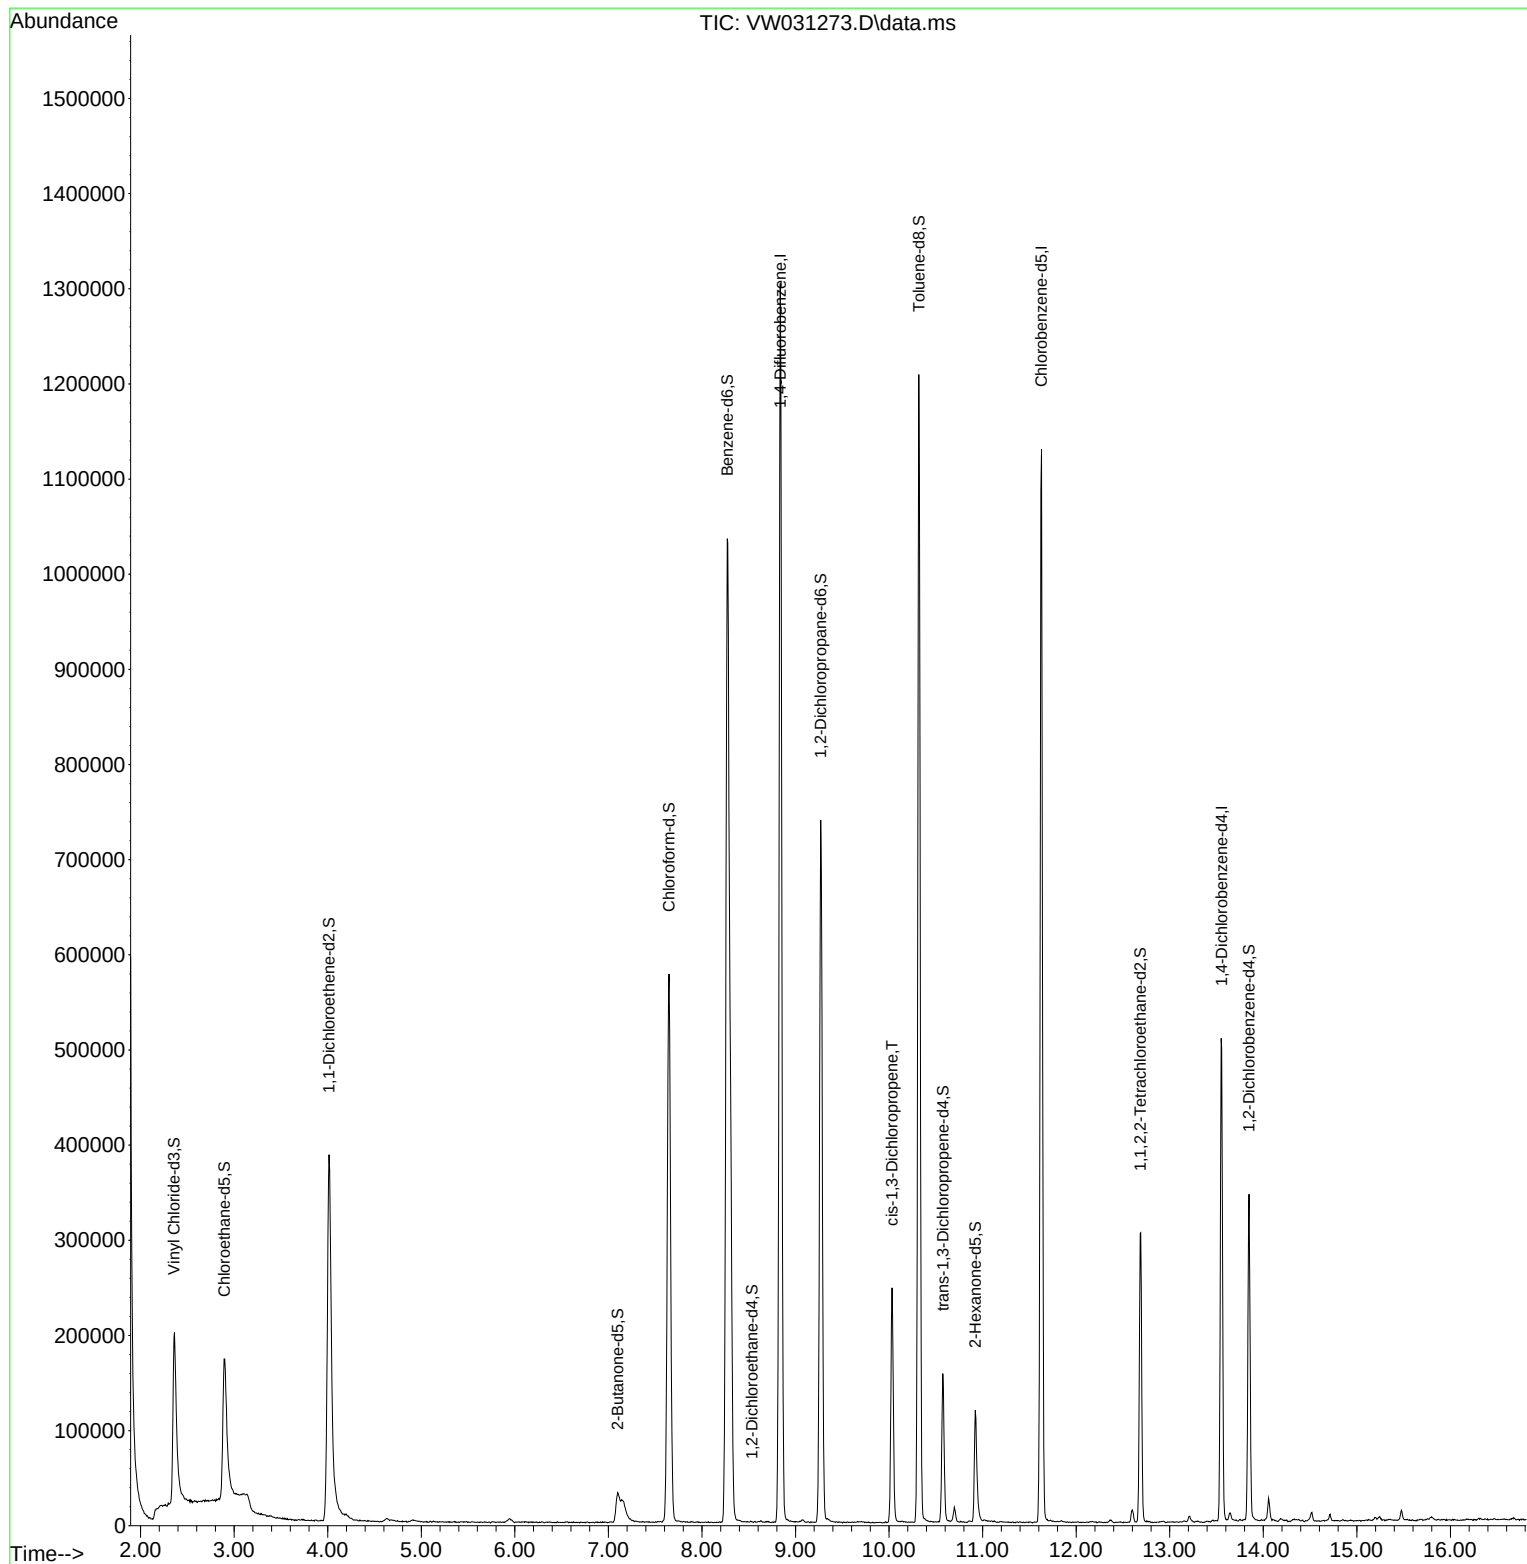

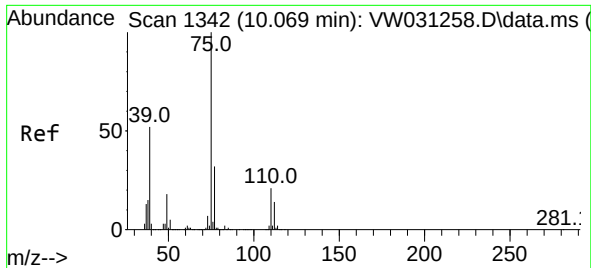

#39
 cis-1,3-Dichloropropene
 Concen: 0.413 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW031273.D
 Acq: 16 Dec 2024 15:47

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 6568
 Ion Ratio Lower Upper
 75 100
 77 45.7 21.8 40.4#

