

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027771.D
 Acq On : 19 Dec 2023 12:03
 Operator : SY/MD
 Sample : 05794-09RE
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 19 22:34:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	537893	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	412179	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	128491	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	154465	20.277	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.120%
7) Chloroethane-d5	2.905	69	126369	21.306	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.240%
11) 1,1-Dichloroethene-d2	4.021	65	61896	20.288	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.160%
21) 2-Butanone-d5	7.087	46	50221	38.715	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.440%
24) Chloroform-d	7.648	84	287551	22.466	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.880%
26) 1,2-Dichloroethane-d4	8.307	65	132648	22.072	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.280%
32) Benzene-d6	8.276	84	611133	25.370	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.480%
36) 1,2-Dichloropropane-d6	9.276	67	175389	25.699	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.800%
41) Toluene-d8	10.325	98	525170	23.498	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.000%
43) trans-1,3-Dichloroprop...	10.575	79	55913	21.161	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.640%
47) 2-Hexanone-d5	10.922	63	44938	45.185	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.360%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	112834	21.863	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	108142	23.512	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.040%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	4026	0.458	ug/L	# 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
Data File : VW027771.D
Acq On : 19 Dec 2023 12:03
Operator : SY/MD
Sample : 05794-09RE
Misc : 5.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 19 22:34:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

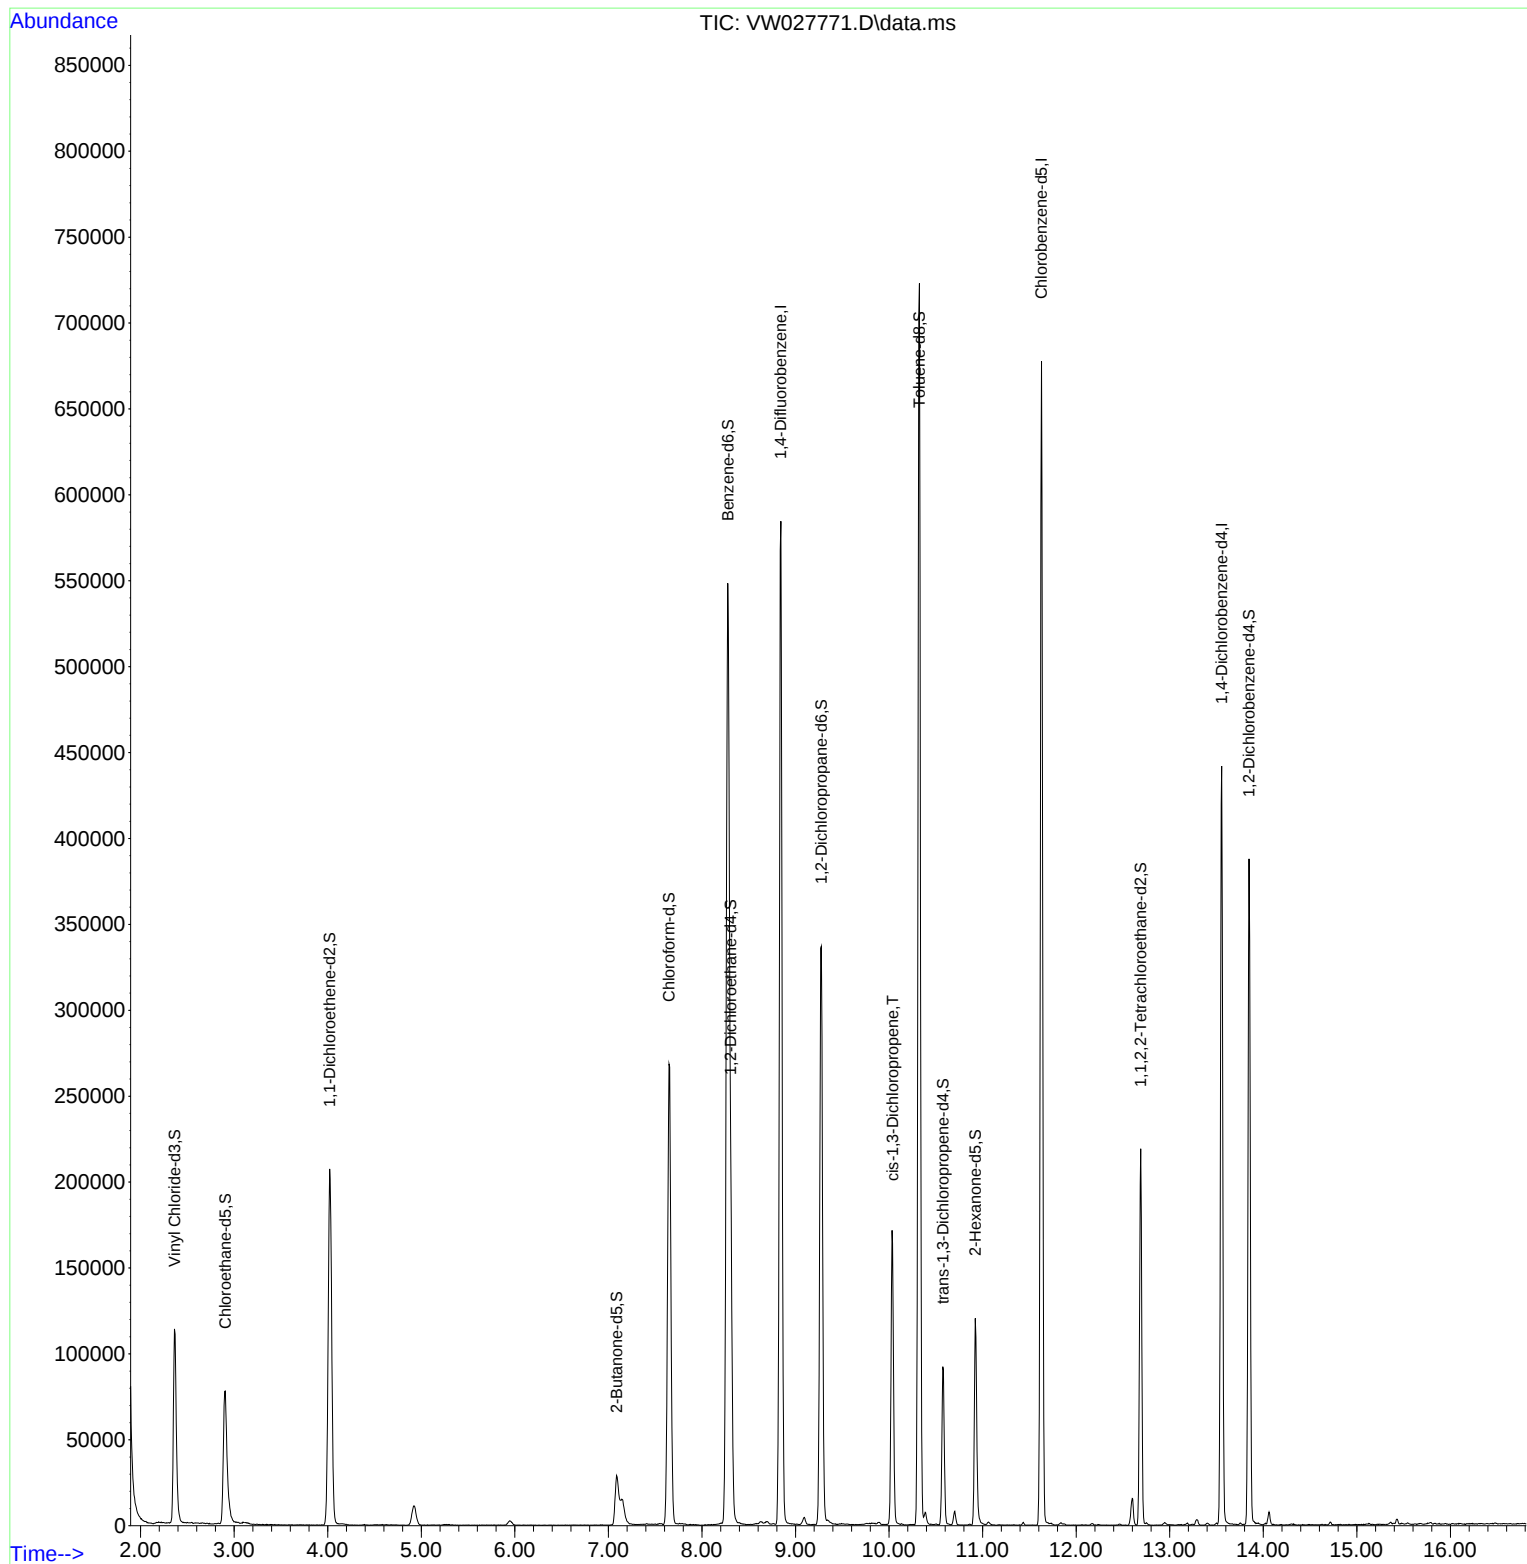

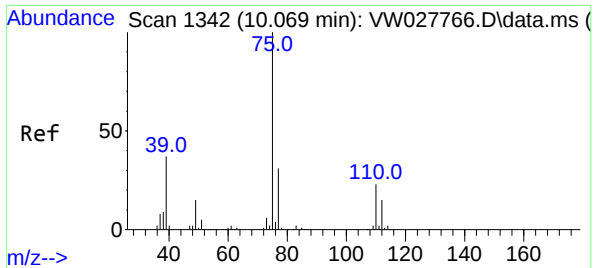

#39
cis-1,3-Dichloropropene
Concen: 0.458 ug/L
RT: 10.038 min Scan# 11
Delta R.T. -0.031 min
Lab File: VW027771.D
Acq: 19 Dec 2023 12:03

Instrument :
MSVOA_W
ClientSampleId :

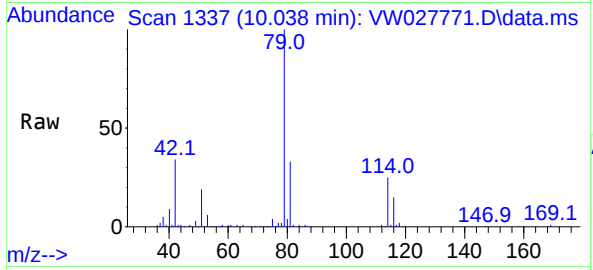

Tgt Ion: 75 Resp: 4026
Ion Ratio Lower Upper
75 100
77 42.9 21.8 40.6#

