




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027786.D
 Acq On : 19 Dec 2023 17:57
 Operator : SY/MD
 Sample : 05808-19RE
 Misc : 3.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B15

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:37:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

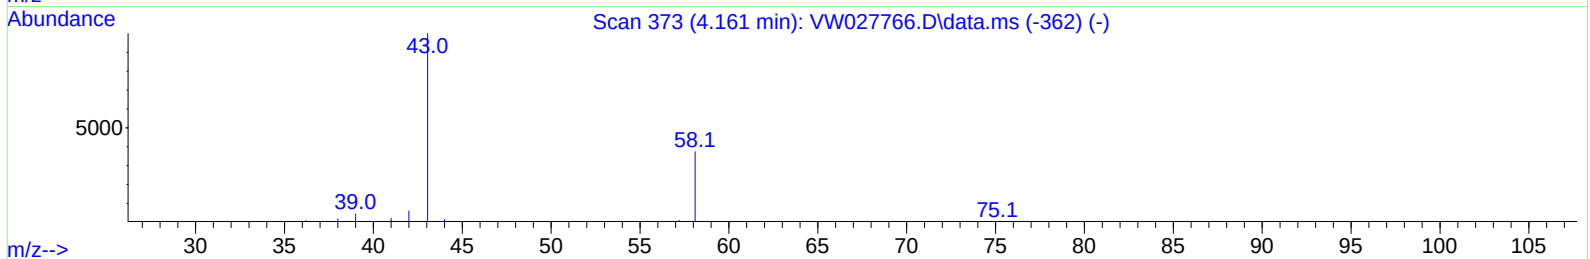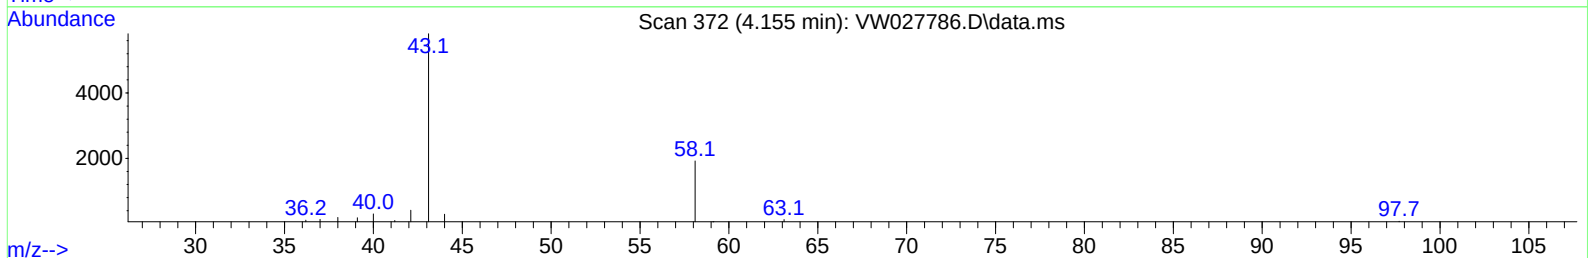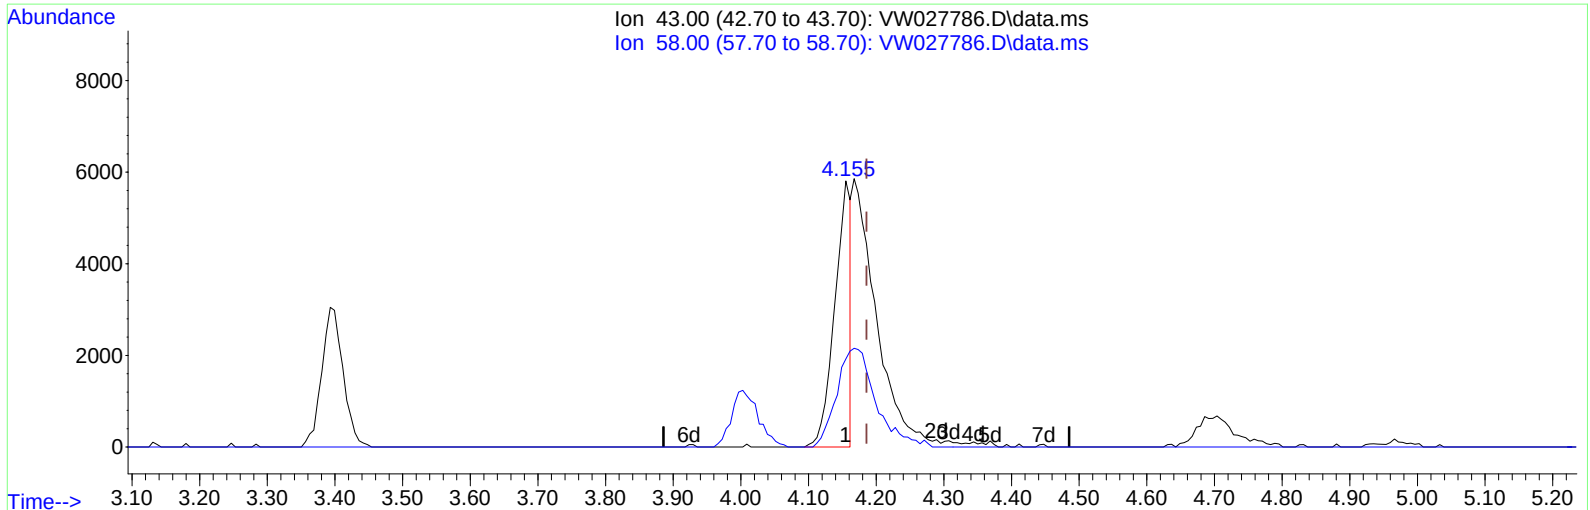

TIC: VW027786.D\data.ms

(13) Acetone (T)

4.155min (-0.031) 6.59 ug/L

response 9578

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.30	89.16#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027786.D
 Acq On : 19 Dec 2023 17:57
 Operator : SY/MD
 Sample : 05808-19RE
 Misc : 3.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B15

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:37:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

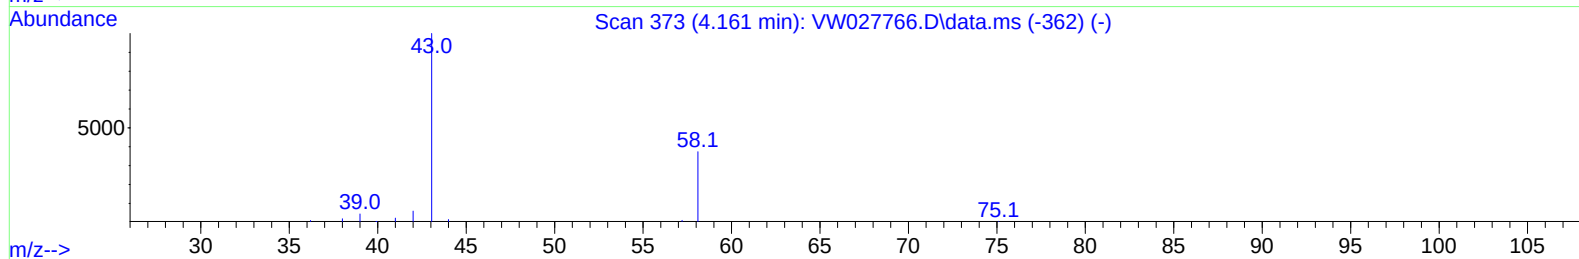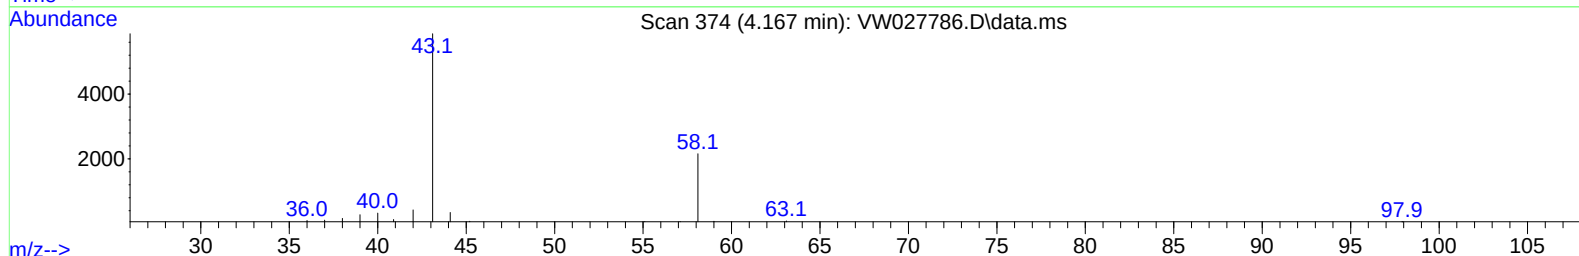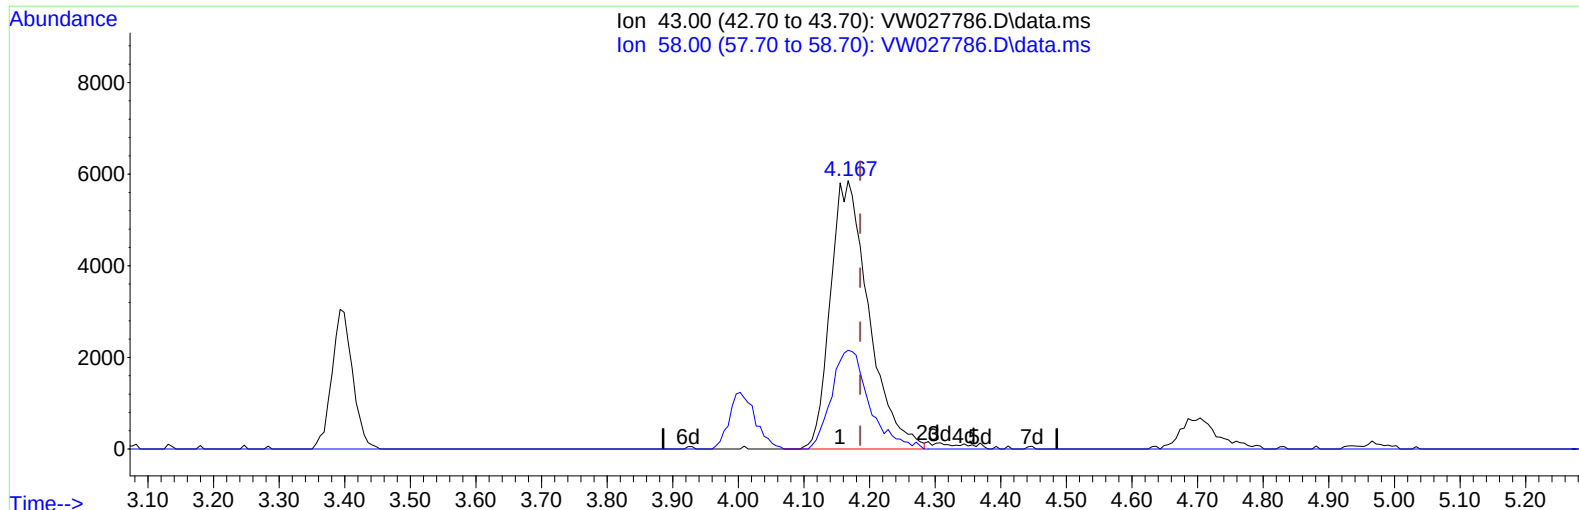

TIC: VW027786.D\data.ms

(13) Acetone (T)

4.167min (-0.018) 16.39 ug/L m

response 23823

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.30	35.85
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027786.D
 Acq On : 19 Dec 2023 17:57
 Operator : SY/MD
 Sample : 05808-19RE
 Misc : 3.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B15

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

Quant Time: Dec 19 22:37:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

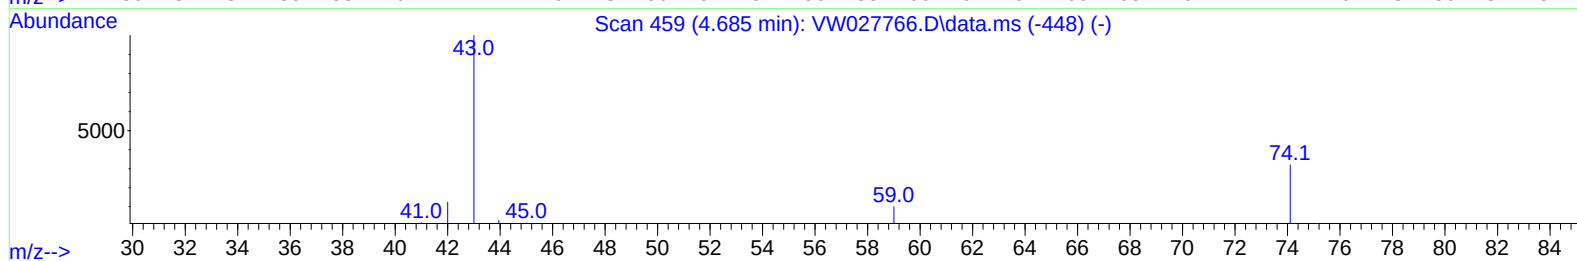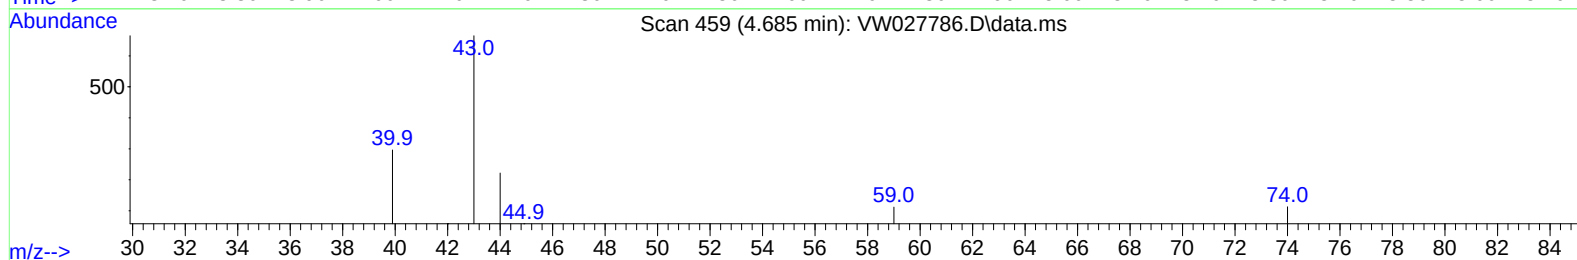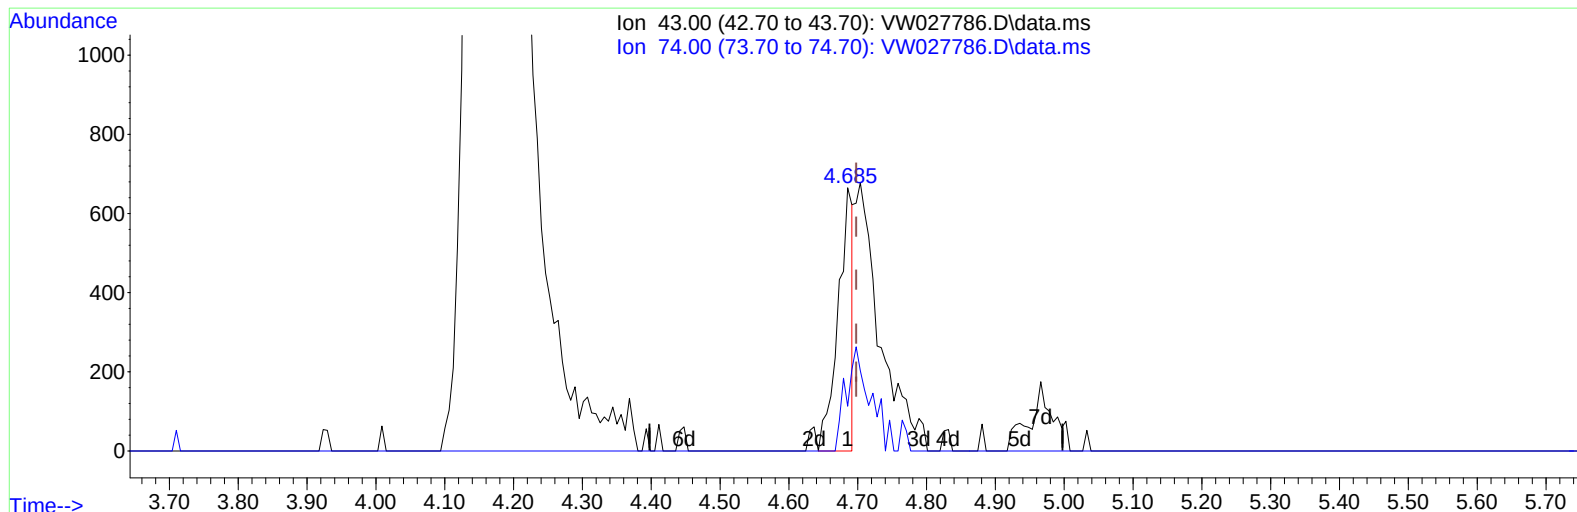

TIC: VW027786.D\data.ms

(15) Methyl Acetate (T)

4.685min (-0.012) 0.38 ug/L

response 994

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.60	13.78#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027786.D
 Acq On : 19 Dec 2023 17:57
 Operator : SY/MD
 Sample : 05808-19RE
 Misc : 3.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B15

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

Quant Time: Dec 19 22:37:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

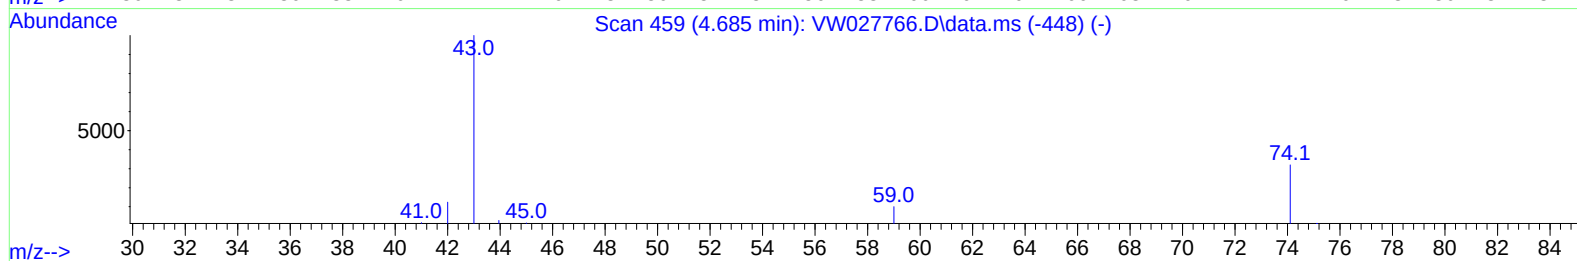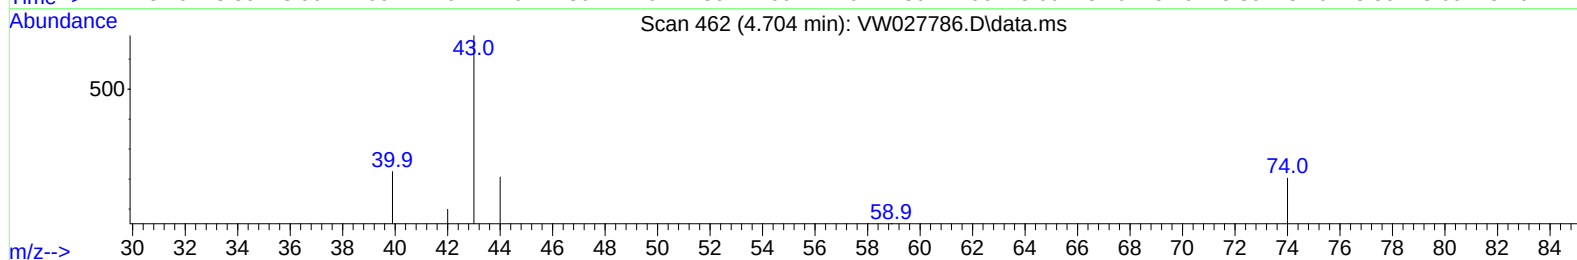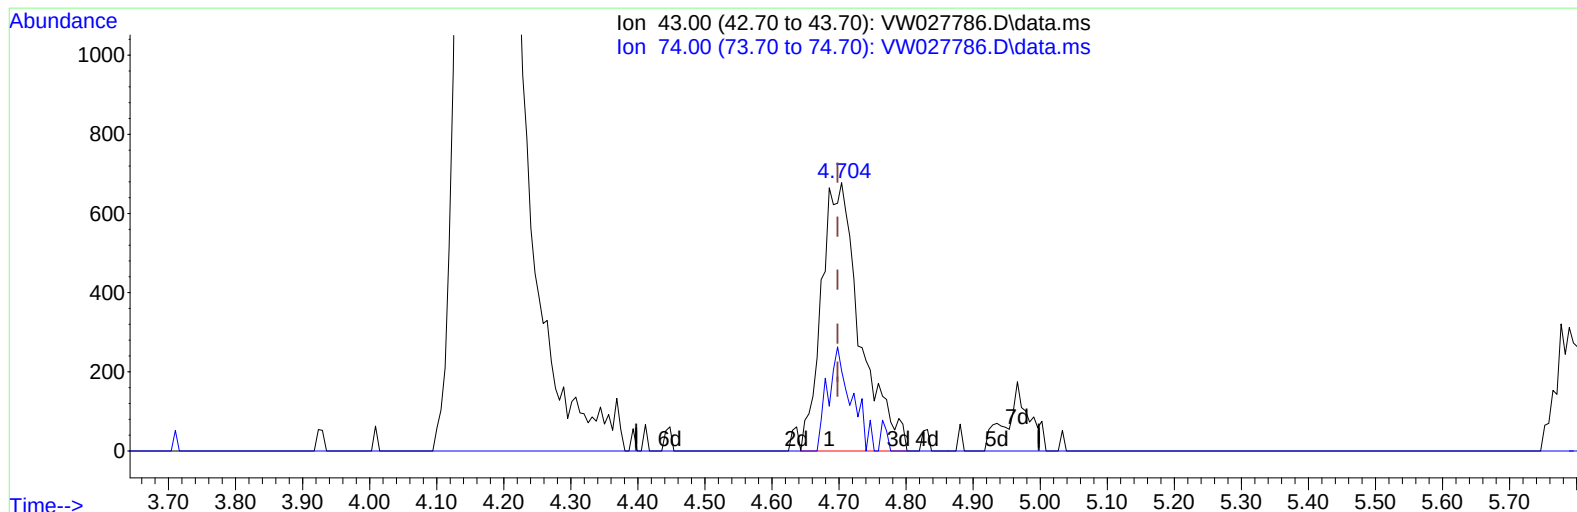

TIC: VW027786.D\data.ms

(15) Methyl Acetate (T)

4.704min (+ 0.006) 1.03 ug/L m

response 2709

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.60	5.06#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027786.D
 Acq On : 19 Dec 2023 17:57
 Operator : SY/MD
 Sample : 05808-19RE
 Misc : 3.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B15

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:37:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

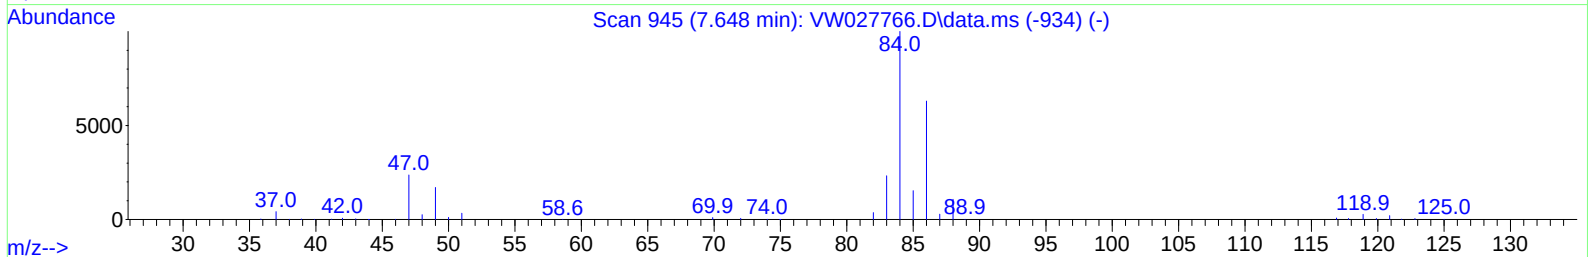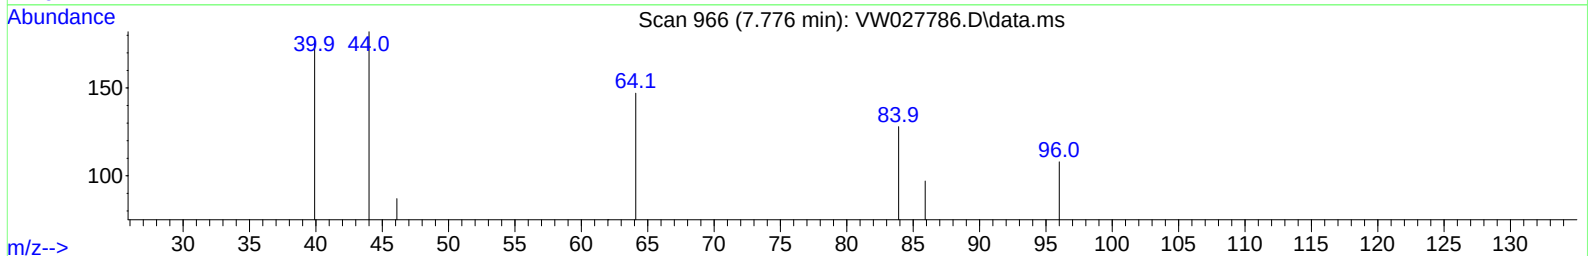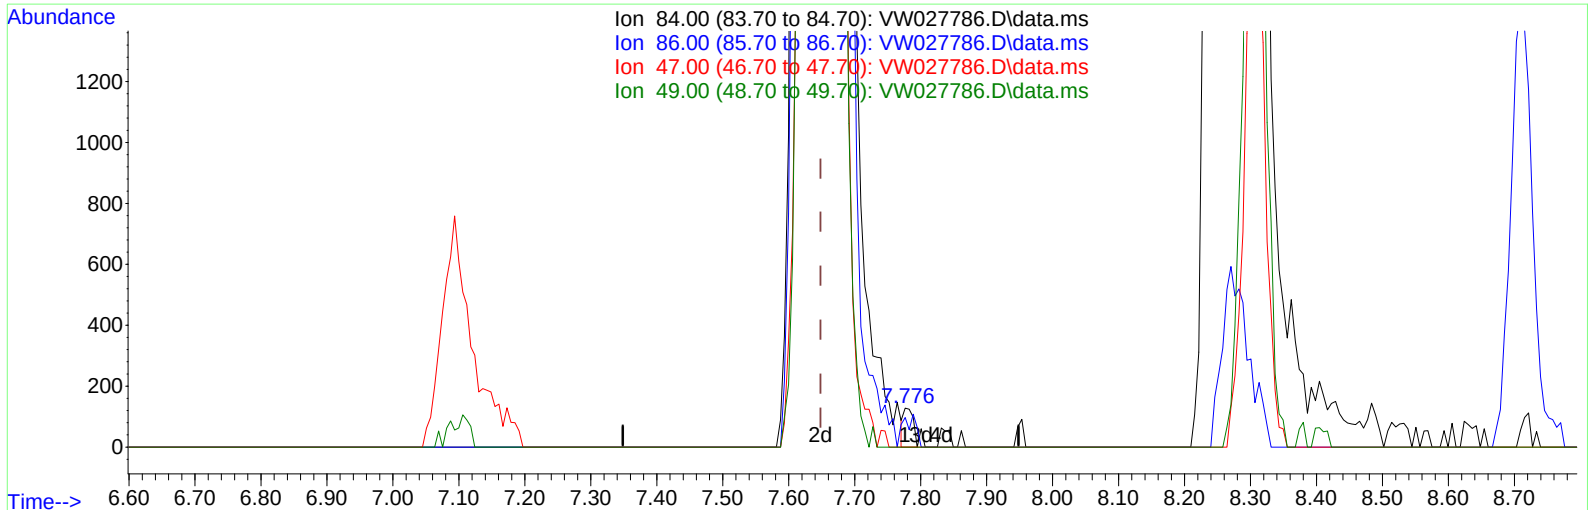

TIC: VW027786.D\data.ms

(24) Chloroform-d (S)

7.776min (+ 0.128) 0.01 ug/L

response 128

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.50	64.84
47.00	37.10	31.25
49.00	21.70	18.75




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027786.D
 Acq On : 19 Dec 2023 17:57
 Operator : SY/MD
 Sample : 05808-19RE
 Misc : 3.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B15

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:37:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

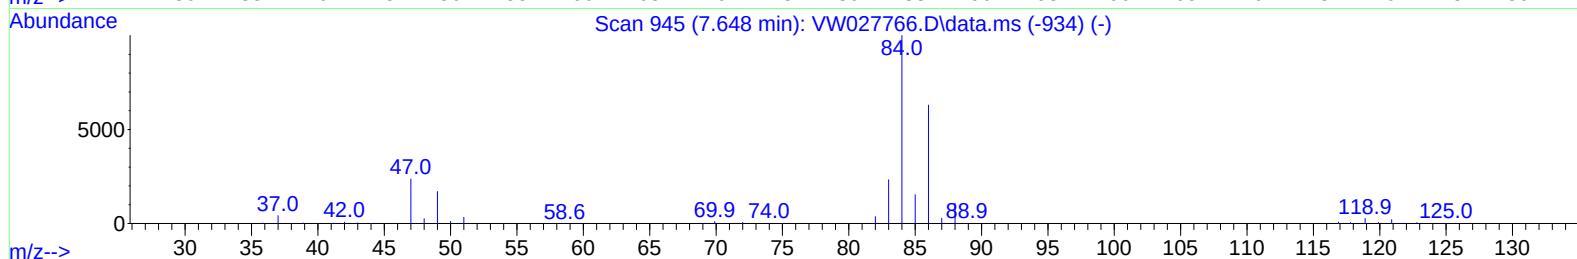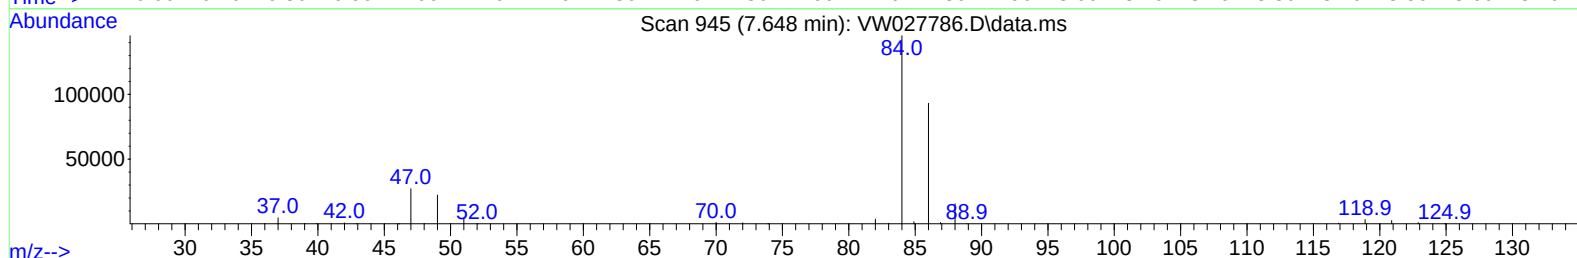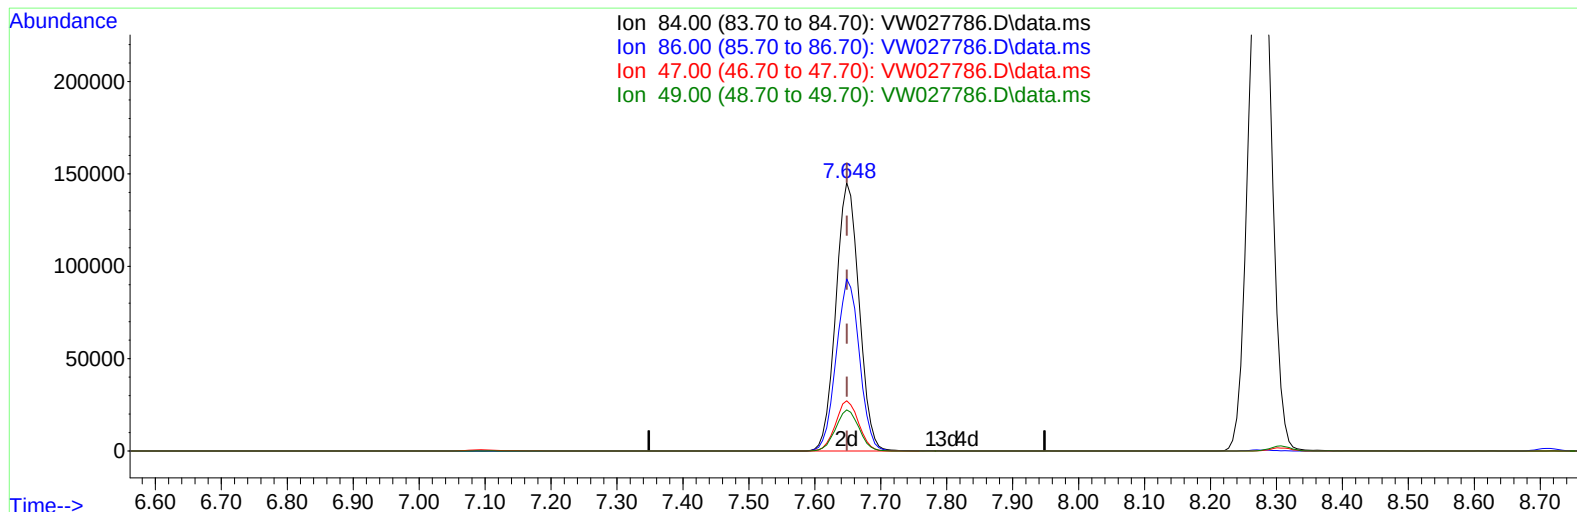

TIC: VW027786.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 22.52 ug/L m

response 355708

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.50	0.02#
47.00	37.10	0.01#
49.00	21.70	0.01#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027786.D
 Acq On : 19 Dec 2023 17:57
 Operator : SY/MD
 Sample : 05808-19RE
 Misc : 3.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B15

Manual IntegrationsAPPROVED

Quant Time: Dec 19 22:37:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	663801	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	469246	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	119968	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	189783	20.188	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.760%		
7) Chloroethane-d5	2.899	69	136651	18.669	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.680%		
11) 1,1-Dichloroethene-d2	4.021	65	78353	20.811	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	83.240%		
21) 2-Butanone-d5	7.094	46	76436	47.748	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.500%		
24) Chloroform-d	7.648	84	355708m	22.520	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.080%		
26) 1,2-Dichloroethane-d4	8.307	65	169211	22.816	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.280%		
32) Benzene-d6	8.276	84	753224	27.466	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	109.880%		
36) 1,2-Dichloropropane-d6	9.270	67	214420	27.598	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	110.400%		
41) Toluene-d8	10.319	98	626098	24.607	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	98.440%		
43) trans-1,3-Dichloroprop...	10.575	79	74543	24.780	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	99.120%		
47) 2-Hexanone-d5	10.922	63	74949	66.196	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	132.400%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	136584	23.246	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.000%		
66) 1,2-Dichlorobenzene-d4	13.848	152	96096	22.377	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.520%		
Target Compounds						Qvalue
13) Acetone	4.167	43	23823m	16.394	ug/L	
15) Methyl Acetate	4.704	43	2709m	1.032	ug/L	
53) m,p-Xylene	11.831	106	17623	1.391	ug/L	99
54) o-Xylene	12.160	106	7727	0.655	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
Data File : VW027786.D
Acq On : 19 Dec 2023 17:57
Operator : SY/MD
Sample : 05808-19RE
Misc : 3.56g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B15

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2023
Supervised By :Mahesh Dadoda 12/20/2023

Quant Time: Dec 19 22:37:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

