

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027780.D
 Acq On : 19 Dec 2023 15:35
 Operator : SY/MD
 Sample : 05835-04
 Misc : 2.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B34

Quant Time: Dec 19 22:36:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	671653	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	625475	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	301429	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	184099	19.354	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.400%
7) Chloroethane-d5	2.899	69	136067	18.372	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.480%
11) 1,1-Dichloroethene-d2	4.021	65	76692	20.131	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.520%
21) 2-Butanone-d5	7.094	46	67189	41.481	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.960%
24) Chloroform-d	7.648	84	353800	22.137	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.560%
26) 1,2-Dichloroethane-d4	8.307	65	167813	22.363	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.440%
32) Benzene-d6	8.276	84	761620	20.835	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.320%
36) 1,2-Dichloropropane-d6	9.276	67	212663	20.535	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.120%
41) Toluene-d8	10.325	98	705940	20.815	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.240%
43) trans-1,3-Dichloroprop...	10.575	79	84256	21.013	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.040%
47) 2-Hexanone-d5	10.922	63	70945	47.008	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.020%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	168910	21.567	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.280%
66) 1,2-Dichlorobenzene-d4	13.849	152	244470	22.657	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.640%
Target Compounds						
13) Acetone	4.173	43	19230	13.078	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
Data File : VW027780.D
Acq On : 19 Dec 2023 15:35
Operator : SY/MD
Sample : 05835-04
Misc : 2.14g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B34

Quant Time: Dec 19 22:36:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

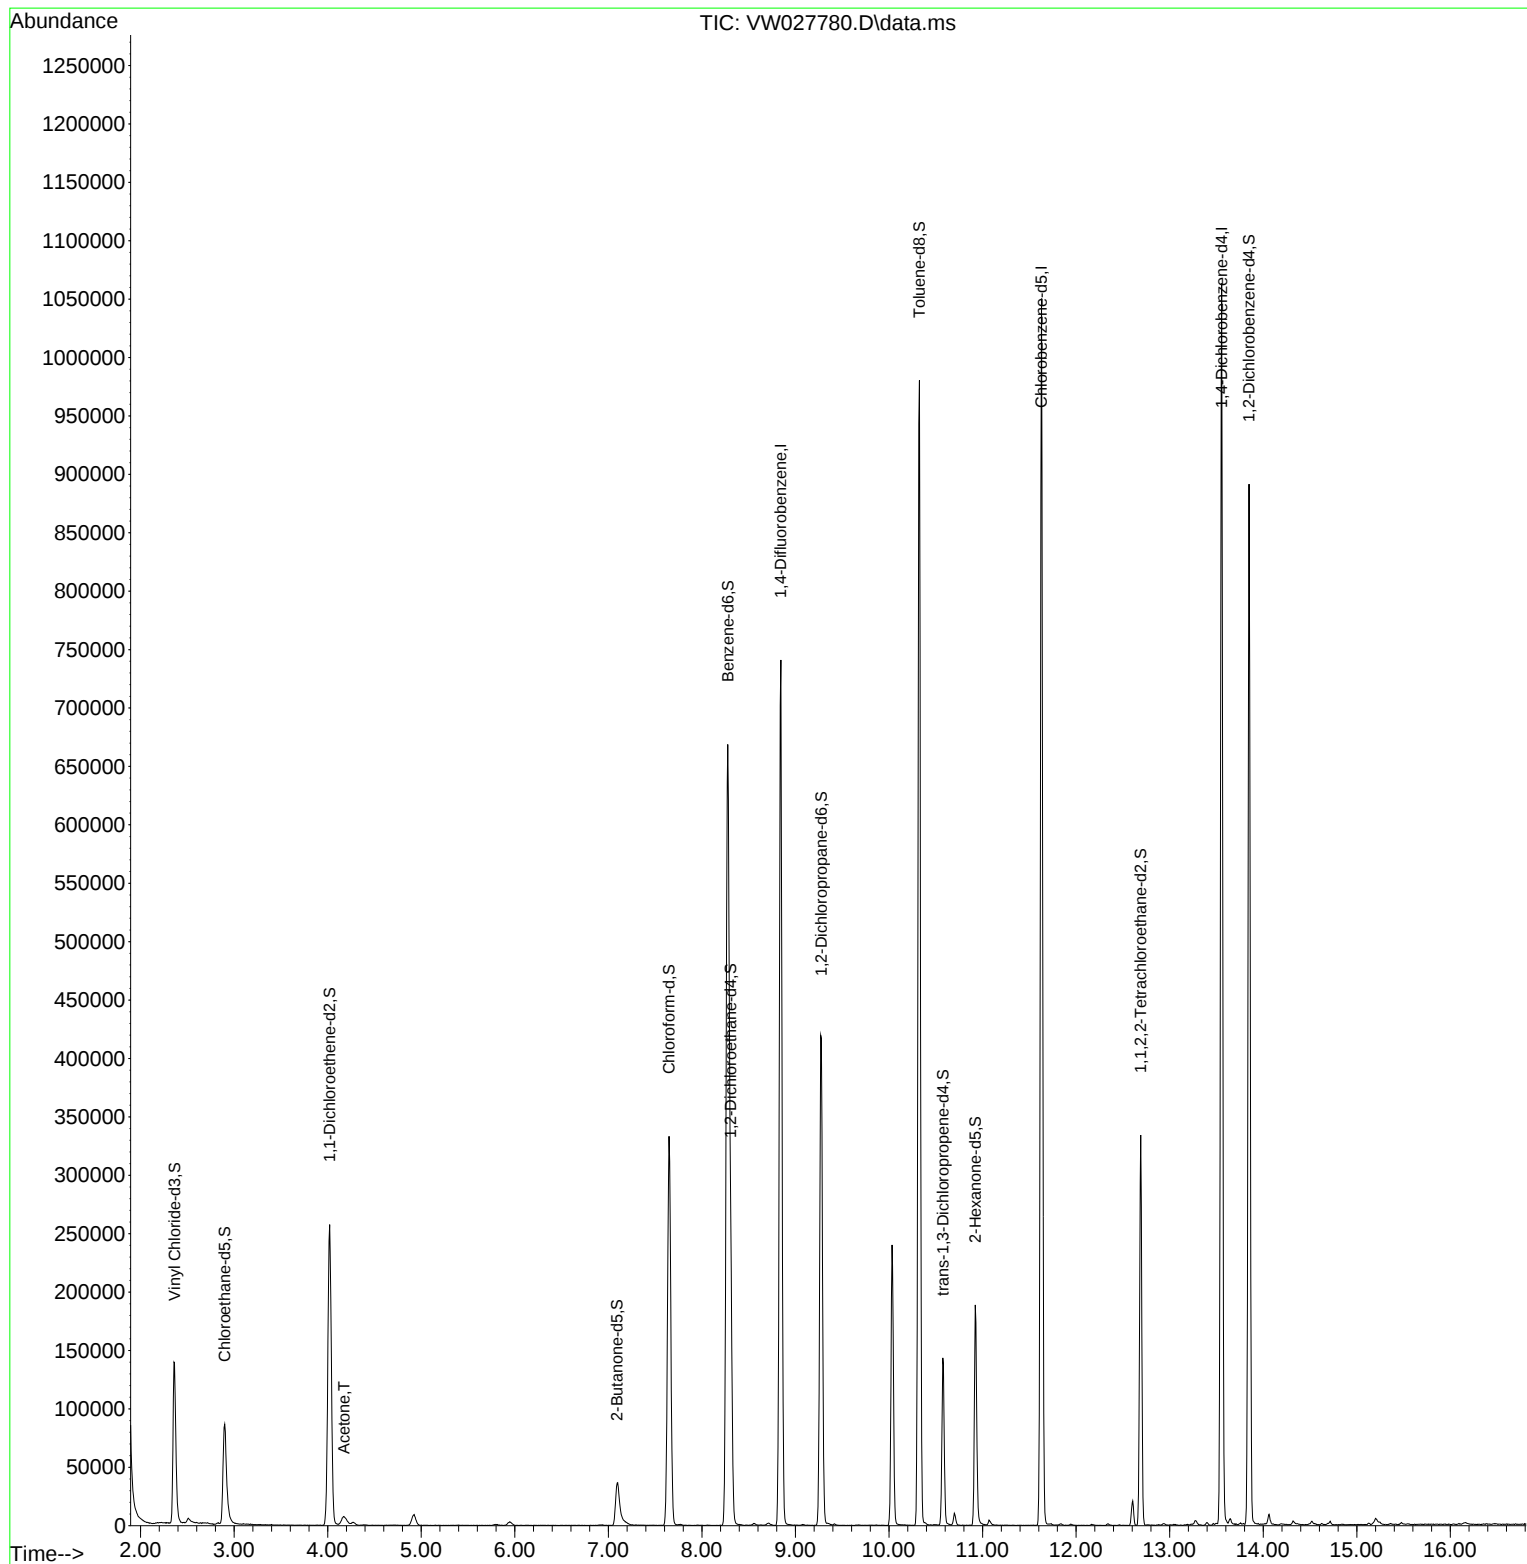

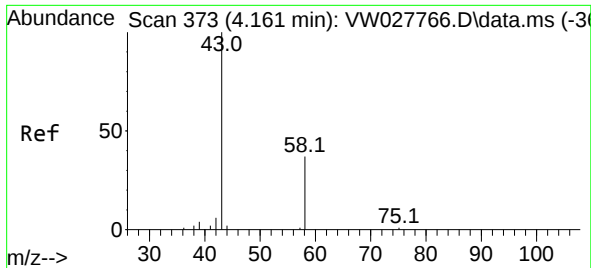

#13
 Acetone
 Concen: 13.078 ug/L
 RT: 4.173 min Scan# 31
 Delta R.T. -0.012 min
 Lab File: VW027780.D
 Acq: 19 Dec 2023 15:35

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B34

Tgt Ion: 43 Resp: 19230
 Ion Ratio Lower Upper
 43 100
 58 24.5 0.0 68.6

