

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
 Data File : VW027784.D
 Acq On : 19 Dec 2023 17:10
 Operator : SY/MD
 Sample : 05808-07
 Misc : 6.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AZ9

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

Quant Time: Dec 19 22:36:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	609916	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	545705	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	250963	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	162756	18.842	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.360%		
7) Chloroethane-d5	2.899	69	116972	17.393	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.560%		
11) 1,1-Dichloroethene-d2	4.021	65	66906	19.340	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	77.360%		
21) 2-Butanone-d5	7.088	46	80567	54.775	ug/L	-0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	109.540%		
24) Chloroform-d	7.648	84	312507	21.533	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	86.120%		
26) 1,2-Dichloroethane-d4	8.307	65	156425	22.955	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.840%		
32) Benzene-d6	8.276	84	665516	20.867	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.480%		
36) 1,2-Dichloropropane-d6	9.270	67	192743	21.332	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	85.320%		
41) Toluene-d8	10.319	98	617218	20.859	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	83.440%		
43) trans-1,3-Dichloroprop...	10.575	79	76255	21.798	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	87.200%		
47) 2-Hexanone-d5	10.922	63	82170	62.405	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	124.800%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	176802	25.875	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.480%		
66) 1,2-Dichlorobenzene-d4	13.849	152	200235	22.289	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.160%		
Target Compounds						Qvalue
15) Methyl Acetate	4.679	43	2997m	1.242	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121923\
Data File : VW027784.D
Acq On : 19 Dec 2023 17:10
Operator : SY/MD
Sample : 05808-07
Misc : 6.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AZ9

Quant Time: Dec 19 22:36:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2023
Supervised By :Mahesh Dadoda 12/20/2023

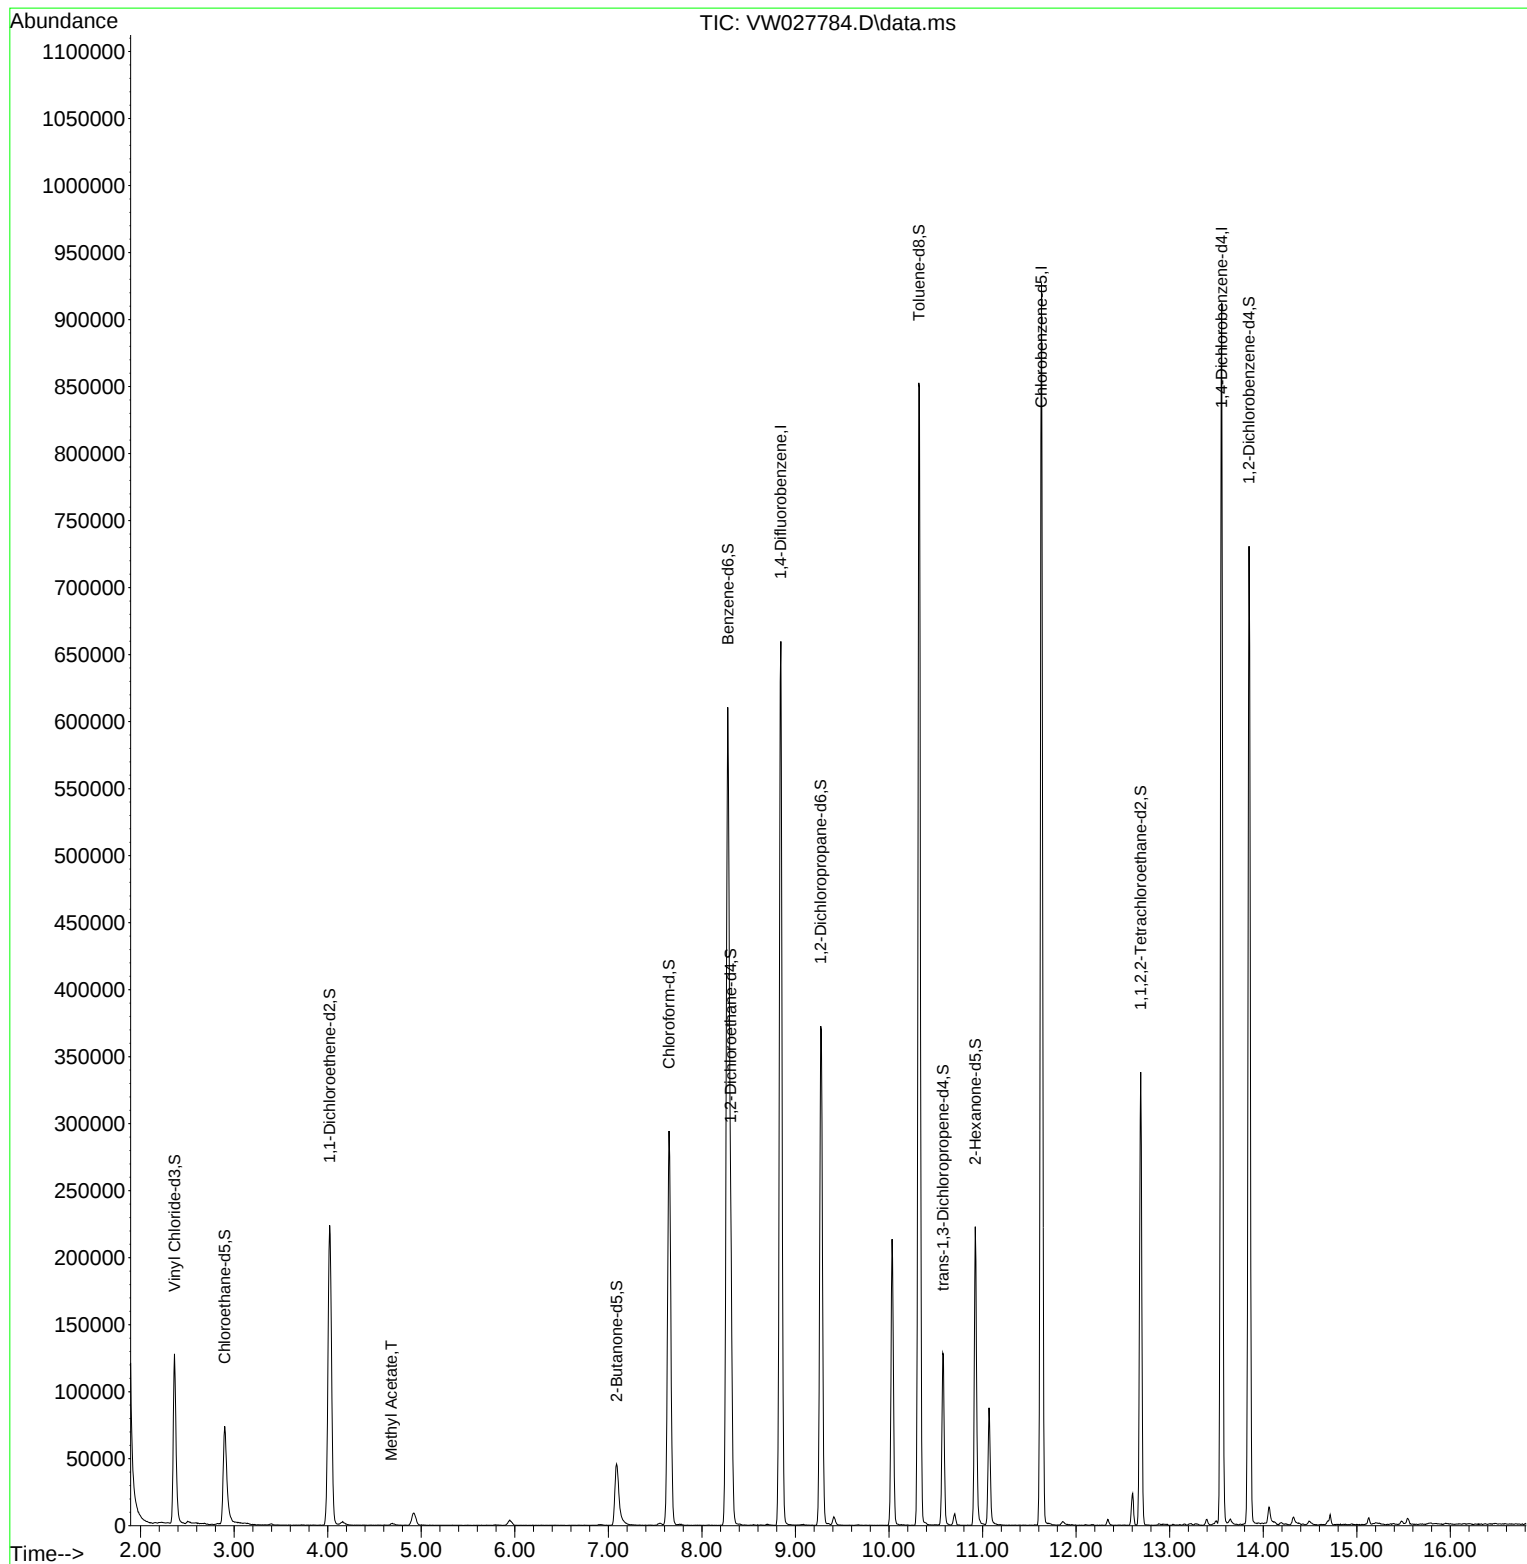

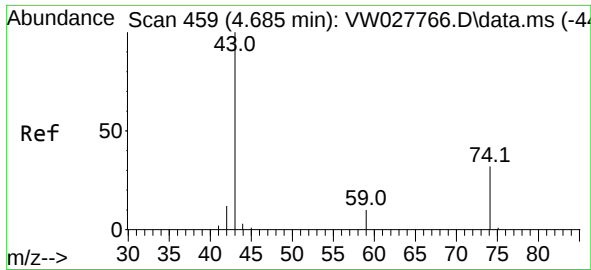

#15
Methyl Acetate
Concen: 1.242 ug/L m
RT: 4.679 min Scan# 41
Delta R.T. -0.018 min
Lab File: VW027784.D
Acq: 19 Dec 2023 17:10

Instrument :
MSVOA_W
ClientSampleId :
C0AZ9

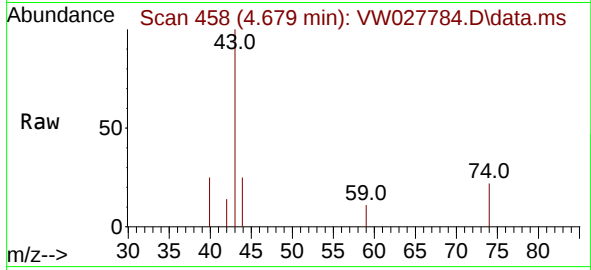

Tgt Ion: 43 Resp: 299
Ion Ratio Lower Upper
43 100
74 16.6 22.1 33.1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2023
Supervised By :Mahesh Dadoda 12/20/2023

