




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122023\
Data File : VW027810.D
Acq On : 20 Dec 2023 15:07
Operator : SY/MD
Sample : 05835-20
Misc : 5.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B24

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/21/2023
Supervised By :Mahesh Dadoda 12/21/2023

Quant Time: Dec 20 23:16:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

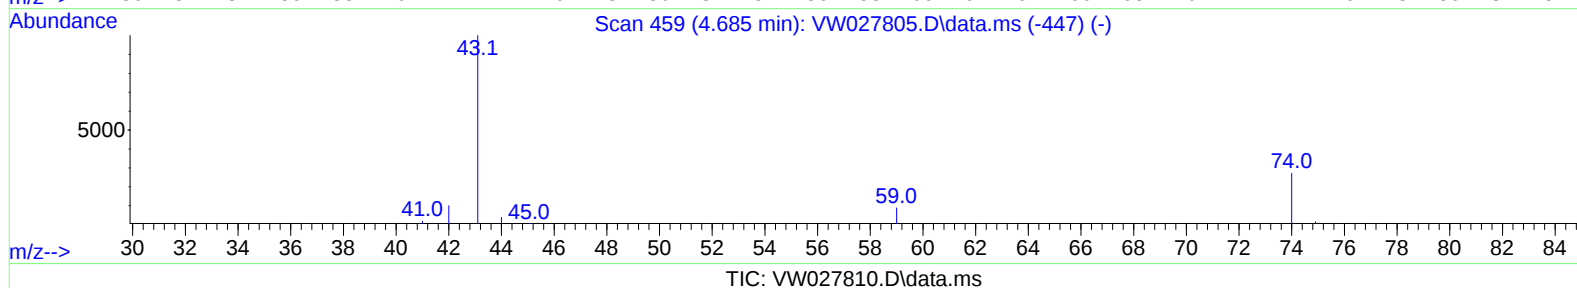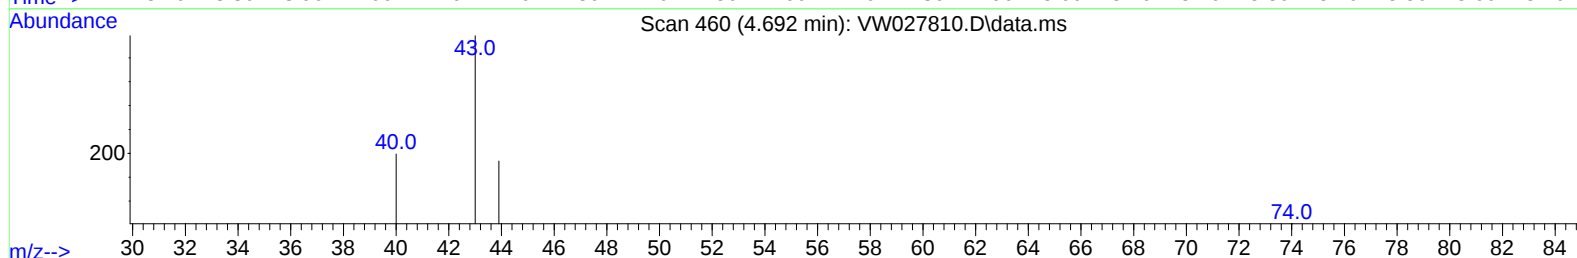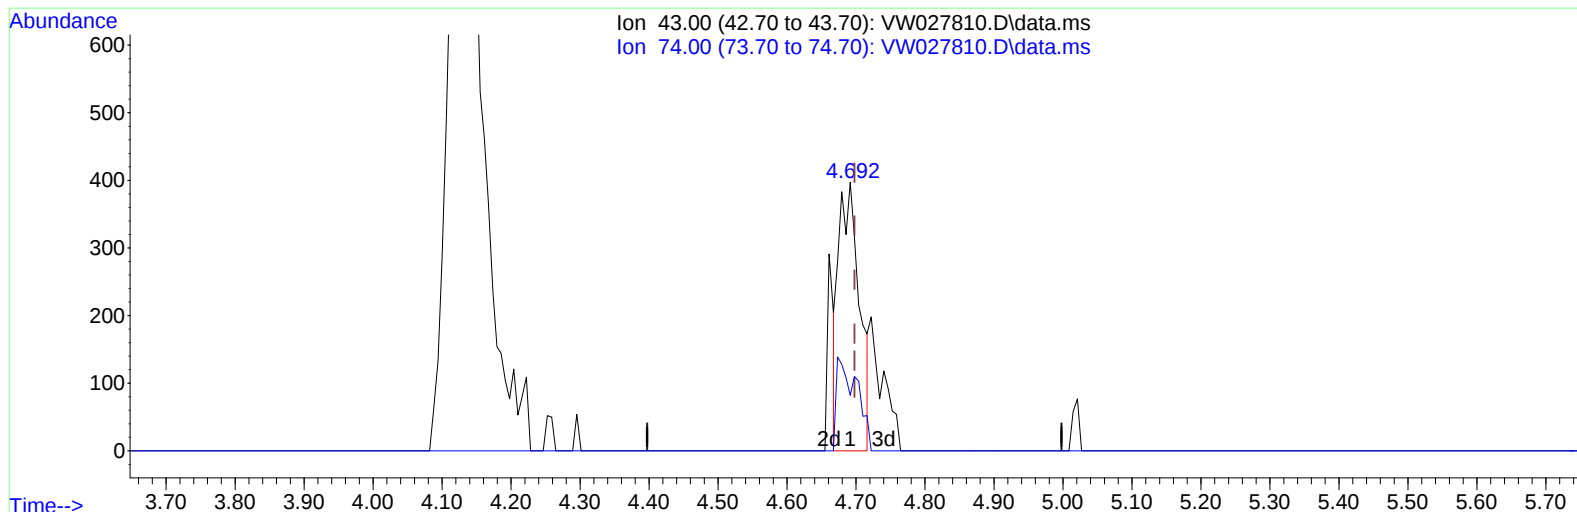

TIC: VW027810.D\data.ms

(15) Methyl Acetate (T)

4.692min (-0.006) 2.67 ug/L

response 831

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.60	13.96#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122023\
 Data File : VW027810.D
 Acq On : 20 Dec 2023 15:07
 Operator : SY/MD
 Sample : 05835-20
 Misc : 5.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B24

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/21/2023
 Supervised By :Mahesh Dadoda 12/21/2023

Quant Time: Dec 20 23:16:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

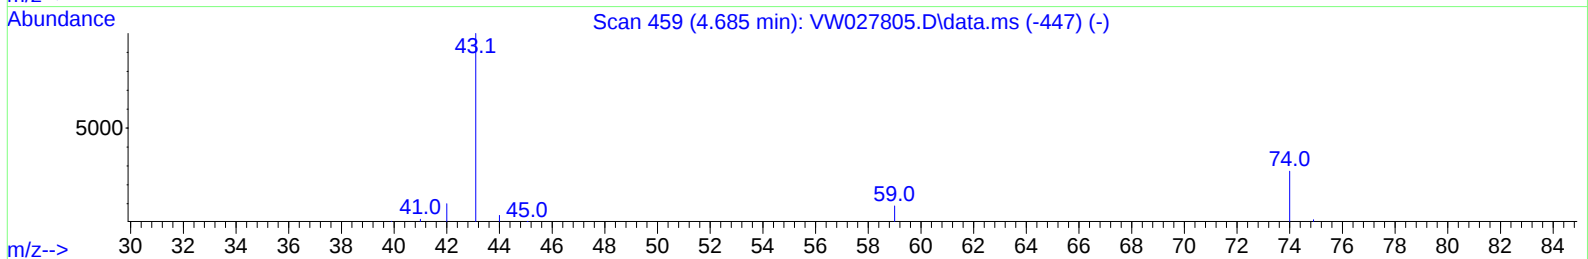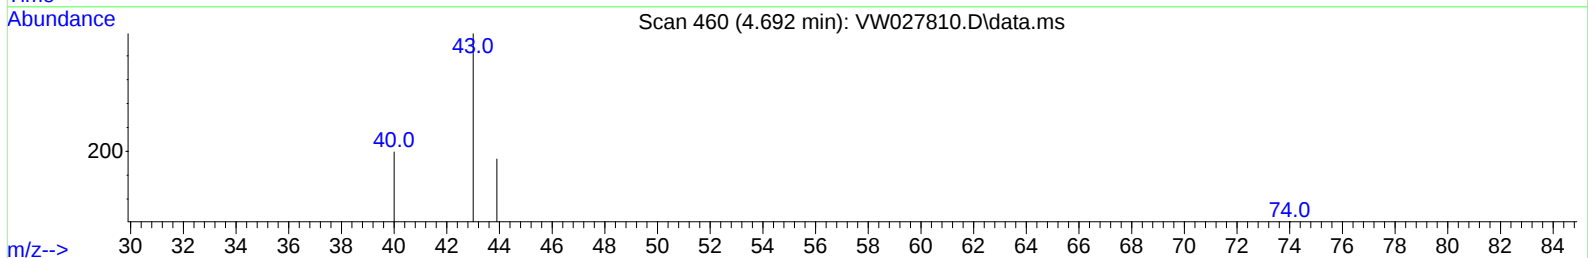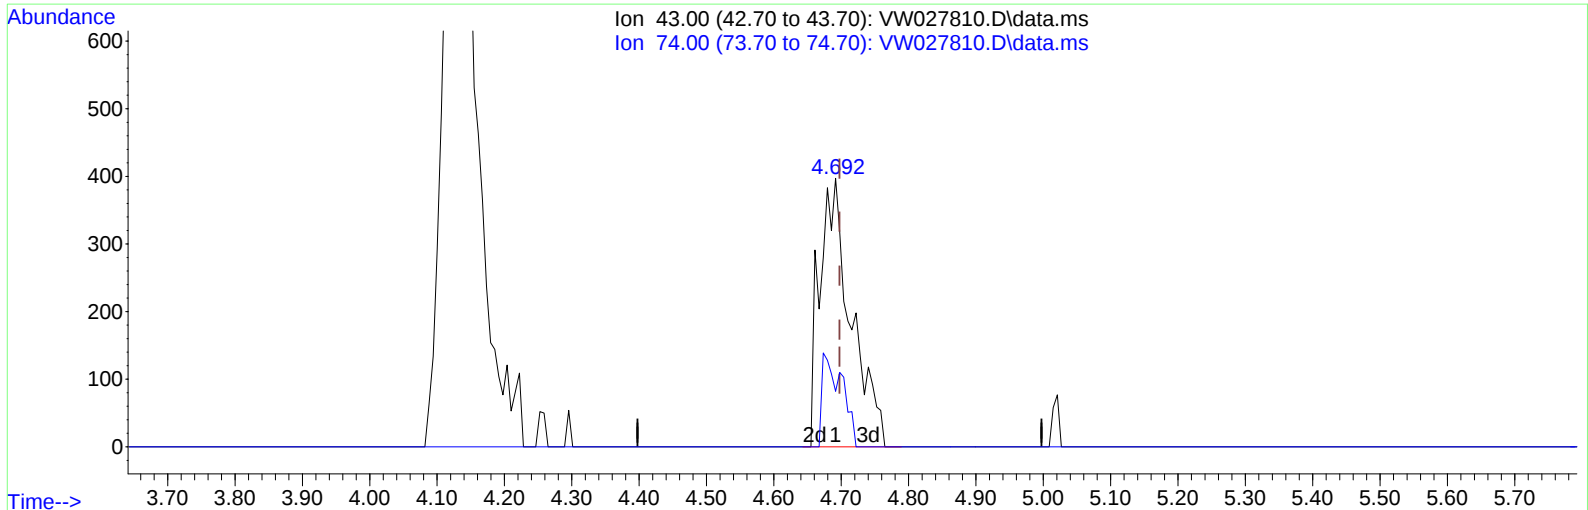

TIC: VW027810.D\data.ms

(15) Methyl Acetate (T)

4.692min (-0.006) 4.12 ug/L m

response 1280

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.60	9.06#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122023\
 Data File : VW027810.D
 Acq On : 20 Dec 2023 15:07
 Operator : SY/MD
 Sample : 05835-20
 Misc : 5.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B24

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/21/2023
 Supervised By :Mahesh Dadoda 12/21/2023

Quant Time: Dec 20 23:16:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	78562	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	70223	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	27529	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	21965	19.742	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.960%		
7) Chloroethane-d5	2.899	69	19080	22.025	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.120%		
11) 1,1-Dichloroethene-d2	4.027	65	8890	19.951	ug/L	0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	79.800%		
21) 2-Butanone-d5	7.081	46	9139	48.237	ug/L	-0.02
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.480%		
24) Chloroform-d	7.654	84	43548	23.295	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.200%		
26) 1,2-Dichloroethane-d4	8.307	65	22543	25.683	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	102.720%		
32) Benzene-d6	8.276	84	86814	21.153	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	84.600%		
36) 1,2-Dichloropropane-d6	9.276	67	26659	22.928	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.720%		
41) Toluene-d8	10.325	98	75241	19.760	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	79.040%		
43) trans-1,3-Dichloroprop...	10.581	79	8756	19.450	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.800%		
47) 2-Hexanone-d5	10.922	63	4324	25.519	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	51.040%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	22960	26.112	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	104.440%		
66) 1,2-Dichlorobenzene-d4	13.849	152	22730	23.066	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.280%		
Target Compounds						Qvalue
13) Acetone	4.131	43	3863	22.461	ug/L	100
15) Methyl Acetate	4.692	43	1280m	4.119	ug/L	
51) Chlorobenzene	11.654	112	3898	1.393	ug/L	96
65) 1,4-Dichlorobenzene	13.574	146	4232	2.509	ug/L	92
70) 1,2,4-trichlorobenzene	15.129	180	632	0.659	ug/L #	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122023\
Data File : VW027810.D
Acq On : 20 Dec 2023 15:07
Operator : SY/MD
Sample : 05835-20
Misc : 5.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B24

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/21/2023
Supervised By :Mahesh Dadoda 12/21/2023

Quant Time: Dec 20 23:16:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

