




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122023\
Data File : VW027812.D
Acq On : 20 Dec 2023 17:03
Operator : SY/MD
Sample : 05835-20RE
Misc : 3.86g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B24RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/21/2023
Supervised By :Mahesh Dadoda 12/21/2023

Quant Time: Dec 20 23:17:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

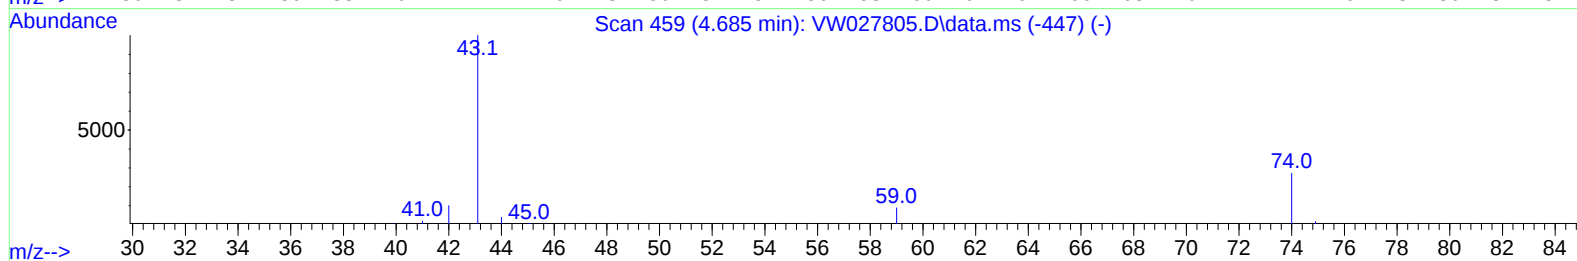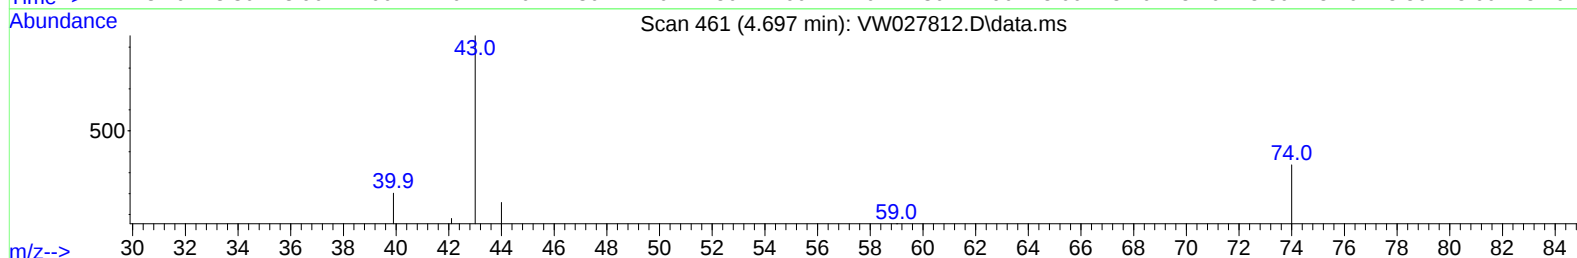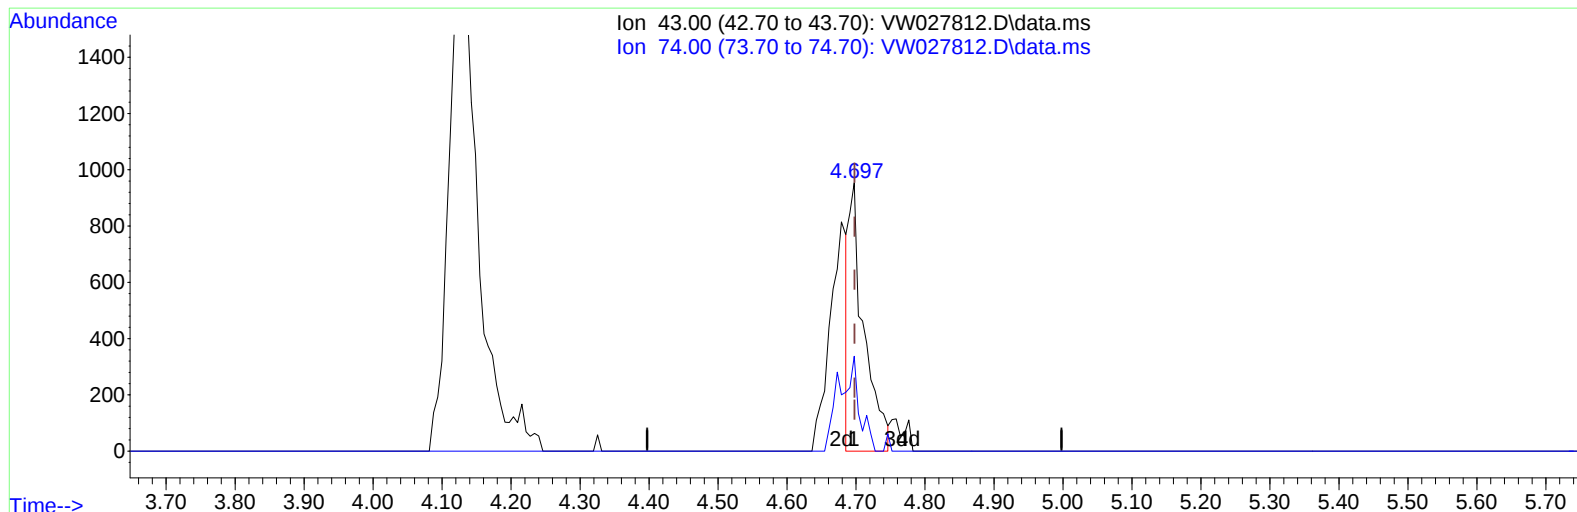

TIC: VW027812.D\data.ms

(15) Methyl Acetate (T)

4.697min (-0.000) 5.47 ug/L

response 1449

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.60	19.39#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122023\
 Data File : VW027812.D
 Acq On : 20 Dec 2023 17:03
 Operator : SY/MD
 Sample : 05835-20RE
 Misc : 3.86g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B24RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/21/2023
 Supervised By :Mahesh Dadoda 12/21/2023

Quant Time: Dec 20 23:17:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

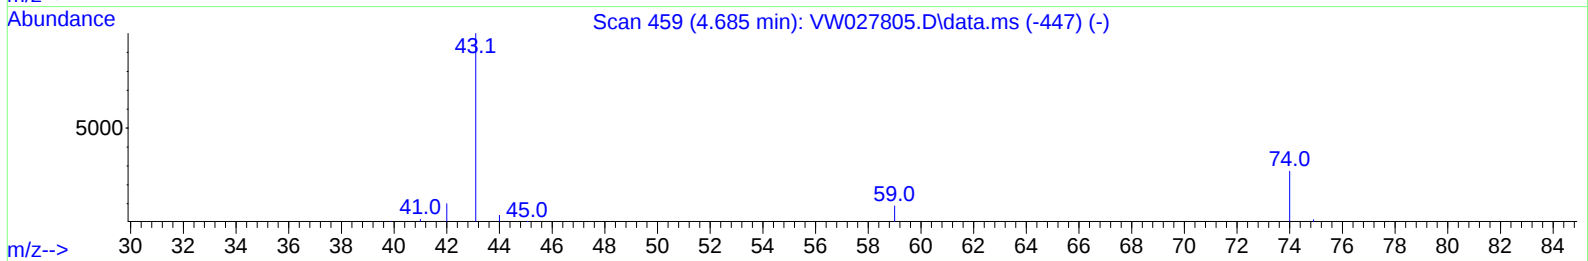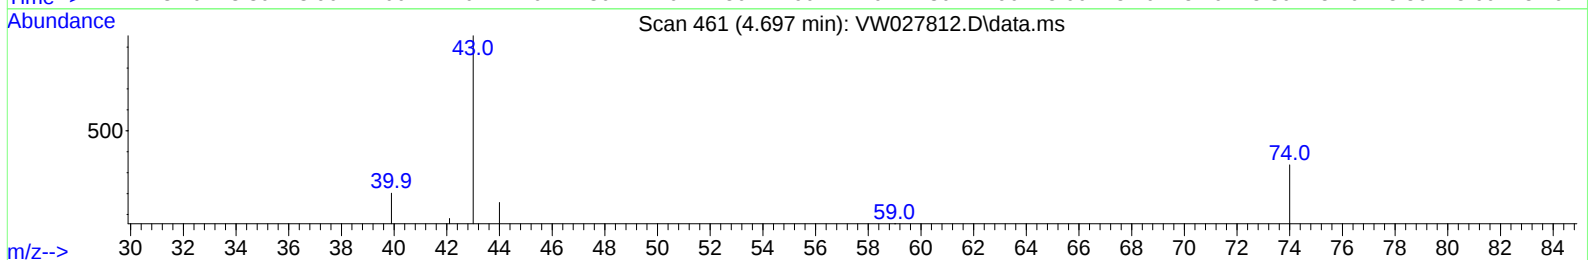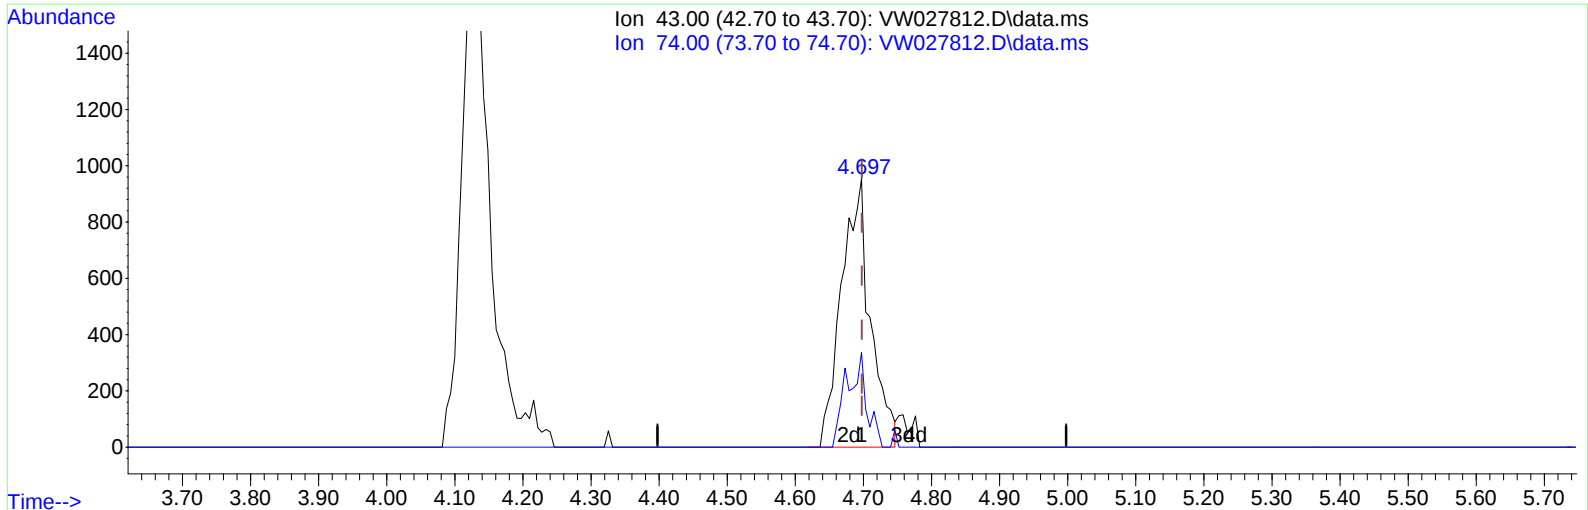

TIC: VW027812.D\data.ms

(15) Methyl Acetate (T)

4.697min (-0.000) 10.63 ug/L m

response 2816

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.60	9.98#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122023\
 Data File : VW027812.D
 Acq On : 20 Dec 2023 17:03
 Operator : SY/MD
 Sample : 05835-20RE
 Misc : 3.86g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B24RE

Manual IntegrationsAPPROVED

Quant Time: Dec 20 23:17:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/21/2023
 Supervised By :Mahesh Dadoda 12/21/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	67000	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	60631	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.549	152	25309	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	17915	18.880	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	75.520%	
7) Chloroethane-d5	2.899	69	15741	21.306	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	85.240%	
11) 1,1-Dichloroethene-d2	4.027	65	7293	19.191	ug/L	0.01
Spiked Amount	25.000	Range 45 - 110	Recovery	=	76.760%	
21) 2-Butanone-d5	7.087	46	6290	38.929	ug/L	-0.01
Spiked Amount	50.000	Range 20 - 135	Recovery	=	77.860%	
24) Chloroform-d	7.654	84	34526	21.656	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	86.640%	
26) 1,2-Dichloroethane-d4	8.306	65	17353	23.182	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	92.720%	
32) Benzene-d6	8.276	84	70277	19.833	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	79.320%	
36) 1,2-Dichloropropane-d6	9.276	67	20650	20.570	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	82.280%	
41) Toluene-d8	10.324	98	60180	18.305	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	73.200%	
43) trans-1,3-Dichloroprop...	10.580	79	6862	17.655	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	70.600%	
47) 2-Hexanone-d5	10.928	63	1545	10.561	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	21.120%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	17041	22.446	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	89.800%	
66) 1,2-Dichlorobenzene-d4	13.848	152	19426	21.443	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	85.760%	
Target Compounds						
13) Acetone	4.130	43	4951	33.755	ug/L	Qvalue 94
15) Methyl Acetate	4.697	43	2816m	10.627	ug/L	
42) Toluene	10.385	91	4728	1.250	ug/L	91
51) Chlorobenzene	11.659	112	2366	0.979	ug/L	94
63) 1,2,4-Trimethylbenzene	13.269	105	21652	7.703	ug/L #	46
65) 1,4-Dichlorobenzene	13.574	146	1870	1.206	ug/L #	77
70) 1,2,4-trichlorobenzene	15.128	180	354	0.401	ug/L #	64

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122023\
Data File : VW027812.D
Acq On : 20 Dec 2023 17:03
Operator : SY/MD
Sample : 05835-20RE
Misc : 3.86g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B24RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/21/2023
Supervised By :Mahesh Dadoda 12/21/2023

Quant Time: Dec 20 23:17:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

