
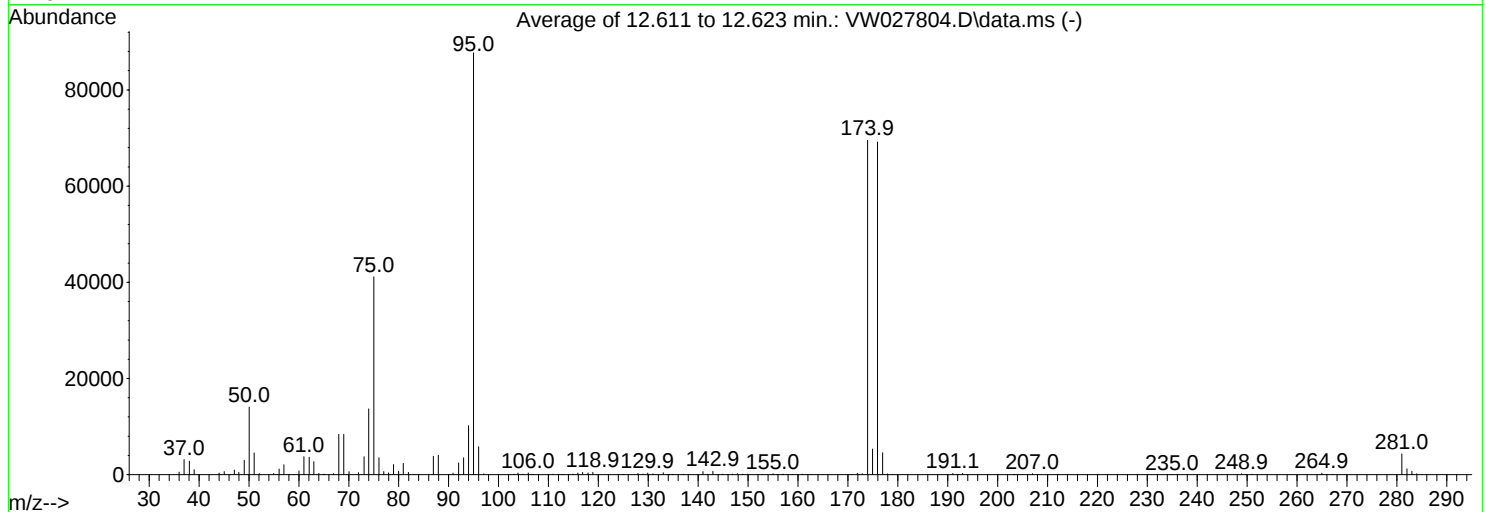


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122023\
Data File : VW027804.D
Acq On : 20 Dec 2023 11:41
Operator : SY/MD
Sample : BFB422
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB422

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Title : SFAM01.0
Last Update : Sun Dec 17 01:25:09 2023

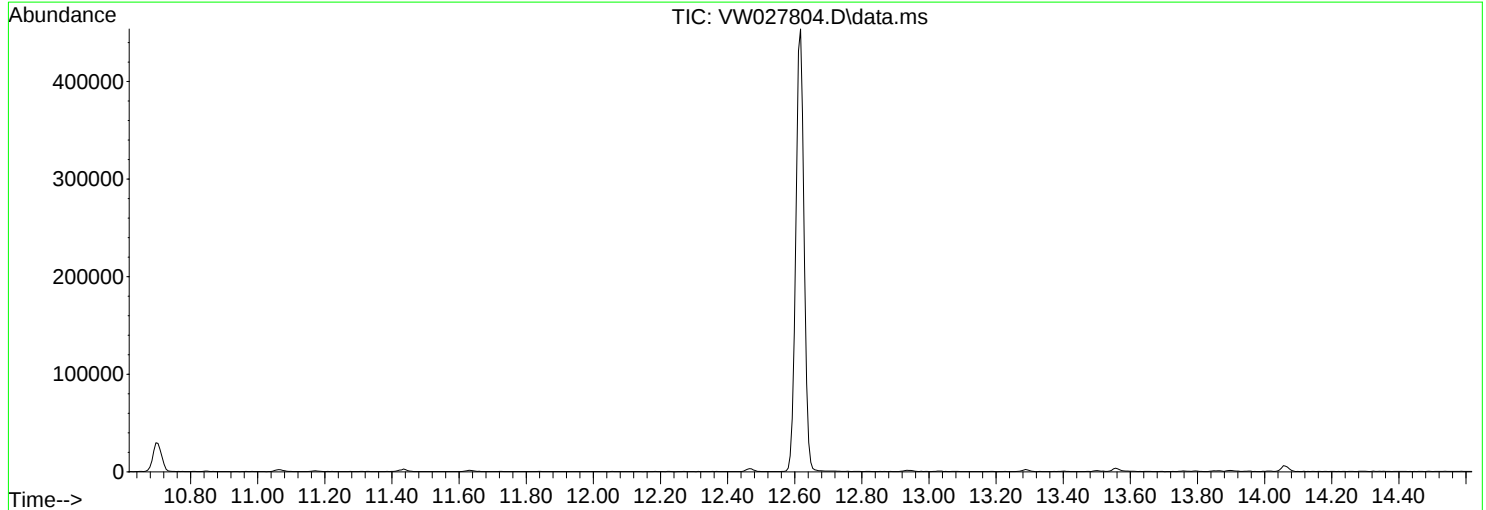

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	14032	PASS
75	95	30	80	46.9	41136	PASS
95	95	100	100	100.0	87715	PASS
96	95	5	9	6.6	5777	PASS
173	174	0.00	2	0.3	211	PASS
174	95	50	120	79.2	69509	PASS
175	174	5	9	7.7	5334	PASS
176	174	95	101	99.5	69176	PASS
177	176	5	9	6.6	4576	PASS

m/z	Abundance
40.00	226.0
44.10	193.0

Instrument :
MSVOA_W
ClientSampleId :
BFB422

m/z	Abundance
36.00	637.0
37.00	3427.0
38.10	2956.0
39.00	1187.0
40.00	256.0
44.00	590.0
45.10	750.0
46.30	64.0
47.10	1131.0
48.00	547.0
49.10	3231.0
50.00	14942.0
51.00	4851.0
52.10	266.0
54.90	229.0
56.10	1290.0
57.00	2235.0
58.10	95.0
59.00	86.0
60.00	872.0
61.00	4005.0
62.00	3899.0
63.00	2676.0
64.10	216.0
64.90	223.0
66.90	235.0
68.00	8847.0
69.00	9203.0
70.00	657.0
71.90	494.0
73.10	3906.0
74.00	13826.0
75.00	42528.0
76.00	3787.0
77.00	707.0
77.90	456.0
79.00	2058.0
80.00	774.0
80.90	2492.0
82.00	423.0
83.10	58.0
86.00	106.0
87.00	4479.0
88.00	3936.0
90.90	434.0
92.00	2521.0
93.00	3628.0
94.00	10603.0
95.00	91312.0
96.00	5847.0
97.10	154.0
103.10	118.0
103.90	396.0
104.90	174.0
105.90	474.0
107.00	77.0
110.00	65.0
110.90	104.0
112.70	86.0
113.10	57.0
115.00	108.0
115.90	372.0
116.90	460.0
117.90	402.0
118.90	544.0
125.00	195.0
126.00	154.0
128.00	309.0
129.00	127.0
129.90	316.0
130.90	223.0
133.00	791.0
133.80	110.0
134.80	211.0
136.90	115.0
140.90	556.0
141.80	120.0
143.00	620.0
144.90	77.0
145.80	171.0
146.90	168.0
147.90	205.0
148.80	112.0
149.90	75.0
152.90	72.0
155.00	162.0
156.90	168.0
157.80	67.0
158.90	53.0
160.90	99.0
162.80	69.0
165.00	97.0

Instrument :
MSVOA_W
ClientSampleId :
BFB422

170.80	78.0
171.90	307.0
172.90	632.0
174.00	68936.0
174.90	4936.0
176.00	64672.0
176.90	4639.0
177.90	161.0
179.00	111.0
191.00	504.0
192.00	106.0
193.00	371.0
194.00	72.0
203.20	52.0
204.90	106.0
207.00	385.0
208.10	96.0
235.00	61.0
248.90	393.0
249.90	79.0
250.90	153.0
264.90	499.0
266.00	83.0
267.20	151.0
279.90	60.0
281.00	7160.0
282.00	1835.0
283.00	1202.0
284.00	225.0
285.00	97.0

Instrument :
MSVOA_W
ClientSampleId :
BFB422

m/z	Abundance
36.00	554.0
37.00	3584.0
38.00	3243.0
39.00	1166.0
40.00	246.0
44.00	447.0
45.00	639.0
47.00	1050.0
48.00	534.0
49.10	3267.0
50.10	15944.0
51.10	4977.0
52.00	194.0
55.00	227.0
56.00	1280.0
57.00	2201.0
58.00	79.0
60.00	891.0
61.00	4351.0
62.10	3767.0
63.00	3355.0
64.00	306.0
65.10	178.0
67.00	188.0
68.00	9212.0
69.00	9716.0
70.10	757.0
72.00	467.0
73.00	4387.0
74.00	15703.0
75.00	45024.0
76.10	3990.0
77.00	654.0
78.00	396.0
78.90	2443.0
80.00	760.0
80.90	2597.0
81.90	550.0
83.10	91.0
86.00	136.0
87.00	3744.0
87.90	4590.0
90.90	378.0
92.00	2685.0
93.00	3774.0
94.00	11741.0
95.00	97048.0
96.00	6581.0
97.00	266.0
103.10	103.0
103.90	347.0
104.80	71.0
106.00	397.0
107.00	126.0
110.80	141.0
114.80	112.0
115.90	364.0
116.80	602.0
118.00	437.0
118.90	483.0
125.20	106.0
125.90	90.0
127.90	287.0
128.90	151.0
129.90	480.0
131.00	111.0
133.00	221.0
133.70	73.0
134.10	55.0
135.00	151.0
137.00	123.0
141.00	788.0
141.90	72.0
143.00	802.0
145.00	107.0
146.00	113.0
146.90	68.0
147.80	149.0
148.90	96.0
149.90	97.0
152.80	71.0
155.00	300.0
157.10	164.0
158.80	85.0
160.90	151.0
162.70	51.0
170.80	54.0
171.90	288.0
174.00	68784.0
175.00	6207.0
175.90	76464.0
177.00	5402.0

Instrument :
MSVOA_W
ClientSampleId :
BFB422

177.90	199.0
179.00	69.0
191.10	201.0
192.10	50.0
193.00	458.0
207.00	174.0
208.00	66.0
248.90	236.0
251.00	143.0
265.00	315.0
265.90	98.0
267.00	68.0
281.00	3939.0
282.00	1233.0
283.00	697.0
283.90	208.0

Instrument :
MSVOA_W
ClientSampleId :
BFB422

m/z	Abundance
36.00	408.0
37.00	2405.0
38.10	2213.0
39.10	784.0
40.00	292.0
44.00	524.0
45.00	502.0
47.00	697.0
47.90	467.0
49.00	2541.0
50.00	11209.0
51.00	3789.0
52.10	106.0
54.90	232.0
56.10	979.0
57.00	1753.0
58.10	71.0
60.00	562.0
61.00	2814.0
62.00	3204.0
63.00	2074.0
63.90	247.0
65.00	115.0
66.90	176.0
68.00	7151.0
69.00	6245.0
70.00	507.0
71.90	352.0
73.00	2870.0
74.00	11552.0
75.00	35856.0
76.10	2817.0
77.00	530.0
78.00	228.0
78.90	1836.0
80.00	609.0
80.90	1865.0
82.00	398.0
83.00	56.0
86.00	68.0
86.90	3282.0
88.00	3571.0
91.00	206.0
92.00	2047.0
93.00	3076.0
94.00	8249.0
95.00	74784.0
96.00	4904.0
97.00	115.0
103.00	64.0
103.90	278.0
105.00	103.0
105.90	235.0
106.70	107.0
111.00	76.0
112.90	57.0
114.90	85.0
115.90	281.0
116.90	388.0
117.90	265.0
118.90	505.0
124.80	62.0
127.90	226.0
129.00	151.0
129.90	223.0
130.90	214.0
133.00	154.0
134.90	97.0
137.10	75.0
140.90	526.0
142.00	91.0
142.90	690.0
143.90	57.0
144.90	98.0
146.00	138.0
147.00	61.0
147.90	242.0
148.90	83.0
149.90	105.0
155.00	189.0
155.80	56.0
157.00	126.0
158.90	111.0
160.90	102.0
171.90	303.0
173.90	70808.0
174.90	4860.0
175.90	66392.0
176.90	3687.0
177.90	113.0
191.00	130.0
207.10	84.0

Instrument :
MSVOA_W
ClientSampleId :
BFB422

264.90	115.0
281.10	1930.0
282.00	544.0
282.90	237.0
283.20	255.0
284.00	87.0

Instrument :

MSVOA_W

ClientSampleId :

BFB422