

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
 Data File : VW031416.D
 Acq On : 20 Dec 2024 10:36
 Operator : SY/MD
 Sample : P5258-13
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 20 21:59:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 20 21:58:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	534656	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	476253	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	226091	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	194272	24.150	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.600%
7) Chloroethane-d5	2.899	69	161072	27.067	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.280%
11) 1,1-Dichloroethene-d2	4.015	65	88535	23.202	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	92.800%
21) 2-Butanone-d5	7.094	46	80896	53.397	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.800%
24) Chloroform-d	7.648	84	378852	25.862	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.440%
26) 1,2-Dichloroethane-d4	8.490	65	94	0.013	ug/L	0.19
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.270	84	762677	24.985	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.960%
36) 1,2-Dichloropropane-d6	9.270	67	222409	25.000	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.000%
41) Toluene-d8	10.319	98	693204	24.411	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.640%
43) trans-1,3-Dichloroprop...	10.575	79	88976	21.690	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.760%
47) 2-Hexanone-d5	10.922	63	64332	53.771	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.540%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	158446	28.366	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.480%
66) 1,2-Dichlorobenzene-d4	13.854	152	219890	26.198	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.800%
Target Compounds					Qvalue	
25) Chloroform	7.673	83	11278	0.866	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
Data File : VW031416.D
Acq On : 20 Dec 2024 10:36
Operator : SY/MD
Sample : P5258-13
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 20 21:59:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 20 21:58:26 2024
Response via : Initial Calibration

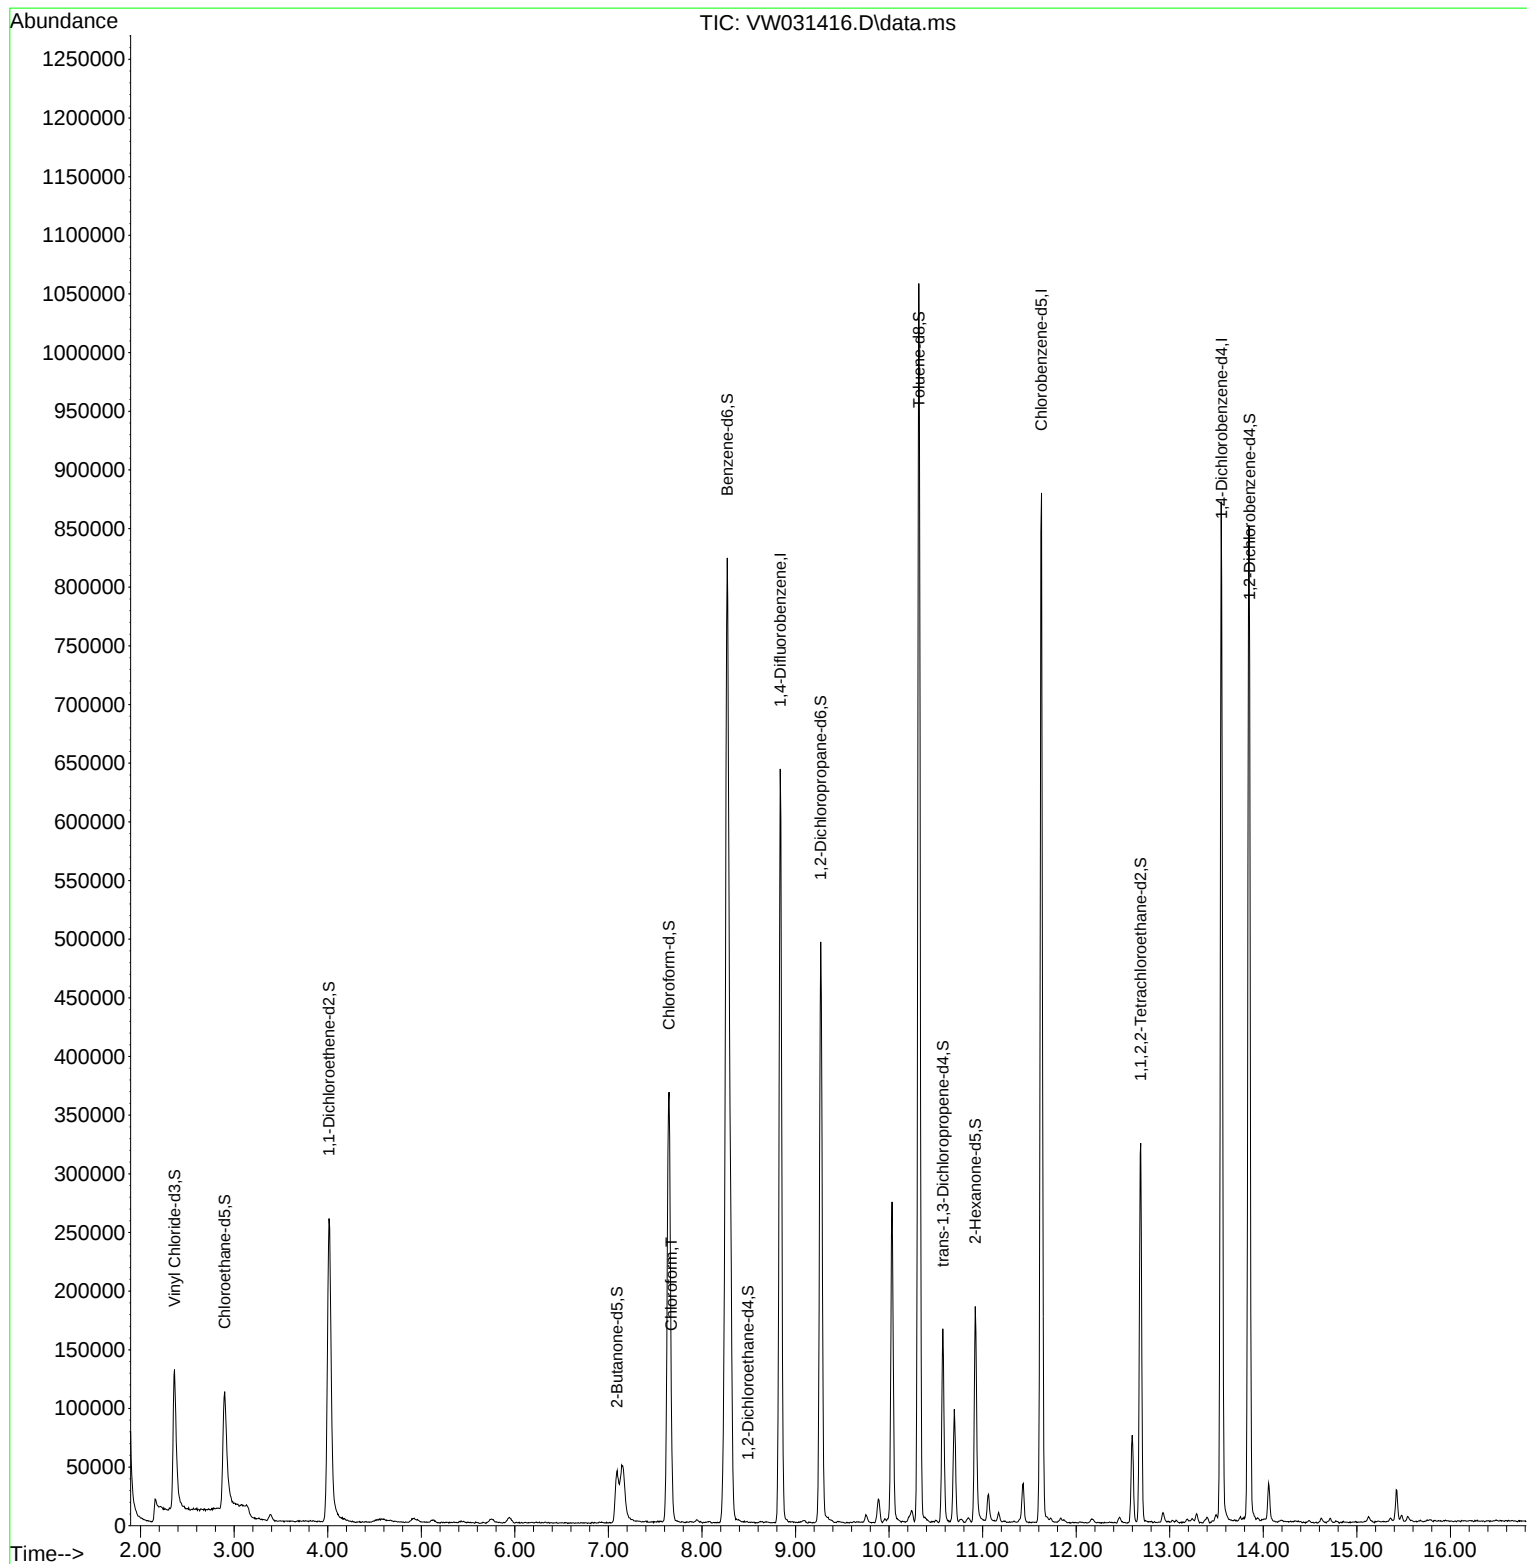

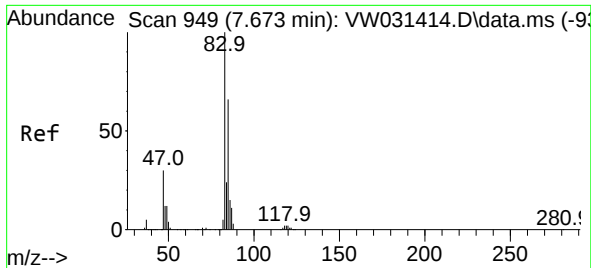

#25
 Chloroform
 Concen: 0.866 ug/L
 RT: 7.673 min Scan# 949
 Delta R.T. -0.000 min
 Lab File: VW031416.D
 Acq: 20 Dec 2024 10:36

Instrument :
 MSVOA_W
 ClientSampleId :

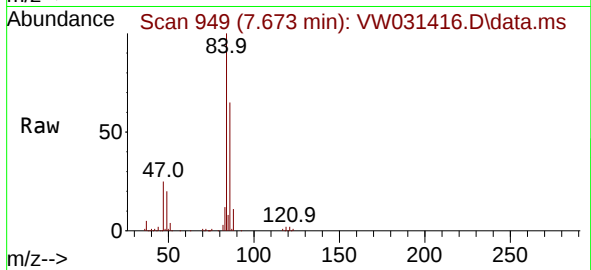

Tgt Ion: 83 Resp: 11278
 Ion Ratio Lower Upper
 83 100
 85 67.8 46.1 85.5

