

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
 Data File : VW031426.D
 Acq On : 20 Dec 2024 14:38
 Operator : SY/MD
 Sample : P5265-06
 Misc : 5.06g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 20 22:03:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 20 21:58:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	590630	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	524647	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	260300	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	147601	16.609	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.440%
7) Chloroethane-d5	2.893	69	126751	19.281	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.120%
11) 1,1-Dichloroethene-d2	4.015	65	66099	15.680	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.720%
21) 2-Butanone-d5	7.094	46	77178	46.115	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.240%
24) Chloroform-d	7.642	84	309143	19.103	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	76.400%
26) 1,2-Dichloroethane-d4	8.301	65	174466	21.467	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.880%
32) Benzene-d6	8.270	84	618683	18.398	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.600%
36) 1,2-Dichloropropane-d6	9.270	67	189399	19.326	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	77.320%
41) Toluene-d8	10.319	98	565403	18.074	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.280%
43) trans-1,3-Dichloroprop...	10.575	79	72269	15.993	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	63.960%
47) 2-Hexanone-d5	10.922	63	59583	45.208	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.420%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	146614	23.827	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	191100	19.776	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.120%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	6400	0.468	ug/L	# 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
Data File : VW031426.D
Acq On : 20 Dec 2024 14:38
Operator : SY/MD
Sample : P5265-06
Misc : 5.06g/10mL/MSVOA_W/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 20 22:03:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 20 21:58:26 2024
Response via : Initial Calibration

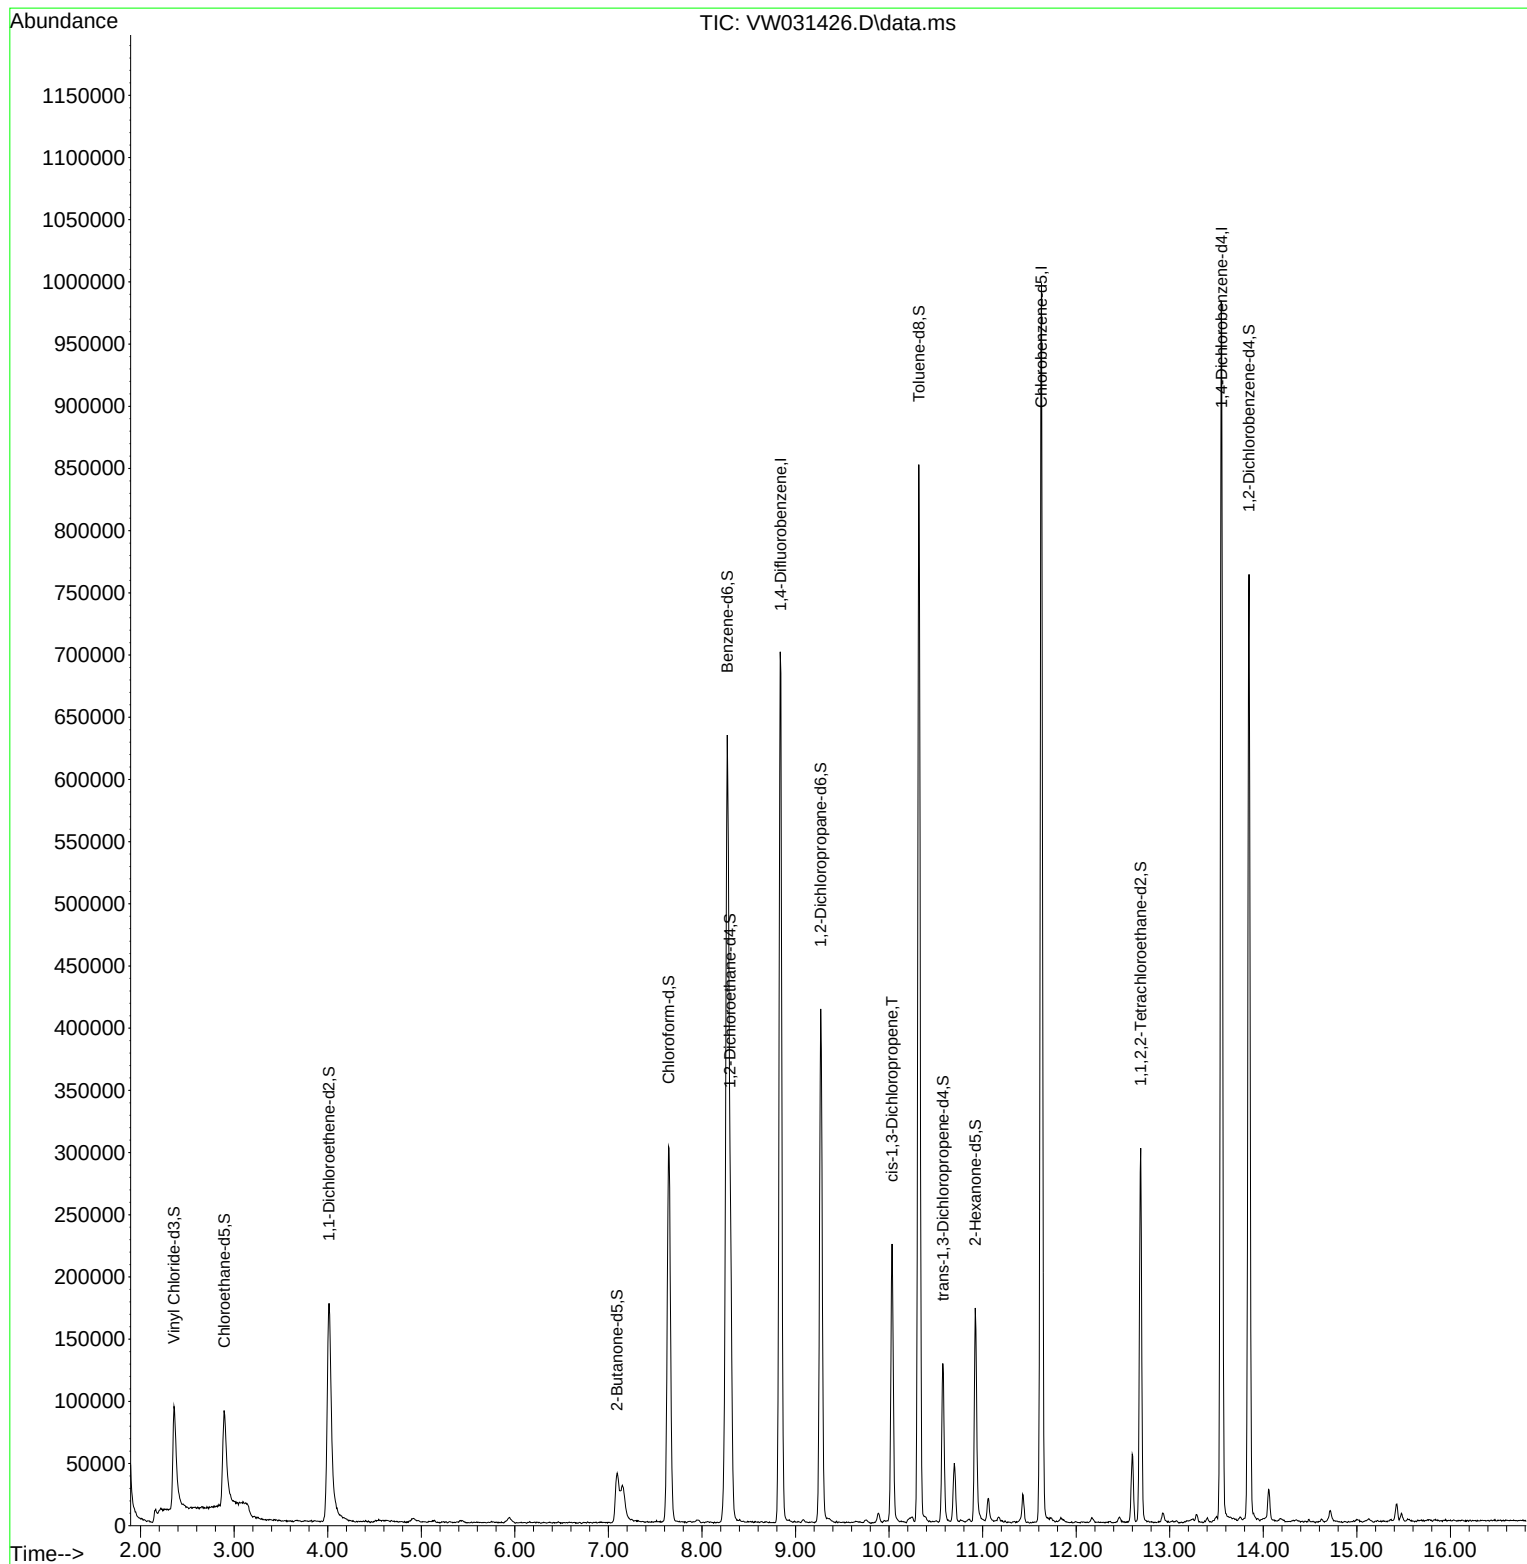

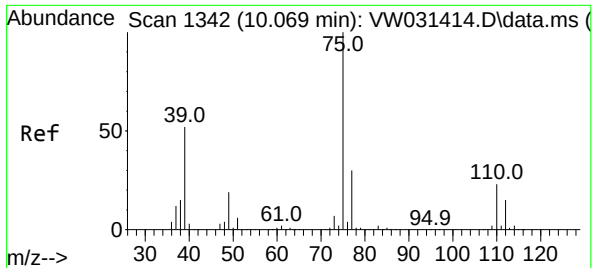

#39
 cis-1,3-Dichloropropene
 Concen: 0.468 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW031426.D
 Acq: 20 Dec 2024 14:38

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 6400
 Ion Ratio Lower Upper
 75 100
 77 52.5 21.8 40.4#

