




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
 Data File : VW031432.D
 Acq On : 20 Dec 2024 17:02
 Operator : SY/MD
 Sample : P5333-07RE
 Misc : 7.53g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E2910RE

Manual IntegrationsAPPROVED

Quant Time: Dec 20 22:04:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 20 21:58:26 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/23/2024
 Supervised By :Mahesh Dadoda 12/23/2024

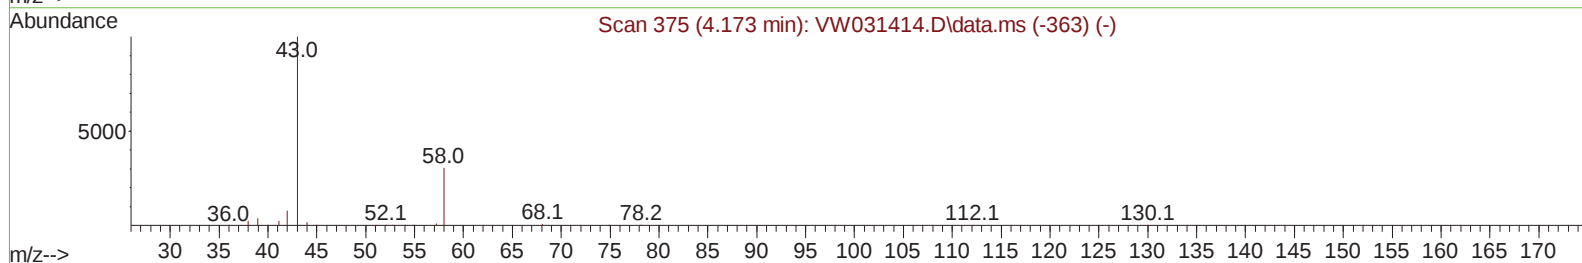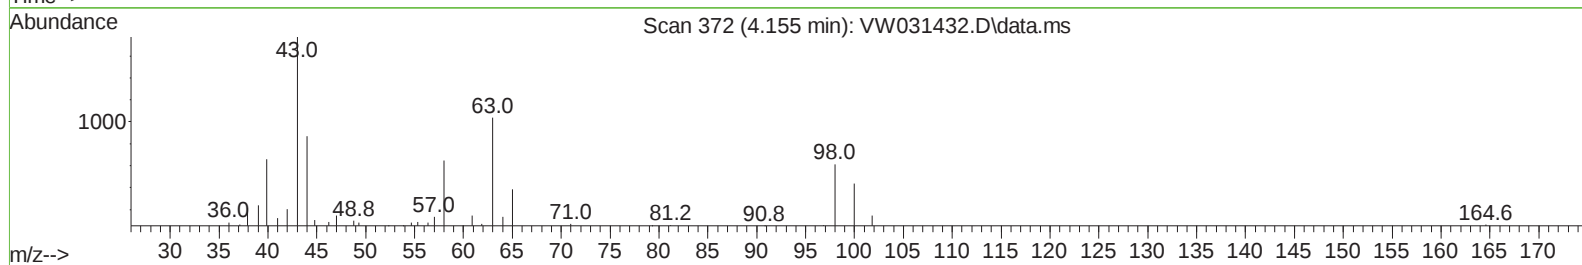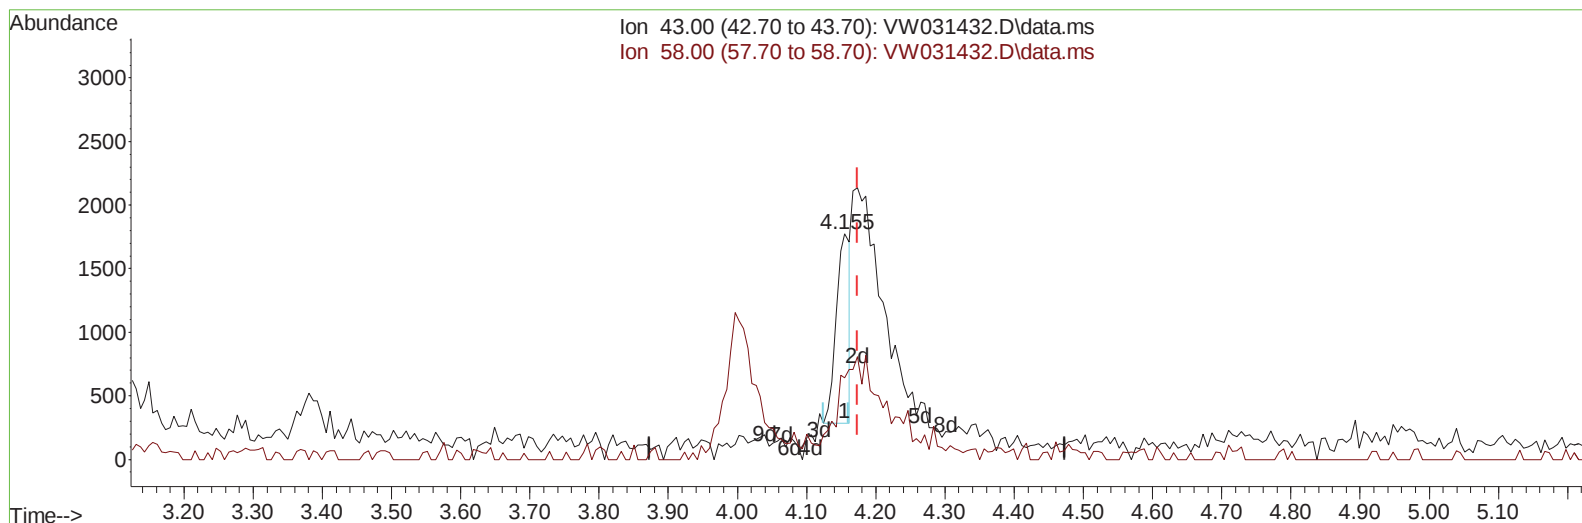

TIC: VW031432.D\data.ms

(13) Acetone (T)

4.155min (-0.018) 1.55 ug/L

response 2040

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	0.00	14.36#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
 Data File : VW031432.D
 Acq On : 20 Dec 2024 17:02
 Operator : SY/MD
 Sample : P5333-07RE
 Misc : 7.53g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E2910RE

Manual IntegrationsAPPROVED

Quant Time: Dec 20 22:04:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 20 21:58:26 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/23/2024
 Supervised By :Mahesh Dadoda 12/23/2024

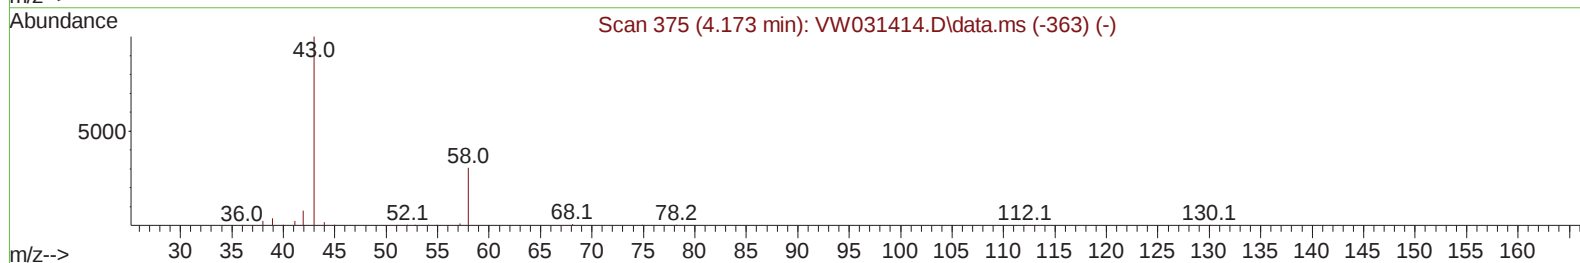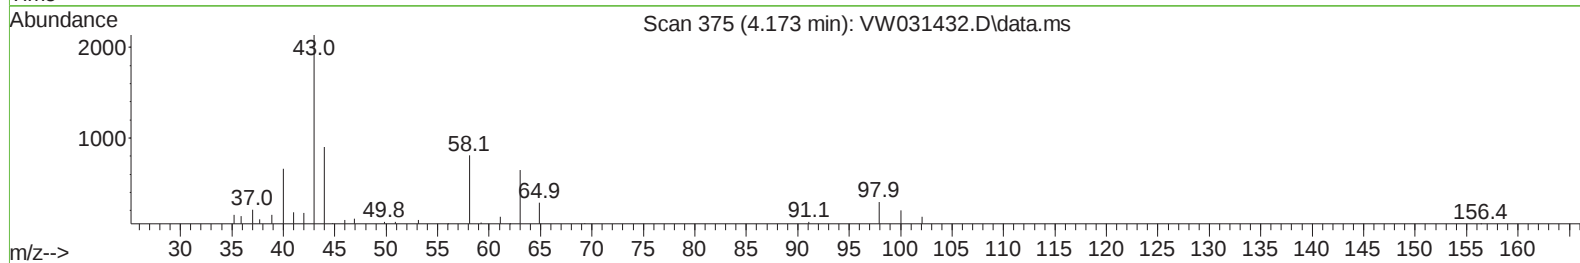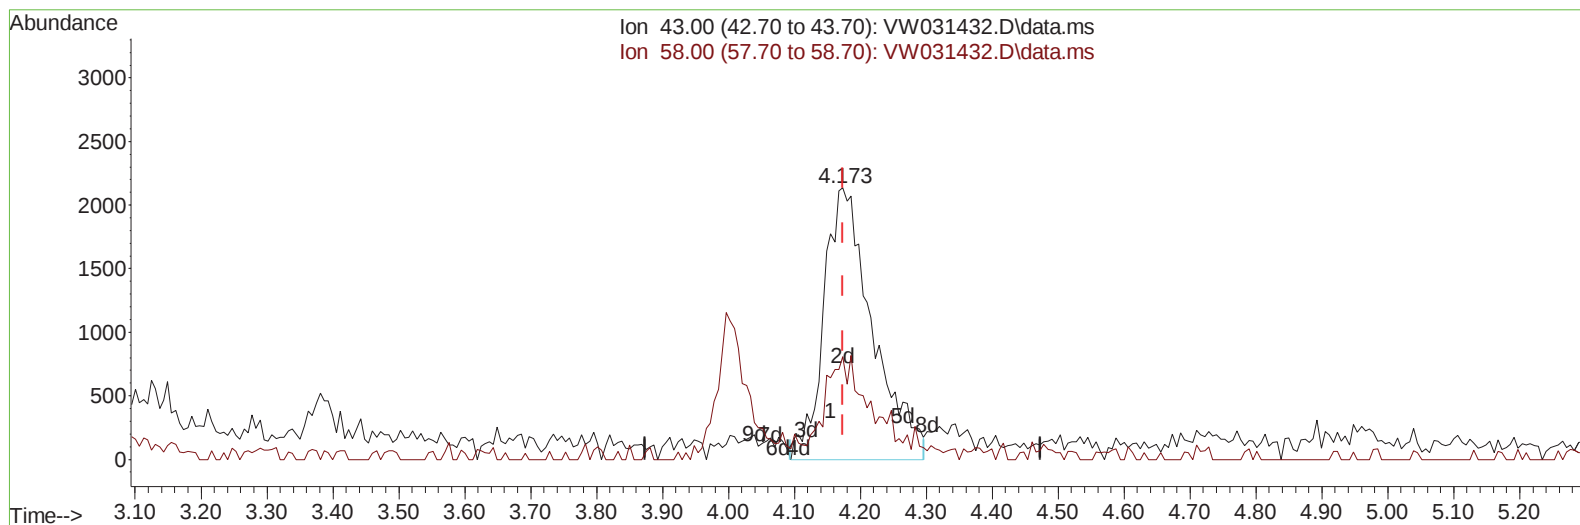

TIC: VW031432.D\data.ms

(13) Acetone (T)

4.173min (0.000) 8.33 ug/L m

response 10964

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	0.00	2.67#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
 Data File : VW031432.D
 Acq On : 20 Dec 2024 17:02
 Operator : SY/MD
 Sample : P5333-07RE
 Misc : 7.53g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E2910RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
 Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 22:04:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 20 21:58:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	333502	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	101675	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	15963	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	199020	39.662	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	158.640%#	
7) Chloroethane-d5	2.893	69	152976	41.212	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	164.840%#	
11) 1,1-Dichloroethene-d2	4.015	65	53592	22.515	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	90.080%	
21) 2-Butanone-d5	7.094	46	103652	109.685	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	219.360%#	
24) Chloroform-d	7.648	84	231447	25.329	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	101.320%	
26) 1,2-Dichloroethane-d4	8.307	65	139962	30.499	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	122.000%	
32) Benzene-d6	8.270	84	413807	63.499	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	254.000%#	
36) 1,2-Dichloropropane-d6	9.270	67	142699	75.133	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	300.520%#	
41) Toluene-d8	10.319	98	180248	29.731	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	118.920%	
43) trans-1,3-Dichloroprop...	10.575	79	20352	23.239	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	92.960%	
47) 2-Hexanone-d5	10.922	63	54567	213.636	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	427.280%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	100679	84.426	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	337.720%#	
66) 1,2-Dichlorobenzene-d4	13.848	152	13338	22.507	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	90.040%	
Target Compounds						Qvalue
13) Acetone	4.173	43	10964m	8.331	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
Data File : VW031432.D
Acq On : 20 Dec 2024 17:02
Operator : SY/MD
Sample : P5333-07RE
Misc : 7.53g/10mL/MSVOA_W/SOIL/B
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E2910RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 22:04:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 20 21:58:26 2024
Response via : Initial Calibration

