




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
 Data File : VW031448.D
 Acq On : 21 Dec 2024 00:15
 Operator : SY/MD
 Sample : P5325-01
 Misc : 6.07g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YE680

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
 Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 21 01:34:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 20 23:42:37 2024
 Response via : Initial Calibration

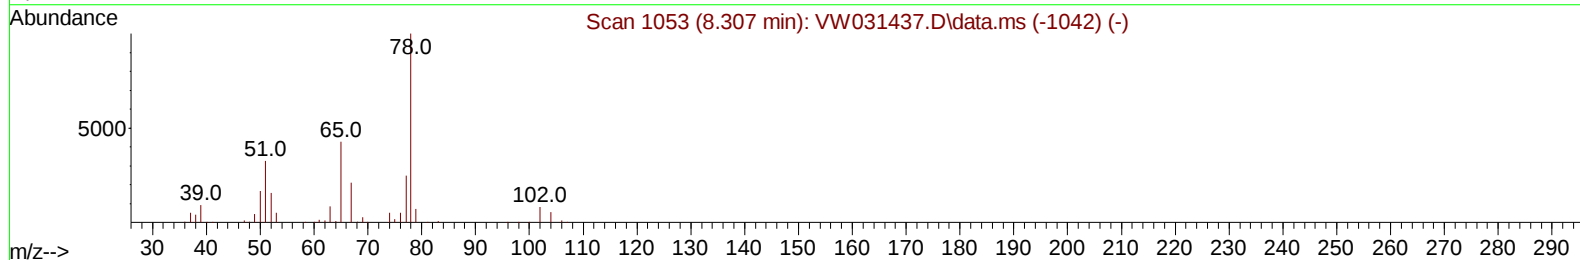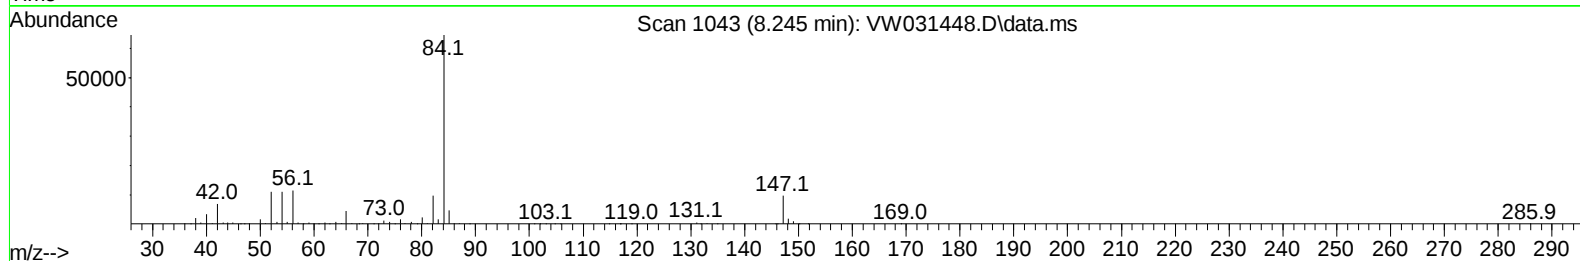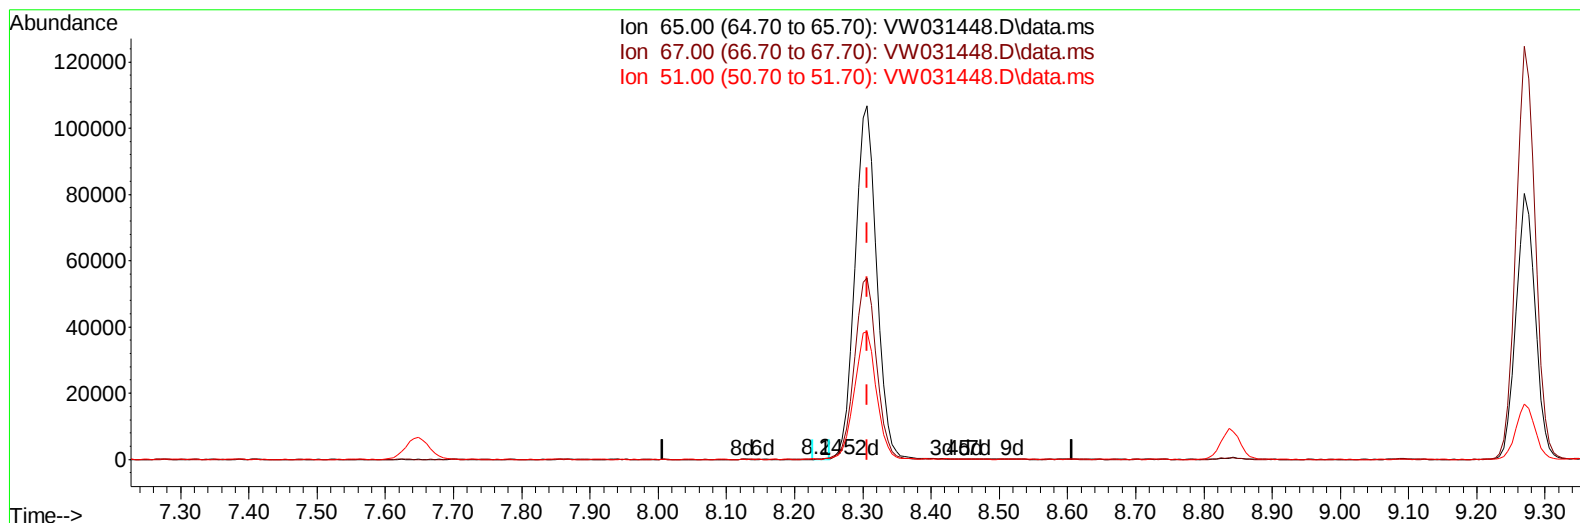

TIC: VW031448.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.245min (-0.061) 0.02 ug/L

response 224

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	68.75
51.00	108.10	77.23
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
Data File : VW031448.D
Acq On : 21 Dec 2024 00:15
Operator : SY/MD
Sample : P5325-01
Misc : 6.07g/10mL/MSVOA_W/SOIL/A
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YE680

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 21 01:34:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 20 23:42:37 2024
Response via : Initial Calibration

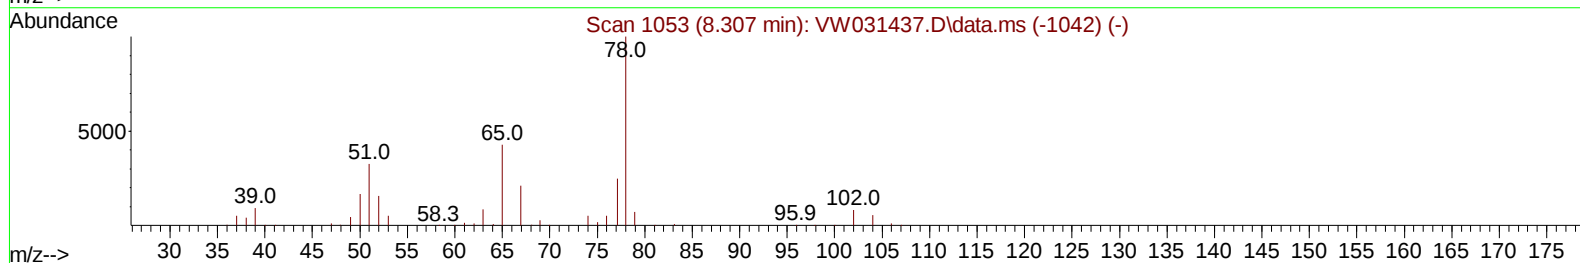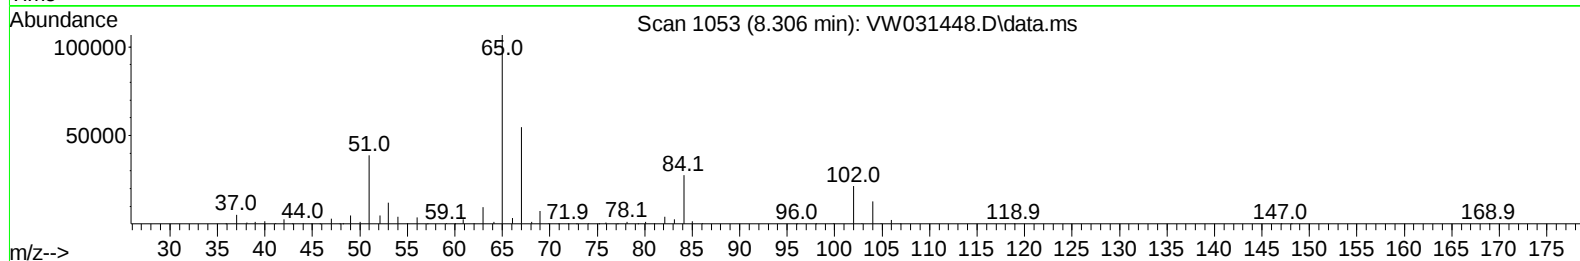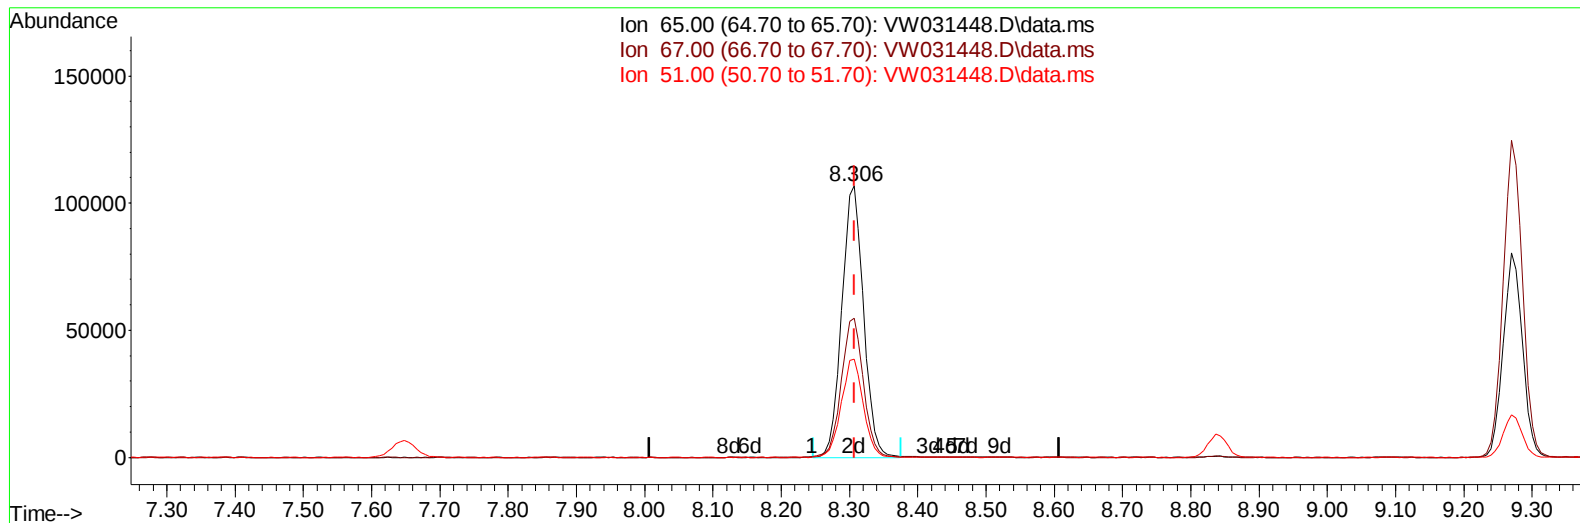

TIC: VW031448.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.306min (-0.000) 18.80 ug/L m

response 235573

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.07#
51.00	108.10	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122024\
 Data File : VW031448.D
 Acq On : 21 Dec 2024 00:15
 Operator : SY/MD
 Sample : P5325-01
 Misc : 6.07g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YE680

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
 Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 21 01:34:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 20 23:42:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	910648	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	703583	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	263626	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	232080	16.938	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.760%	
7) Chloroethane-d5	2.899	69	181380	17.895	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.600%	
11) 1,1-Dichloroethene-d2	4.015	65	96787	14.892	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	59.560%	
21) 2-Butanone-d5	7.093	46	102196	39.605	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	79.220%	
24) Chloroform-d	7.648	84	406278	16.283	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	65.120%	
26) 1,2-Dichloroethane-d4	8.306	65	235573m	18.800	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	75.200%	
32) Benzene-d6	8.276	84	814158	18.054	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	72.200%	
36) 1,2-Dichloropropane-d6	9.270	67	245685	18.693	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	74.760%	
41) Toluene-d8	10.318	98	671548	16.007	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	64.040%	
43) trans-1,3-Dichloroprop...	10.574	79	87831	14.493	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	57.960%	
47) 2-Hexanone-d5	10.922	63	80818	45.725	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.440%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	186580	22.610	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	90.440%	
66) 1,2-Dichlorobenzene-d4	13.848	152	172418	17.617	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	70.480%#	
Target Compounds						
12) 1,1-Dichloroethene	4.039	96	35326	3.164	ug/L #	1
34) Trichloroethene	9.093	95	24971	2.034	ug/L	85
46) Tetrachloroethene	10.855	164	14540	1.617	ug/L	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
Data File : VW031448.D
Acq On : 21 Dec 2024 00:15
Operator : SY/MD
Sample : P5325-01
Misc : 6.07g/10mL/MSVOA_W/SOIL/A
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YE680

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 21 01:34:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 20 23:42:37 2024
Response via : Initial Calibration

