

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
 Data File : VW031440.D
 Acq On : 20 Dec 2024 21:03
 Operator : SY/MD
 Sample : P5333-19
 Misc : 11.21g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E2921

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
 Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 23:43:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 20 23:42:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	292985	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	96487	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	14083	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	182767	41.460	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 165.840%#			
7) Chloroethane-d5	2.893	69	139974	42.924	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 171.680%#			
11) 1,1-Dichloroethene-d2	4.021	65	56501	27.020	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 108.080%			
21) 2-Butanone-d5	7.112	46	4509m	5.431	ug/L	0.02
Spiked Amount 50.000	Range 20 - 135		Recovery = 10.860%#			
24) Chloroform-d	7.648	84	188121	23.434	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 93.720%			
26) 1,2-Dichloroethane-d4	8.307	65	115458	28.639	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 114.560%			
32) Benzene-d6	8.270	84	320823	51.877	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 207.520%#			
36) 1,2-Dichloropropane-d6	9.270	67	89503	49.658	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 198.640%#			
41) Toluene-d8	10.319	98	137943	23.977	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 95.920%			
43) trans-1,3-Dichloroprop...	10.575	79	15014	18.066	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 72.280%			
47) 2-Hexanone-d5	10.934	63	1975	8.148	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery = 16.300%#			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	37544	33.176	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 132.720%#			
66) 1,2-Dichlorobenzene-d4	13.849	152	9602	18.366	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 73.480%#			
Target Compounds			Qvalue			
15) Methyl Acetate	4.698	43	6207	4.727	ug/L #	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122024\
Data File : VW031440.D
Acq On : 20 Dec 2024 21:03
Operator : SY/MD
Sample : P5333-19
Misc : 11.21g/10mL/MSVOA_W/SOIL/A
ALS Vial : 31 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
E2921

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/23/2024

Quant Time: Dec 20 23:43:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 20 23:42:37 2024
Response via : Initial Calibration

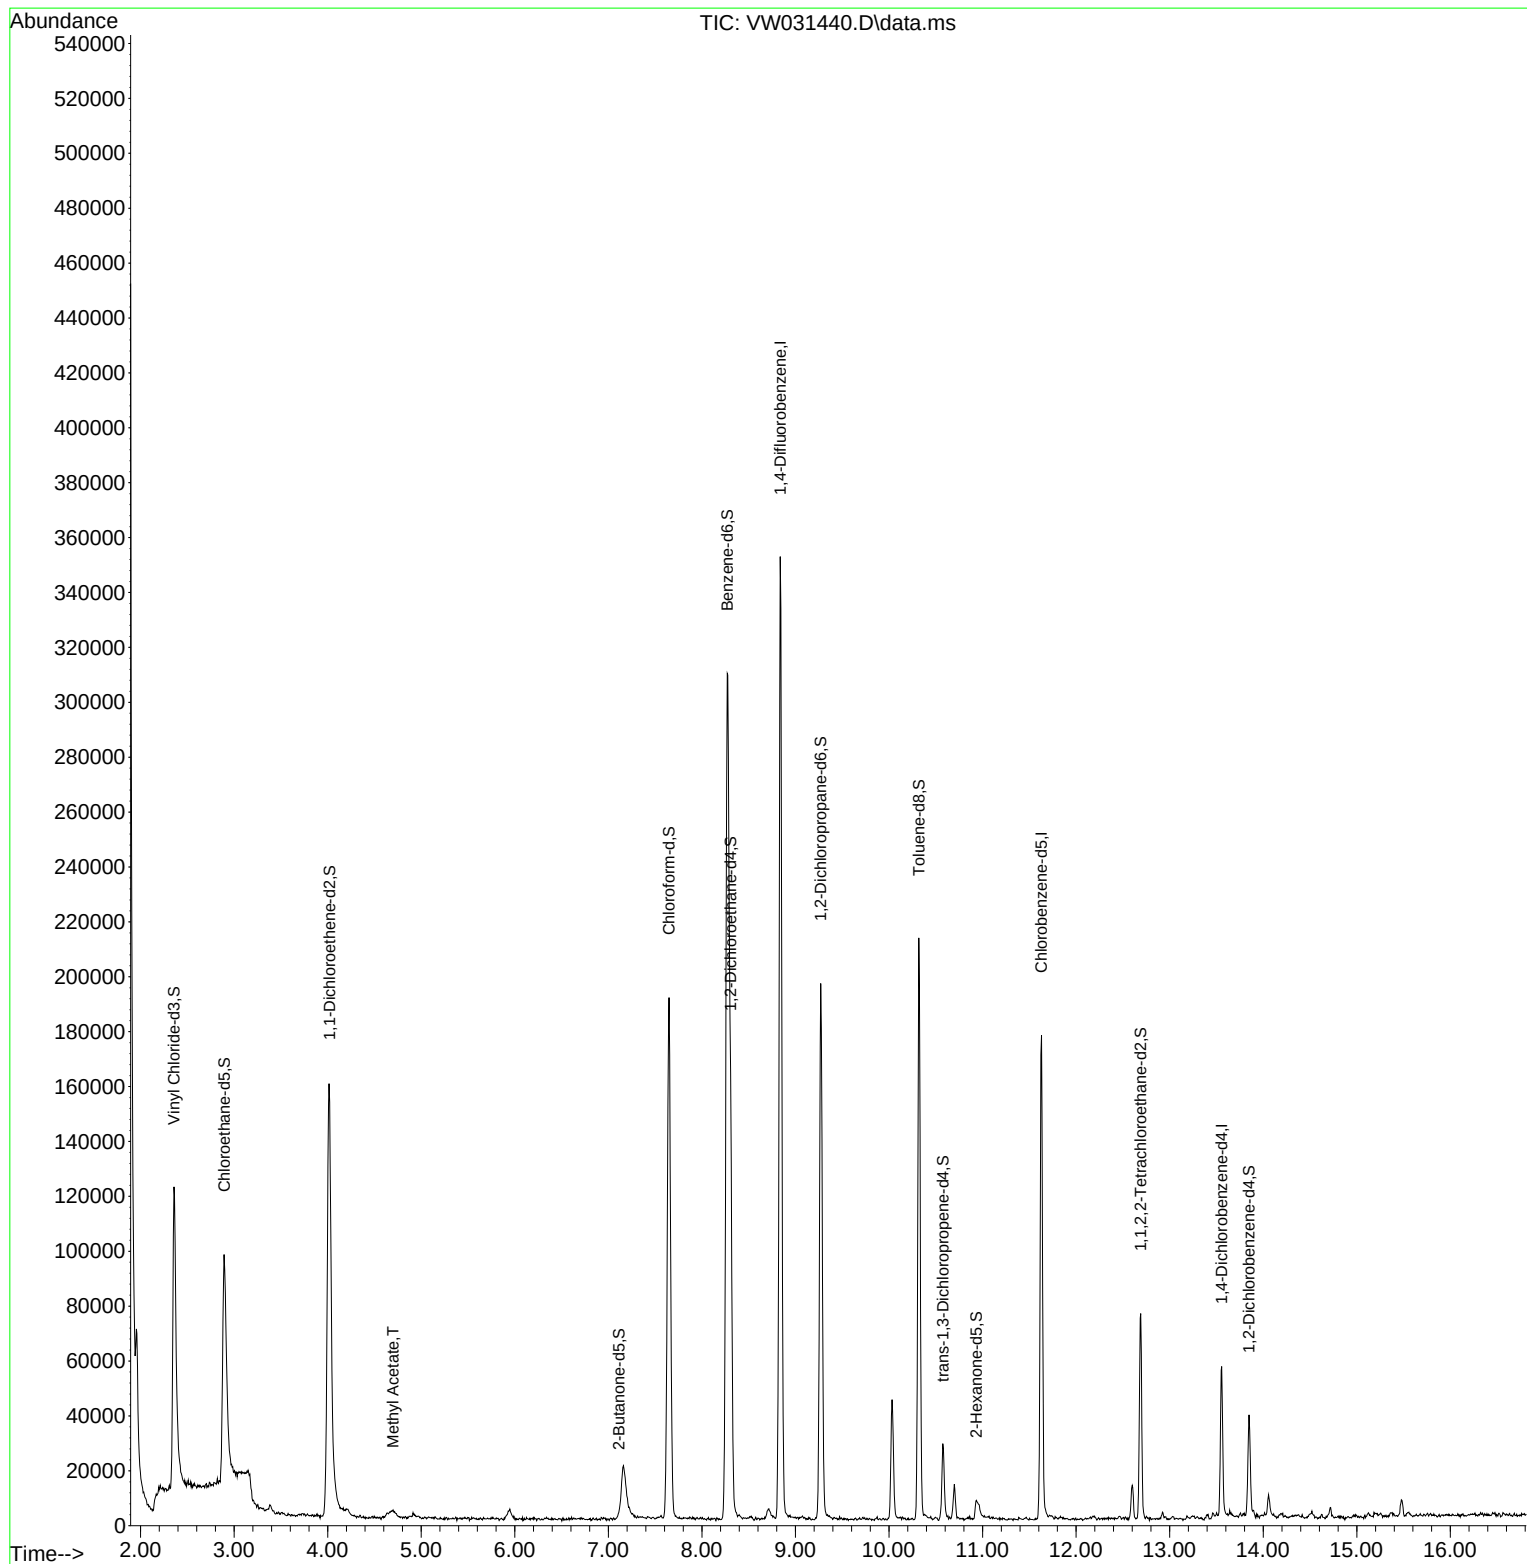

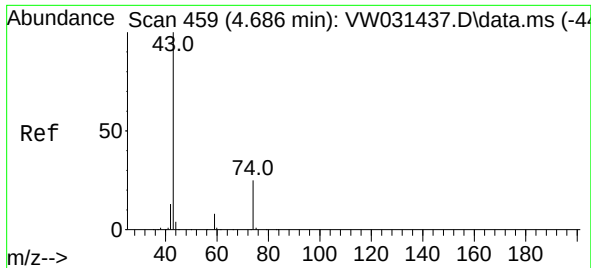

#15

Methyl Acetate

Concen: 4.727 ug/L

RT: 4.698 min Scan# 40

Delta R.T. 0.012 min

Lab File: VW031440.D

Acq: 20 Dec 2024 21:03

Instrument :

MSVOA_W

ClientSampleId :

E2921

Tgt Ion: 43 Resp: 620

Ion Ratio Lower Upper

43 100

74 14.0 18.9 28.3

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024

Supervised By :Mahesh Dadoda 12/23/2024

