




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122121\
Data File : VW021541.D
Acq On : 21 Dec 2021 22:41
Operator : SY/VA
Sample : M5194-07
Misc : 7.08g/10.0mL/MSVOA_W/SOIL
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLB9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/22/2021
Supervised By :Amit Patel 12/24/2021

Quant Time: Dec 22 03:52:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 22 02:57:00 2021
Response via : Initial Calibration

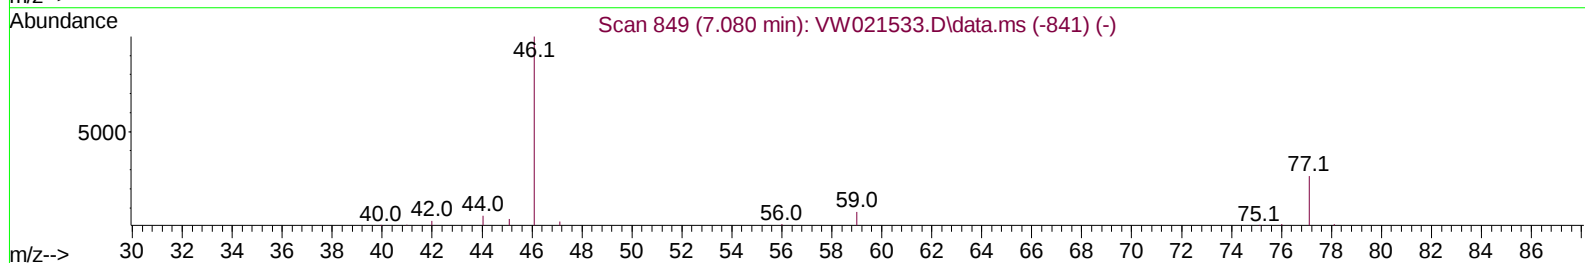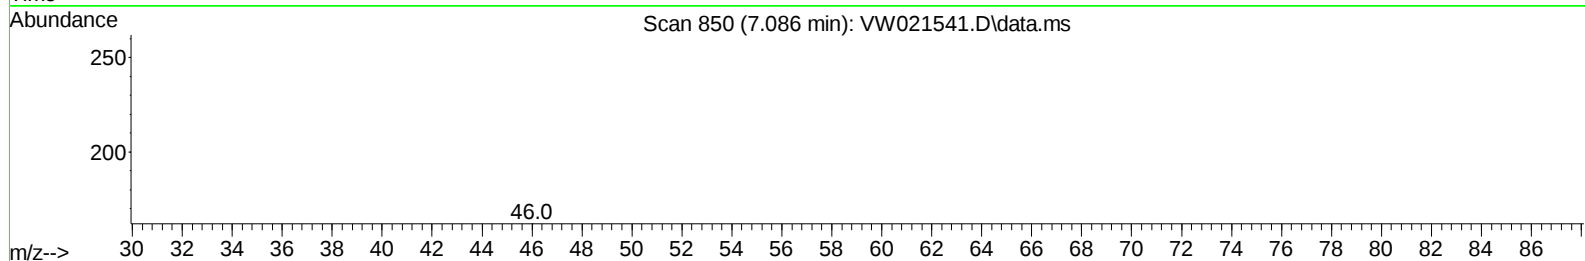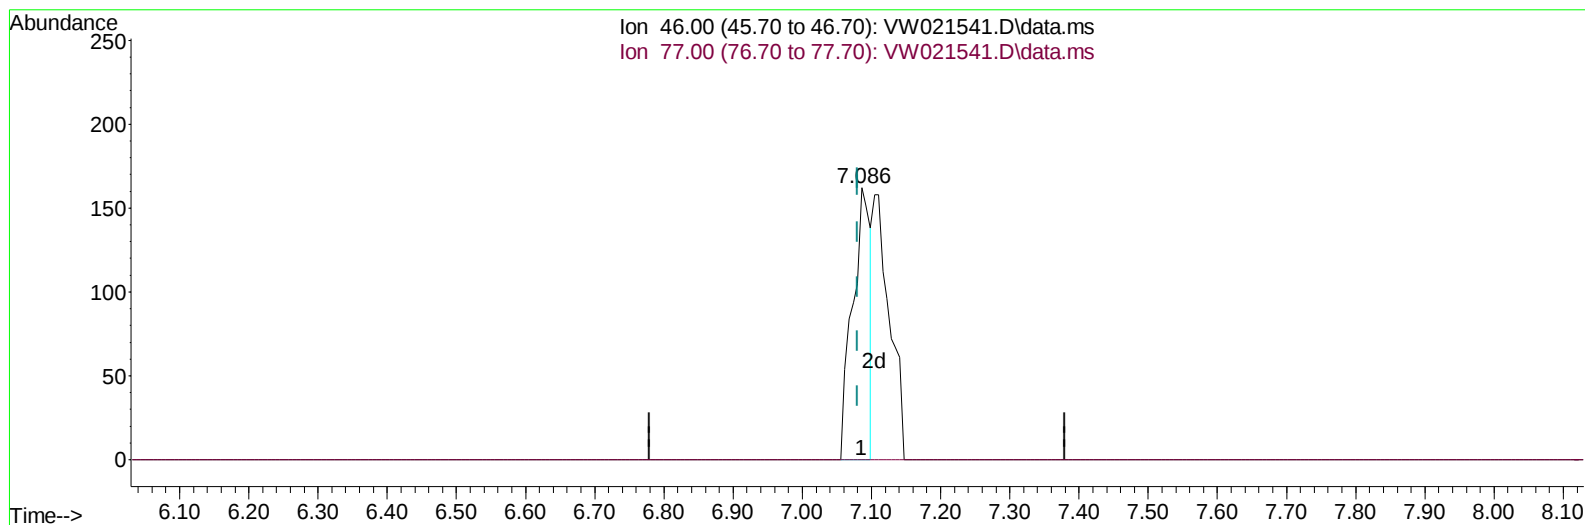

TIC: VW021541.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 28.27 ug/L

response 289

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122121\
 Data File : VW021541.D
 Acq On : 21 Dec 2021 22:41
 Operator : SY/VA
 Sample : M5194-07
 Misc : 7.08g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLB9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/22/2021
 Supervised By :Amit Patel 12/24/2021

Quant Time: Dec 22 03:52:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 22 02:57:00 2021
 Response via : Initial Calibration

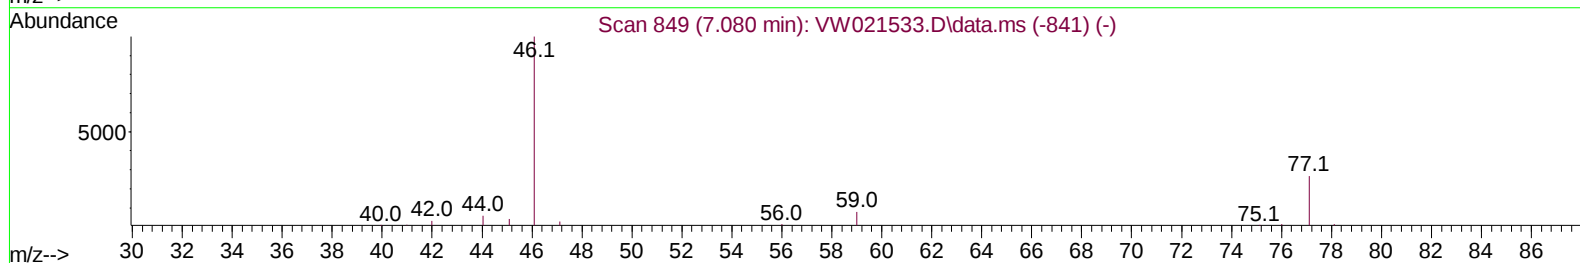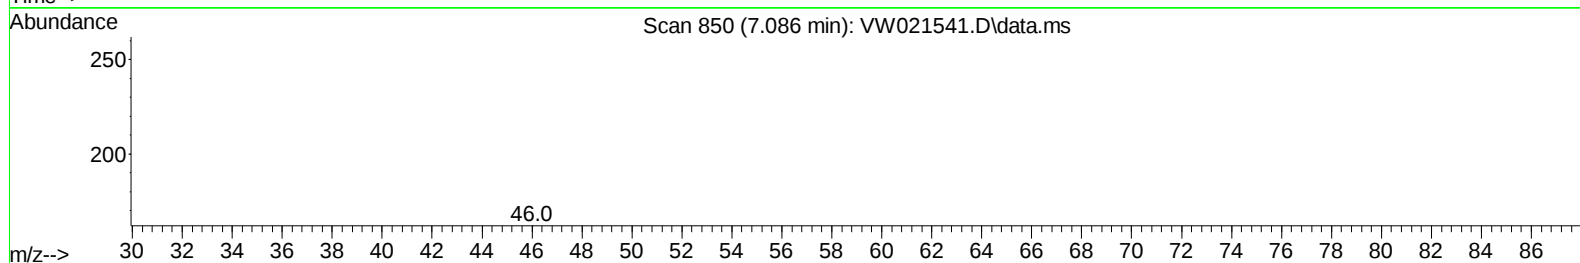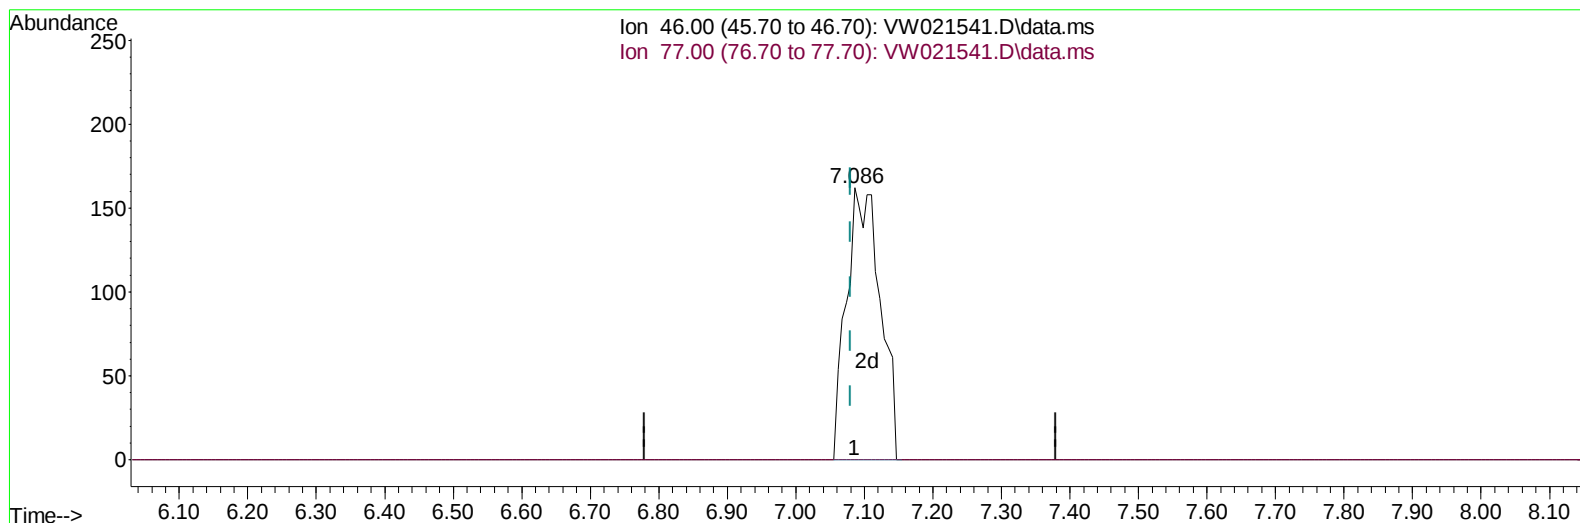

TIC: VW021541.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 54.09 ug/L m

response 553

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122121\
 Data File : VW021541.D
 Acq On : 21 Dec 2021 22:41
 Operator : SY/VA
 Sample : M5194-07
 Misc : 7.08g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLB9

Manual IntegrationsAPPROVED

Quant Time: Dec 22 03:52:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 22 02:57:00 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/22/2021
 Supervised By :Amit Patel 12/24/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	3982	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	4090	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	2379	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	1020	14.065	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	56.240%	
7) Chloroethane-d5	2.898	69	810	16.895	ug/L	0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.600%	
11) 1,1-Dichloroethene-d2	4.032	63	1383	14.304	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	57.200%	
21) 2-Butanone-d5	7.086	46	553m	54.095	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.180%	
24) Chloroform-d	7.659	84	2469	22.249	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	89.000%	
26) 1,2-Dichloroethane-d4	8.305	65	1711	28.986	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	115.960%	
32) Benzene-d6	8.281	84	4671	20.835	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	83.360%	
36) 1,2-Dichloropropane-d6	9.281	67	1364	22.686	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	90.760%	
41) Toluene-d8	10.323	98	4334	18.921	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.680%	
43) trans-1,3-Dichloroprop...	10.579	79	545	19.686	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	78.760%	
47) 2-Hexanone-d5	0.000	63	0	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135	Recovery	=	0.000%#	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	1301	25.172	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	100.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	1829	19.837	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	79.360%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122121\
Data File : VW021541.D
Acq On : 21 Dec 2021 22:41
Operator : SY/VA
Sample : M5194-07
Misc : 7.08g/10.0mL/MSVOA_W/SOIL
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLB9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/22/2021
Supervised By :Amit Patel 12/24/2021

Quant Time: Dec 22 03:52:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 22 02:57:00 2021
Response via : Initial Calibration

