

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122121\
 Data File : VW021516.D
 Acq On : 21 Dec 2021 10:57
 Operator : SY/VA
 Sample : M5101-21
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Dec 22 01:18:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 22 01:15:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	132954	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	125569	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	71296	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	43376	17.913	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.640%
7) Chloroethane-d5	2.885	69	32721	20.441	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.760%
11) 1,1-Dichloroethene-d2	4.013	63	61171	18.949	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.800%
21) 2-Butanone-d5	7.074	46	20542	60.183	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.360%
24) Chloroform-d	7.647	84	91014	24.564	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.240%
26) 1,2-Dichloroethane-d4	8.305	65	51410	26.085	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.320%
32) Benzene-d6	8.275	84	174513	25.355	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.400%
36) 1,2-Dichloropropane-d6	9.275	67	48753	26.411	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.640%
41) Toluene-d8	10.323	98	175357	24.935	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.760%
43) trans-1,3-Dichloroprop...	10.579	79	20726	24.385	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.560%
47) 2-Hexanone-d5	10.921	63	15595	57.133	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.260%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	39227	24.721	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	64721	23.423	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.680%
Target Compounds					Qvalue	
13) Acetone	4.117	43	1405	4.592	ug/L	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122121\
Data File : VW021516.D
Acq On : 21 Dec 2021 10:57
Operator : SY/VA
Sample : M5101-21
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Dec 22 01:18:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 22 01:15:19 2021
Response via : Initial Calibration

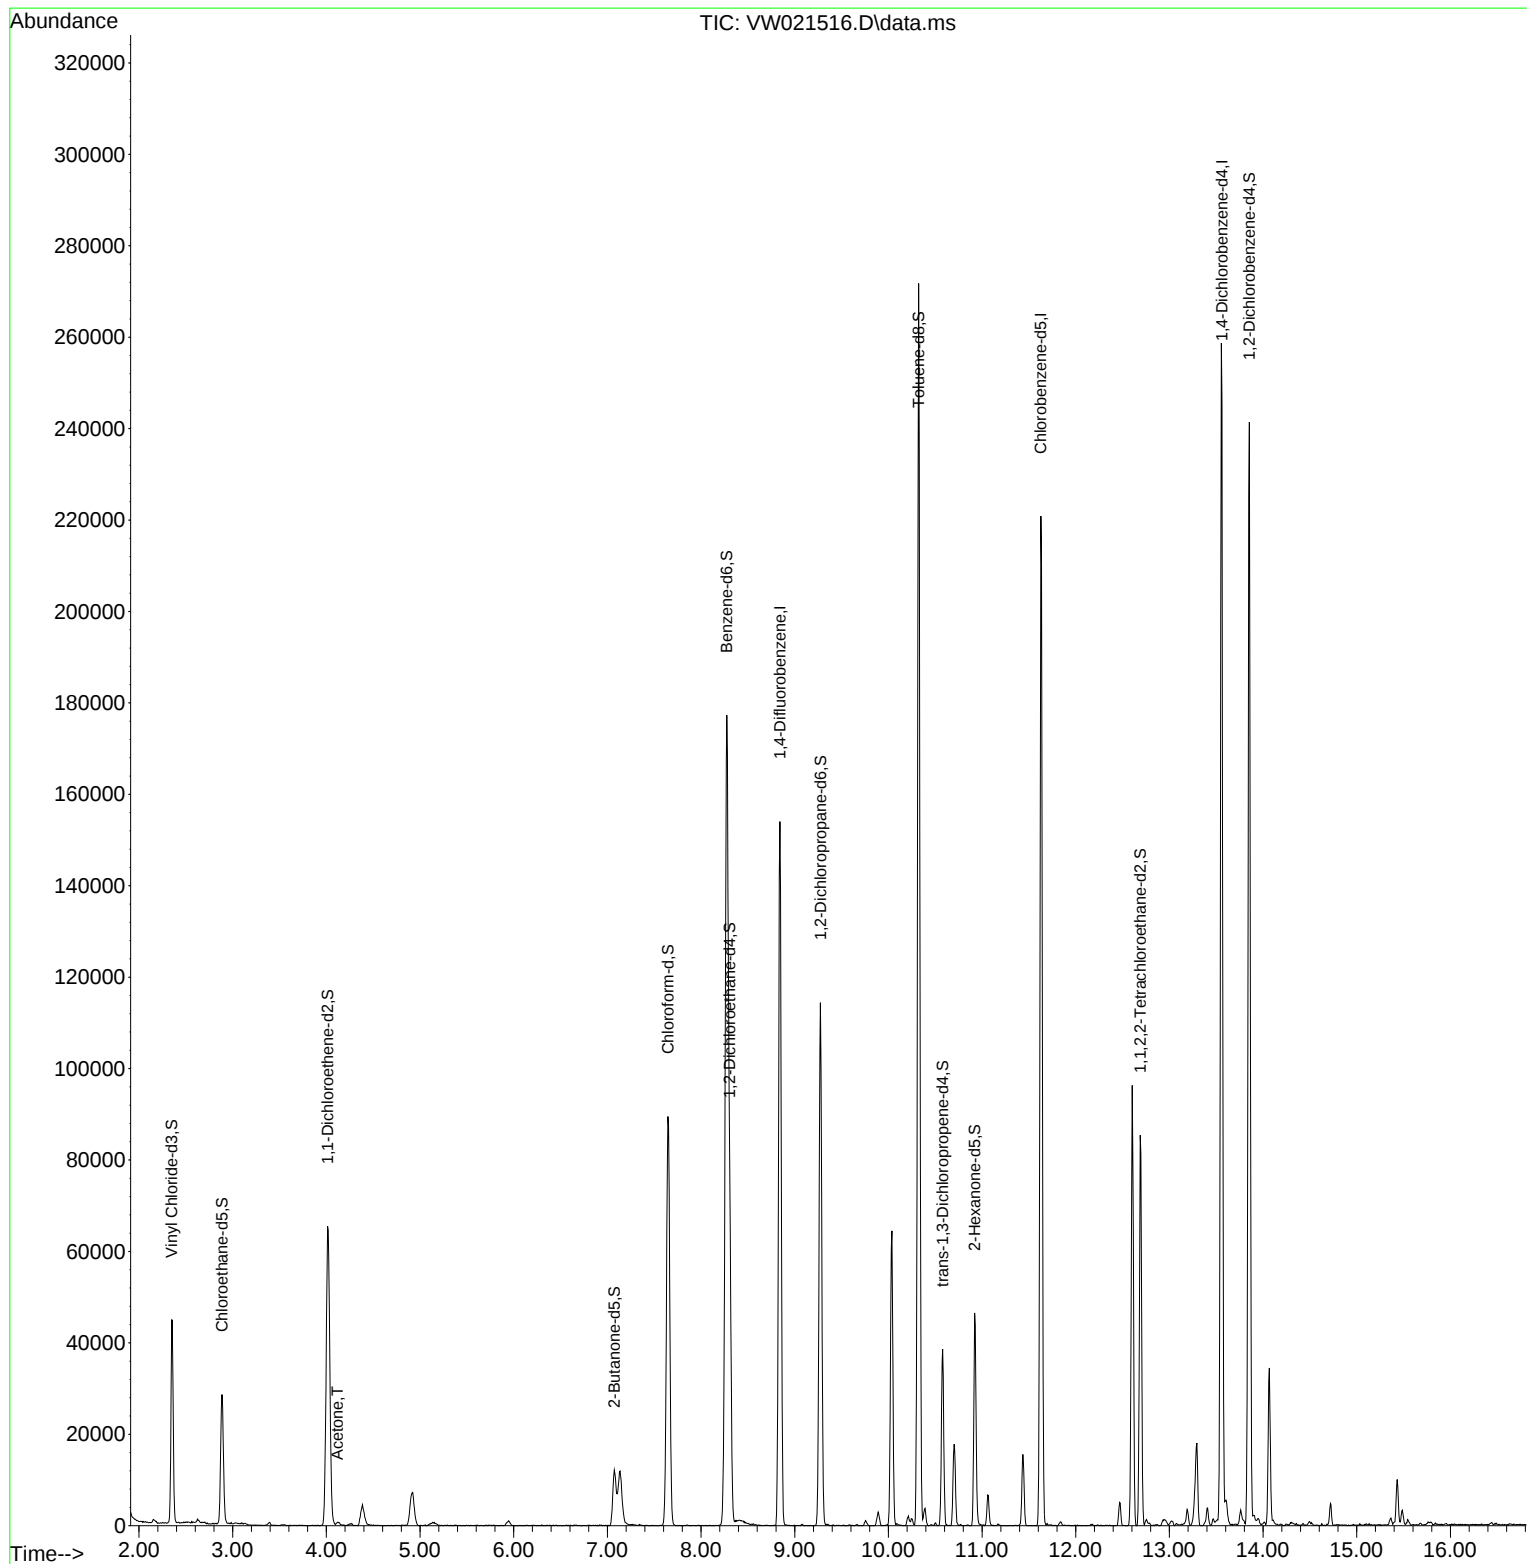

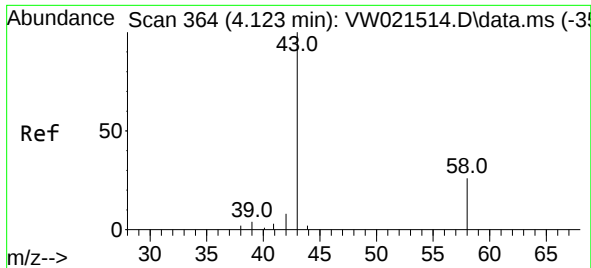

#13
 Acetone
 Concen: 4.592 ug/L
 RT: 4.117 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW021516.D
 Acq: 21 Dec 2021 10:57

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 43 Resp: 1405
 Ion Ratio Lower Upper
 43 100
 58 12.0 0.0 52.8

