

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122121\
 Data File : VW021537.D
 Acq On : 21 Dec 2021 21:05
 Operator : SY/VA
 Sample : M5194-03
 Misc : 5.30g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLB5

Quant Time: Dec 22 03:51:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 22 02:57:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	118350	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.627	117	125006	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	77074	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	32610	15.129	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.520%
7) Chloroethane-d5	2.885	69	21176	14.861	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.440%
11) 1,1-Dichloroethene-d2	4.019	63	48671	16.937	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.760%
21) 2-Butanone-d5	7.079	46	15420	50.751	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.500%
24) Chloroform-d	7.652	84	74424	22.565	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.280%
26) 1,2-Dichloroethane-d4	8.305	65	41930	23.900	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.600%
32) Benzene-d6	8.274	84	141801	20.695	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.760%
36) 1,2-Dichloropropane-d6	9.274	67	40799	22.202	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.800%
41) Toluene-d8	10.323	98	146472	20.922	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.680%
43) trans-1,3-Dichloroprop...	10.579	79	17668	20.881	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.520%
47) 2-Hexanone-d5	10.926	63	13489	49.640	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.280%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	34243	21.677	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.720%
66) 1,2-Dichlorobenzene-d4	13.853	152	61321	20.529	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.120%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	12511	6.398	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122121\
Data File : VW021537.D
Acq On : 21 Dec 2021 21:05
Operator : SY/VA
Sample : M5194-03
Misc : 5.30g/10.0mL/MSVOA_W/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLB5

Quant Time: Dec 22 03:51:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 22 02:57:00 2021
Response via : Initial Calibration

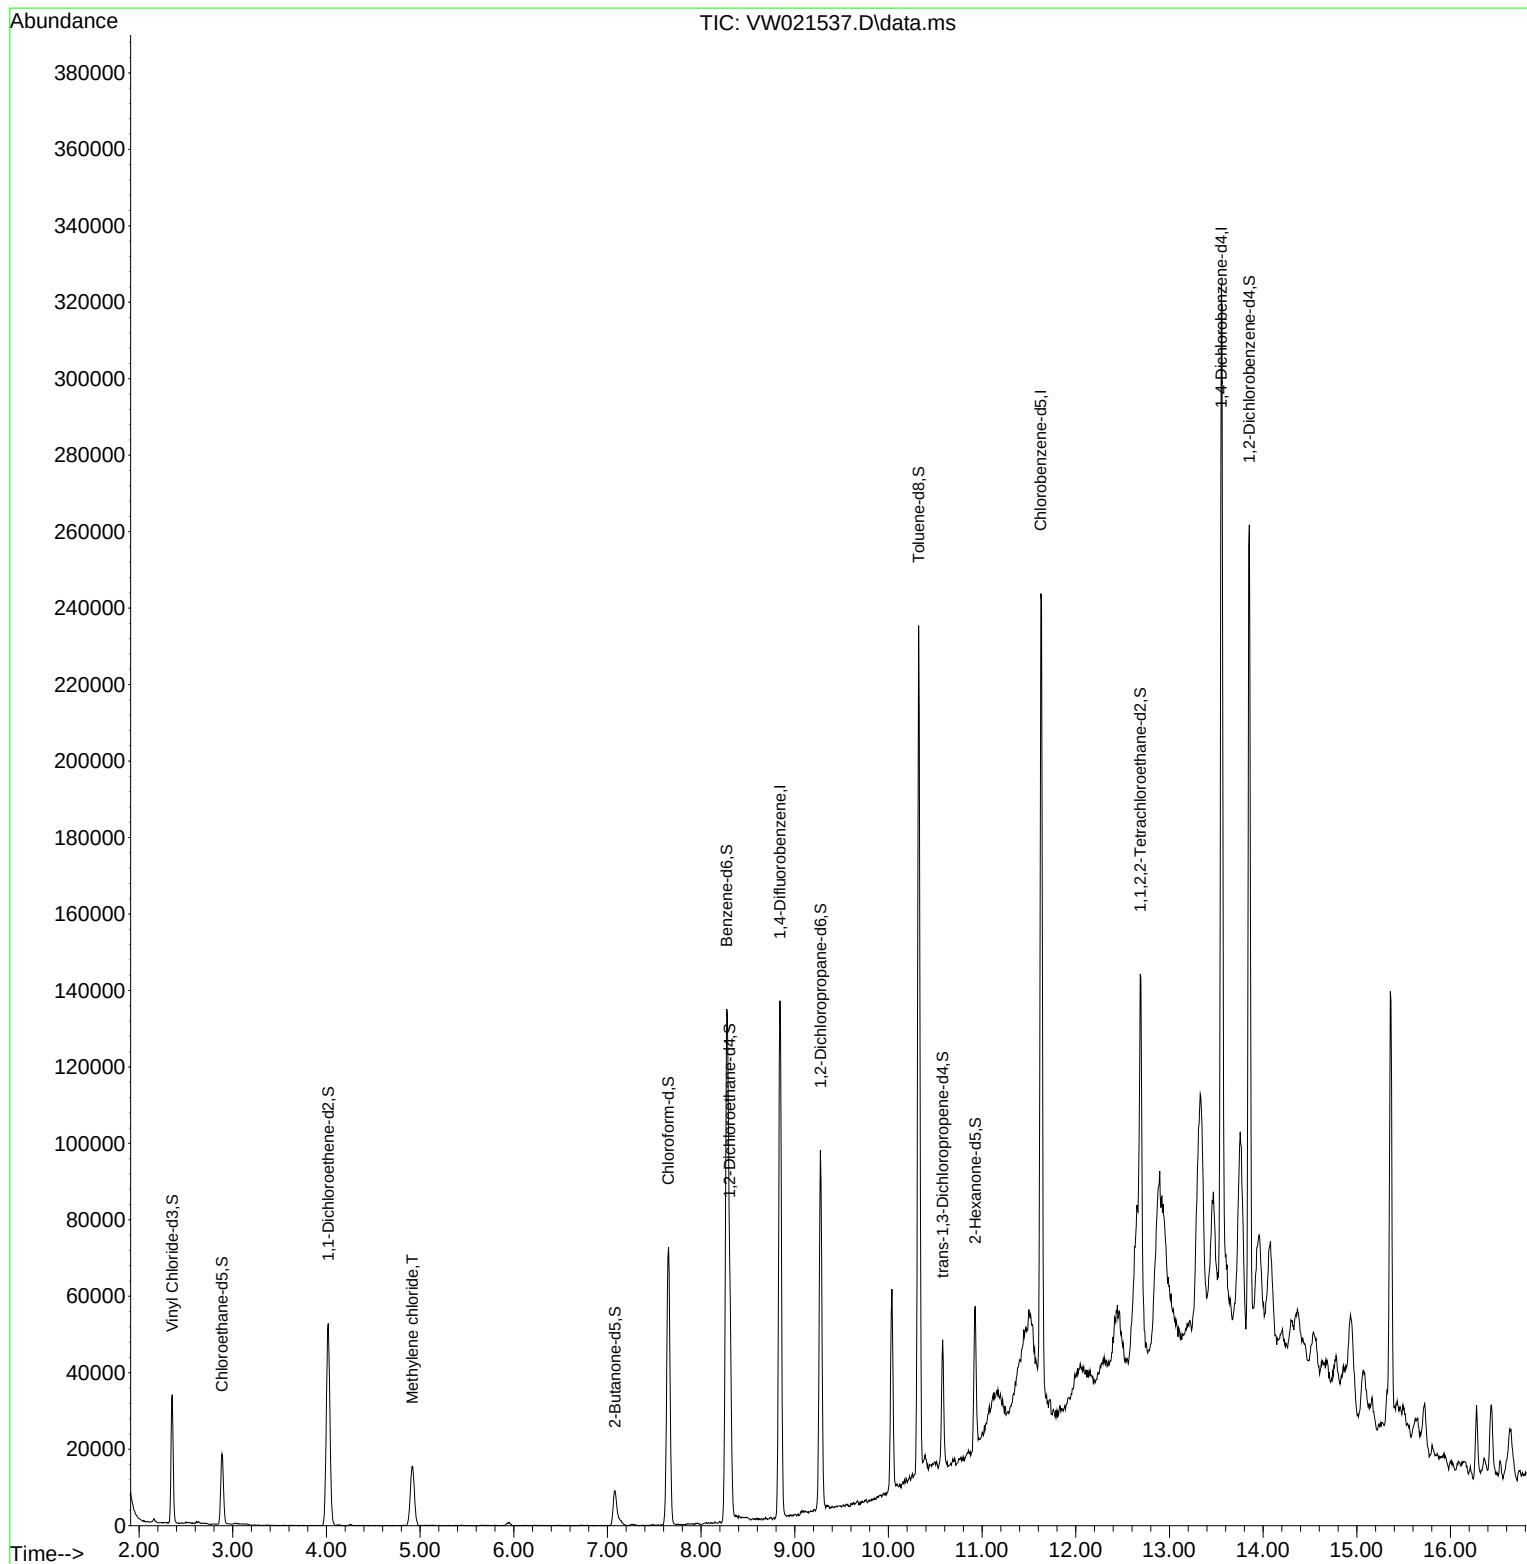

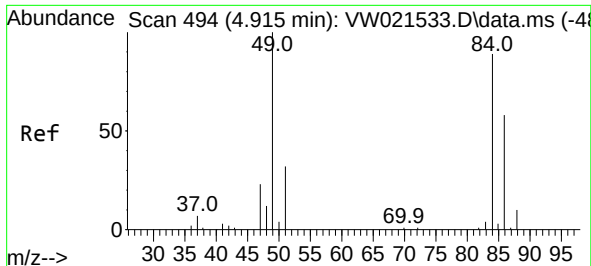

#16
Methylene chloride
Concen: 6.398 ug/L
RT: 4.915 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW021537.D
Acq: 21 Dec 2021 21:05

Instrument :
MSVOA_W
ClientSampleId :
BGLB5

Tgt Ion: 84 Resp: 12511
Ion Ratio Lower Upper
84 100
86 64.4 45.5 84.5
49 110.7 100.5 186.7

